

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028792.D
 Acq On : 31 Oct 2022 19:55
 Operator : SY/MD
 Sample : N5321-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVV0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	102	rBV2	585966	678696	22.57%	4.119%
2	1.564	158	163	177	rVB	213326	242447	8.06%	1.471%
3	2.105	323	331	345	rVB	364473	524205	17.43%	3.181%
4	2.452	436	439	441	rBV4	2493	1346	0.04%	0.008%
5	2.757	524	534	554	rBV	137542	243518	8.10%	1.478%
6	2.886	572	574	576	rBV3	1186	665	0.02%	0.004%
7	2.966	598	599	605	rVB7	2601	1977	0.07%	0.012%
8	3.021	613	616	617	rBV3	1502	716	0.02%	0.004%
9	3.066	628	630	632	rVB3	1660	787	0.03%	0.005%
10	3.188	664	668	670	rBV5	1021	854	0.03%	0.005%
11	3.233	679	682	683	rBV3	2221	1113	0.04%	0.007%
12	3.278	694	696	698	rBV3	1458	810	0.03%	0.005%
13	3.291	698	700	705	rVV4	1746	1080	0.04%	0.007%
14	3.326	709	711	714	rVB4	1163	760	0.03%	0.005%
15	3.368	719	724	727	rBV6	1952	1609	0.05%	0.010%
16	3.465	750	754	756	rBV5	1376	1061	0.04%	0.006%
17	3.526	766	773	774	rBV6	986	1073	0.04%	0.007%
18	3.597	791	795	797	rBV5	1695	1266	0.04%	0.008%
19	3.619	800	802	804	rBV3	1366	700	0.02%	0.004%
20	3.654	811	813	818	rVB5	1797	1644	0.05%	0.010%
21	3.699	824	827	830	rBV3	1739	1081	0.04%	0.007%
22	3.761	844	846	849	rVB3	1849	757	0.03%	0.005%
23	3.786	853	854	858	rVB4	1667	1010	0.03%	0.006%
24	3.809	858	861	864	rBV4	1240	1068	0.04%	0.006%
25	3.902	872	890	917	rBV2	1148058	3007698	100.00%	18.251%
26	4.342	1014	1027	1052	rBV	235295	575870	19.15%	3.495%
27	4.822	1173	1176	1178	rBV3	1163	664	0.02%	0.004%
28	4.896	1196	1199	1204	rBV6	1658	1611	0.05%	0.010%
29	5.040	1226	1244	1270	rBV2	591805	1553934	51.67%	9.430%
30	5.310	1324	1328	1335	rBV9	1653	1650	0.05%	0.010%
31	5.613	1411	1422	1445	rBV	512760	1027207	34.15%	6.233%
32	5.908	1504	1514	1545	rVB	350851	697479	23.19%	4.232%
33	6.066	1551	1563	1590	rVB	358769	728608	24.22%	4.421%
34	6.371	1656	1658	1660	rBV3	1728	785	0.03%	0.005%
35	6.455	1682	1684	1686	rVB3	1663	611	0.02%	0.004%
36	6.481	1690	1692	1698	rVV7	1573	876	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028792.D
 Acq On : 31 Oct 2022 19:55
 Operator : SY/MD
 Sample : N5321-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWV0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	6.577	1720	1722	1724	rBV3	1677	899	0.03%	0.005%
38	6.625	1733	1737	1739	rBV5	1288	1148	0.04%	0.007%
39	6.870	1809	1813	1815	rBV5	1380	789	0.03%	0.005%
40	6.982	1837	1848	1865	rBV	163843	306646	10.20%	1.861%
41	7.310	1939	1950	1971	rBV	654564	1154592	38.39%	7.006%
42	7.619	2036	2046	2066	rBV	104907	197082	6.55%	1.196%
43	7.921	2137	2140	2141	rBV3	1419	788	0.03%	0.005%
44	7.969	2145	2155	2174	rVB	345917	583652	19.41%	3.542%
45	8.085	2182	2191	2222	rBV	424840	841505	27.98%	5.106%
46	8.593	2346	2349	2353	rBV5	2064	1885	0.06%	0.011%
47	8.638	2359	2363	2367	rBV7	1098	1111	0.04%	0.007%
48	8.696	2378	2381	2382	rBV3	1313	798	0.03%	0.005%
49	8.735	2391	2393	2395	rBV3	1342	831	0.03%	0.005%
50	8.847	2417	2428	2453	rBV	751392	1228605	40.85%	7.455%
51	9.259	2552	2556	2557	rBV4	1358	987	0.03%	0.006%
52	9.403	2598	2601	2604	rVB5	1285	833	0.03%	0.005%
53	9.423	2604	2607	2609	rBV4	1781	1043	0.03%	0.006%
54	9.542	2638	2644	2649	rBV8	2477	3008	0.10%	0.018%
55	9.747	2706	2708	2714	rVB6	1183	925	0.03%	0.006%
56	9.776	2714	2717	2718	rBV3	1665	816	0.03%	0.005%
57	9.866	2742	2745	2749	rBV6	2083	1372	0.05%	0.008%
58	9.934	2763	2766	2768	rBV3	1566	1049	0.03%	0.006%
59	9.982	2779	2781	2784	rVB4	1950	882	0.03%	0.005%
60	10.005	2784	2788	2792	rBV6	2247	2004	0.07%	0.012%
61	10.101	2816	2818	2825	rVB7	1915	1586	0.05%	0.010%
62	10.130	2825	2827	2831	rVB5	1973	1284	0.04%	0.008%
63	10.159	2831	2836	2839	rBV6	1782	1862	0.06%	0.011%
64	10.207	2839	2851	2869	rBV	464137	733033	24.37%	4.448%
65	10.442	2922	2924	2927	rBV4	1686	648	0.02%	0.004%
66	10.612	2974	2977	2982	rBV6	2034	1589	0.05%	0.010%
67	10.702	3002	3005	3009	rVB5	2556	2018	0.07%	0.012%
68	10.725	3009	3012	3014	rBV3	2440	1460	0.05%	0.009%
69	10.882	3057	3061	3064	rVB6	1636	1327	0.04%	0.008%
70	10.911	3066	3070	3072	rBV5	2211	1431	0.05%	0.009%
71	10.963	3083	3086	3087	rBV2	1263	667	0.02%	0.004%
72	11.024	3102	3105	3108	rBV4	1437	1147	0.04%	0.007%
73	11.175	3148	3152	3154	rBV5	2056	1572	0.05%	0.010%
74	11.239	3162	3172	3199	rBV	683684	1089709	36.23%	6.613%
75	11.432	3230	3232	3234	rBV3	1793	847	0.03%	0.005%
76	11.503	3252	3254	3256	rBV3	1591	723	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028792.D
 Acq On : 31 Oct 2022 19:55
 Operator : SY/MD
 Sample : N5321-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVV0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	11.616	3278	3289	3307	rBV	605742	967558	32.17%	5.871%
78	11.754	3330	3332	3334	rBV3	1675	1161	0.04%	0.007%
79	11.879	3368	3371	3376	rBV7	1403	1552	0.05%	0.009%
80	11.915	3380	3382	3385	rBV4	1441	931	0.03%	0.006%
81	12.014	3410	3413	3415	rBV4	1577	1100	0.04%	0.007%
82	12.188	3465	3467	3472	rBV5	1674	1024	0.03%	0.006%
83	12.339	3510	3514	3517	rBV6	2046	1537	0.05%	0.009%
84	12.580	3588	3589	3594	rBV5	1978	1464	0.05%	0.009%
85	12.628	3601	3604	3605	rBV3	1336	685	0.02%	0.004%
86	12.686	3618	3622	3628	rVB7	1969	1886	0.06%	0.011%
87	12.751	3639	3642	3646	rBV6	1543	1285	0.04%	0.008%
88	13.194	3777	3780	3783	rBV5	1353	1025	0.03%	0.006%
89	13.281	3805	3807	3811	rBV5	1708	1486	0.05%	0.009%
90	13.750	3949	3953	3956	rBV5	2041	1956	0.07%	0.012%
91	14.133	4066	4072	4074	rBV6	1857	1429	0.05%	0.009%
92	14.149	4074	4077	4078	rBV2	1398	707	0.02%	0.004%
93	14.191	4087	4090	4093	rBV4	2081	1713	0.06%	0.010%
94	14.397	4149	4154	4156	rBV5	1672	1879	0.06%	0.011%
95	14.426	4160	4163	4167	rVV6	1433	1327	0.04%	0.008%
96	14.464	4173	4175	4177	rBV3	1595	982	0.03%	0.006%
97	14.513	4186	4190	4193	rBV6	1903	1763	0.06%	0.011%
98	14.564	4203	4206	4210	rVB6	1685	1048	0.03%	0.006%
99	15.066	4361	4362	4365	rBV2	1314	881	0.03%	0.005%
100	15.207	4402	4406	4409	rBV5	1589	1434	0.05%	0.009%




Sum of corrected areas: 16479202

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028792.D
Acq On : 31 Oct 2022 19:55
Operator : SY/MD
Sample : N5321-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWV0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

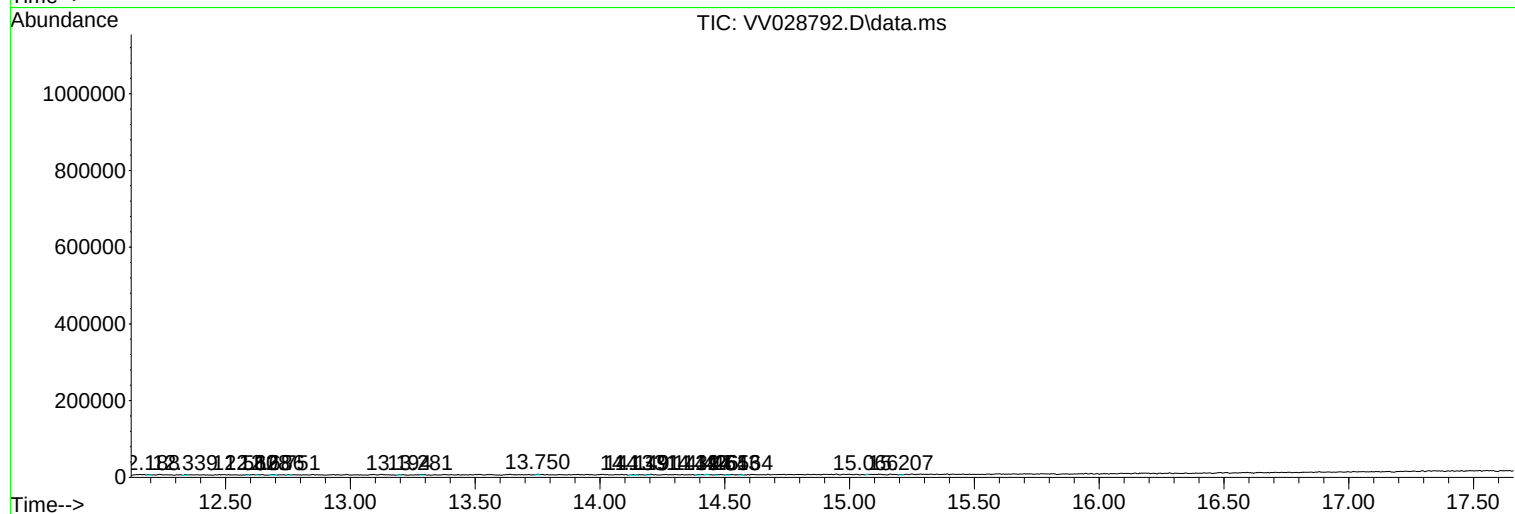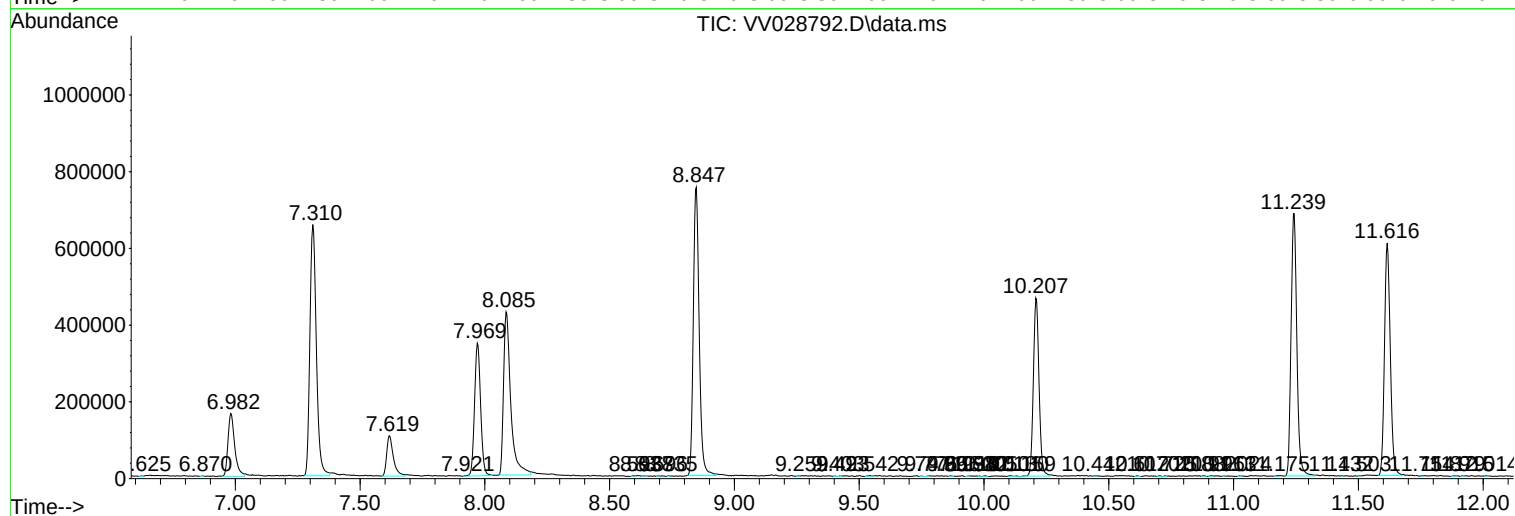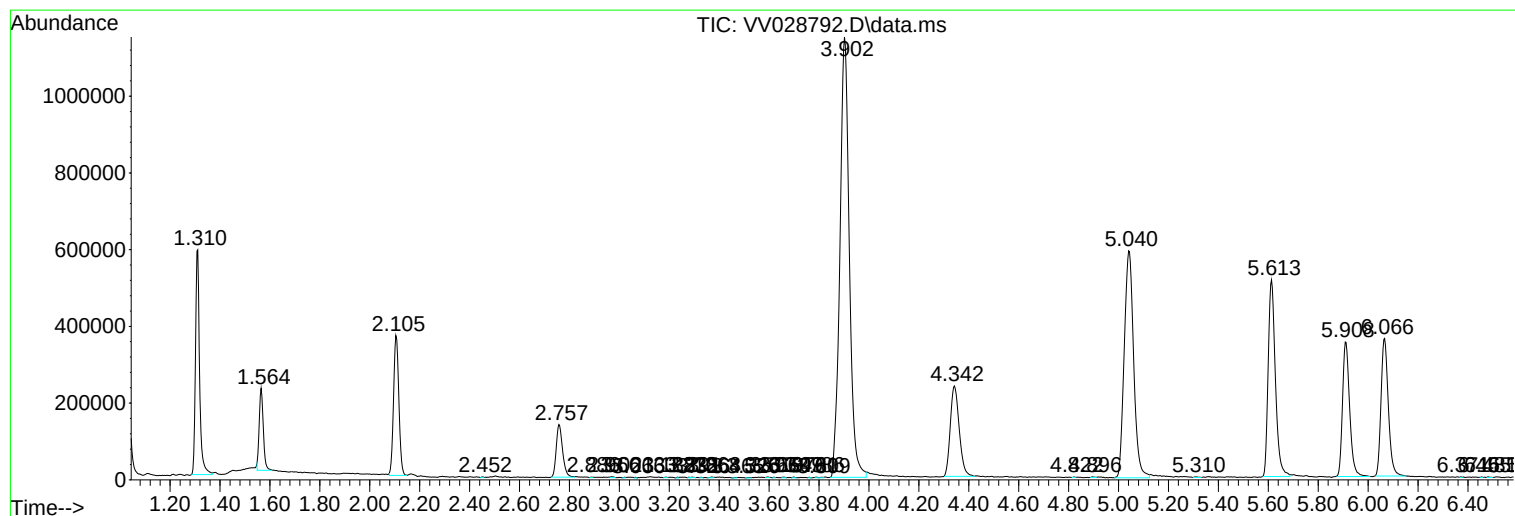

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028792.D
Acq On : 31 Oct 2022 19:55
Operator : SY/MD
Sample : N5321-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVV0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028792.D
Acq On : 31 Oct 2022 19:55
Operator : SY/MD
Sample : N5321-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWV0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc