

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028793.D
 Acq On : 31 Oct 2022 20:19
 Operator : SY/MD
 Sample : N5321-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028793.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	102	rBV2	540872	638423	4.33%	1.368%
2	1.564	157	163	177	rVB	213277	250812	1.70%	0.537%
3	2.108	323	332	345	rVB2	413470	634796	4.31%	1.360%
4	2.474	442	446	449	rBV5	1512	1472	0.01%	0.003%
5	2.754	517	533	566	rBV	1870154	3211521	21.80%	6.879%
6	3.089	635	637	640	rBV3	1282	742	0.01%	0.002%
7	3.188	661	668	669	rBV7	1670	2023	0.01%	0.004%
8	3.236	681	683	689	rBV7	1184	963	0.01%	0.002%
9	3.272	689	694	699	rBV8	1682	1939	0.01%	0.004%
10	3.310	699	706	708	rVV6	1652	1724	0.01%	0.004%
11	3.352	712	719	720	rBV6	1231	924	0.01%	0.002%
12	3.391	729	731	734	rBV4	1344	899	0.01%	0.002%
13	3.510	765	768	771	rBV4	1650	938	0.01%	0.002%
14	3.529	772	774	778	rVB5	1197	788	0.01%	0.002%
15	3.552	778	781	786	rBV7	1489	1433	0.01%	0.003%
16	3.619	796	802	806	rBV9	2112	2329	0.02%	0.005%
17	3.642	806	809	813	rVV5	1557	1170	0.01%	0.003%
18	3.690	821	824	826	rBV3	1093	736	0.00%	0.002%
19	3.744	836	841	842	rBV4	1212	1063	0.01%	0.002%
20	3.828	864	867	870	rVB4	1830	1137	0.01%	0.002%
21	3.902	870	890	938	rBV	3858372	9454572	64.17%	20.252%
22	4.343	1012	1027	1051	rBV	241578	603993	4.10%	1.294%
23	4.806	1168	1171	1173	rBV4	1918	1426	0.01%	0.003%
24	4.851	1182	1185	1188	rBV5	1808	1269	0.01%	0.003%
25	4.966	1217	1221	1224	rVB7	1957	1398	0.01%	0.003%
26	4.986	1224	1227	1228	rBV2	2348	1402	0.01%	0.003%
27	5.040	1228	1244	1275	rVV2	599200	1595489	10.83%	3.418%
28	5.288	1319	1321	1324	rBV4	2355	1423	0.01%	0.003%
29	5.516	1390	1392	1394	rBV2	1554	691	0.00%	0.001%
30	5.613	1411	1422	1452	rBV	515748	1036768	7.04%	2.221%
31	5.908	1499	1514	1549	rBV	7883589	14733614	100.00%	31.560%
32	6.066	1553	1563	1590	rVB	368694	760711	5.16%	1.629%
33	6.561	1714	1717	1718	rBV3	2172	1234	0.01%	0.003%
34	6.619	1733	1735	1736	rBV2	1773	873	0.01%	0.002%
35	6.921	1826	1829	1832	rBV4	1037	831	0.01%	0.002%
36	6.982	1838	1848	1872	rBV	174186	319704	2.17%	0.685%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028793.D
 Acq On : 31 Oct 2022 20:19
 Operator : SY/MD
 Sample : N5321-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	7.178	1903	1909	1910	rBV6	1963	2039	0.01%	0.004%
38	7.310	1938	1950	1969	rBV	692643	1194946	8.11%	2.560%
39	7.619	2037	2046	2062	rBV	110949	193718	1.31%	0.415%
40	7.969	2141	2155	2182	rBV	4295925	7006559	47.55%	15.008%
41	8.085	2182	2191	2224	rVV	424806	826523	5.61%	1.770%
42	8.497	2317	2319	2323	rVB5	1566	893	0.01%	0.002%
43	8.542	2330	2333	2337	rVB6	1420	1103	0.01%	0.002%
44	8.715	2379	2387	2399	rVV	15578	27539	0.19%	0.059%
45	8.847	2415	2428	2450	rBV	757133	1250231	8.49%	2.678%
46	9.246	2549	2552	2556	rBV5	1926	1236	0.01%	0.003%
47	9.468	2617	2621	2624	rVB5	2198	1942	0.01%	0.004%
48	9.493	2624	2629	2632	rBV6	1794	1525	0.01%	0.003%
49	9.625	2666	2670	2674	rVB6	1653	1340	0.01%	0.003%
50	9.651	2674	2678	2682	rBV7	1768	1509	0.01%	0.003%
51	9.731	2698	2703	2706	rBV6	2176	1639	0.01%	0.004%
52	9.860	2739	2743	2745	rBV5	1415	1143	0.01%	0.002%
53	9.892	2750	2753	2755	rBV5	1444	961	0.01%	0.002%
54	9.928	2759	2764	2766	rBV6	1253	1079	0.01%	0.002%
55	9.944	2766	2769	2773	rVB5	1553	1132	0.01%	0.002%
56	9.973	2775	2778	2780	rBV3	1255	913	0.01%	0.002%
57	10.005	2784	2788	2789	rBV3	1289	847	0.01%	0.002%
58	10.207	2836	2851	2869	rBV	469831	748890	5.08%	1.604%
59	10.448	2924	2926	2929	rBV4	1821	897	0.01%	0.002%
60	10.571	2962	2964	2966	rBV4	1295	828	0.01%	0.002%
61	10.600	2971	2973	2977	rBV5	1829	1365	0.01%	0.003%
62	10.673	2994	2996	2999	rBV4	1372	977	0.01%	0.002%
63	10.693	2999	3002	3005	rVV4	1391	962	0.01%	0.002%
64	10.770	3020	3026	3028	rBV7	2253	2350	0.02%	0.005%
65	10.815	3036	3040	3041	rBV4	1822	1172	0.01%	0.003%
66	10.908	3064	3069	3070	rBV4	1600	1345	0.01%	0.003%
67	10.956	3081	3084	3090	rVB8	2657	1963	0.01%	0.004%
68	11.063	3113	3117	3120	rBV5	1272	1137	0.01%	0.002%
69	11.108	3127	3131	3134	rBV6	1636	1483	0.01%	0.003%
70	11.178	3150	3153	3157	rBV6	2109	1914	0.01%	0.004%
71	11.239	3161	3172	3193	rBV	695421	1097511	7.45%	2.351%
72	11.458	3239	3240	3243	rBV3	1042	638	0.00%	0.001%
73	11.493	3248	3251	3252	rBV2	1175	777	0.01%	0.002%
74	11.616	3278	3289	3312	rBV	621881	1003934	6.81%	2.150%
75	12.146	3450	3454	3455	rBV4	1312	757	0.01%	0.002%
76	12.223	3473	3478	3481	rBV5	1902	1676	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028793.D
 Acq On : 31 Oct 2022 20:19
 Operator : SY/MD
 Sample : N5321-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWW1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.464	3549	3553	3555	rBV5	1068	925	0.01%	0.002%
78	12.564	3581	3584	3585	rBV3	1368	600	0.00%	0.001%
79	12.644	3606	3609	3611	rBV4	1308	909	0.01%	0.002%
80	12.773	3647	3649	3652	rVB4	1916	1004	0.01%	0.002%
81	12.815	3660	3662	3665	rBV4	1787	1056	0.01%	0.002%
82	12.866	3676	3678	3680	rBV2	1190	711	0.00%	0.002%
83	12.943	3700	3702	3707	rBV6	1299	1046	0.01%	0.002%
84	12.969	3707	3710	3712	rBV4	1138	623	0.00%	0.001%
85	13.043	3728	3733	3734	rBV4	1272	1073	0.01%	0.002%
86	13.072	3740	3742	3746	rBV4	795	710	0.00%	0.002%
87	13.242	3791	3795	3796	rBV4	1463	929	0.01%	0.002%
88	13.532	3882	3885	3889	rBV4	1692	1411	0.01%	0.003%
89	13.812	3969	3972	3975	rBV4	1339	668	0.00%	0.001%
90	13.831	3975	3978	3979	rBV2	1382	791	0.01%	0.002%
91	14.046	4043	4045	4049	rVB5	1651	915	0.01%	0.002%
92	14.066	4049	4051	4052	rBV2	1257	644	0.00%	0.001%
93	14.175	4084	4085	4088	rVB3	1928	752	0.01%	0.002%
94	14.194	4088	4091	4093	rBV4	1863	982	0.01%	0.002%
95	14.332	4131	4134	4137	rBV5	1818	1271	0.01%	0.003%
96	14.410	4154	4158	4161	rBV6	1071	1012	0.01%	0.002%
97	14.500	4181	4186	4188	rBV6	2290	2183	0.01%	0.005%
98	14.651	4230	4233	4235	rBV4	1233	707	0.00%	0.002%
99	14.731	4255	4258	4262	rBV6	1717	1748	0.01%	0.004%
100	15.197	4402	4403	4406	rBV3	1493	864	0.01%	0.002%




Sum of corrected areas: 46684157

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028793.D
Acq On : 31 Oct 2022 20:19
Operator : SY/MD
Sample : N5321-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

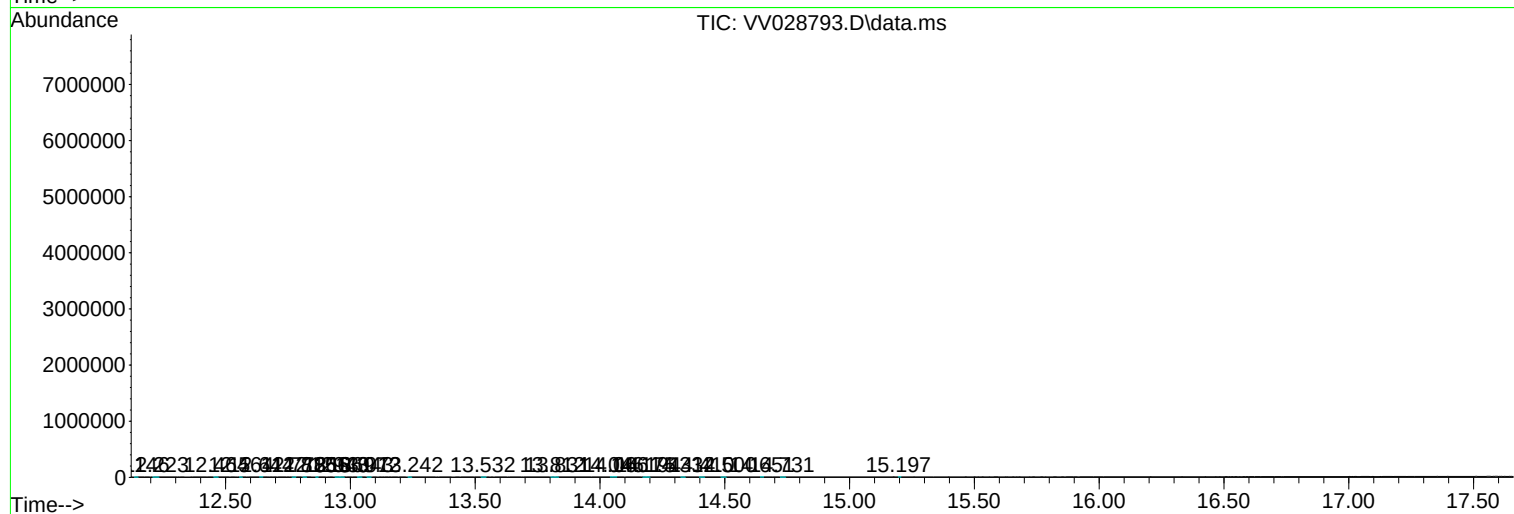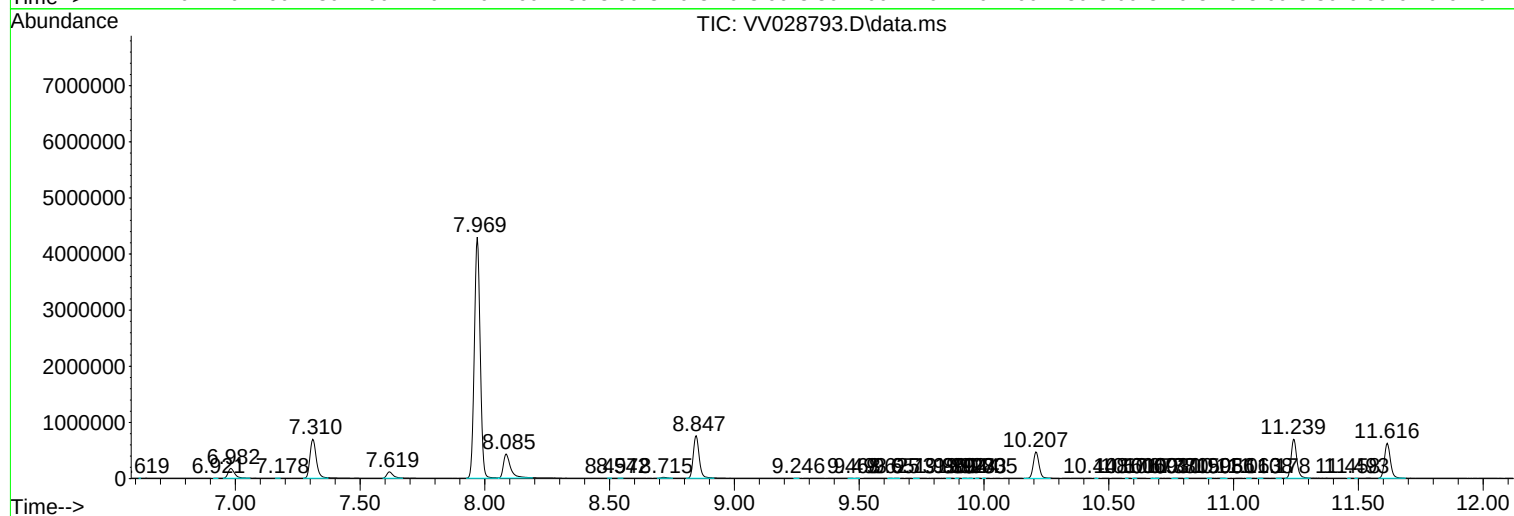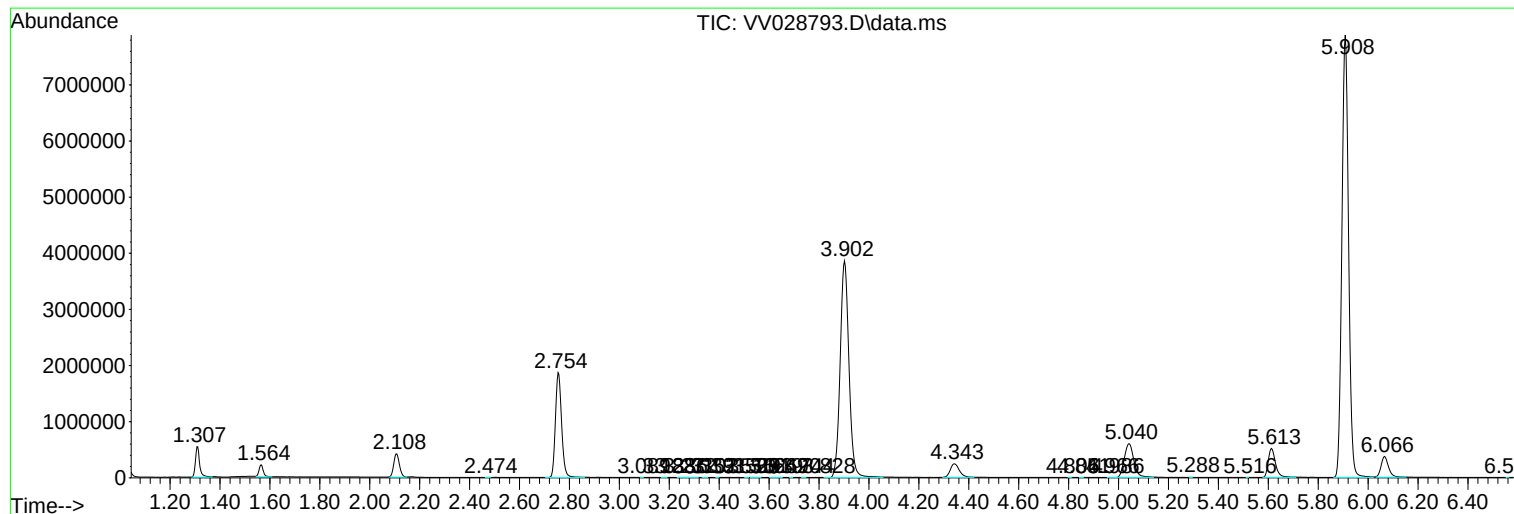

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028793.D
Acq On : 31 Oct 2022 20:19
Operator : SY/MD
Sample : N5321-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028793.D
Acq On : 31 Oct 2022 20:19
Operator : SY/MD
Sample : N5321-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc