

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028798.D
 Acq On : 31 Oct 2022 22:20
 Operator : SY/MD
 Sample : N5321-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028798.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB2	199009	225470	11.76%	1.517%
2	1.561	157	162	178	rVB	189588	224615	11.71%	1.511%
3	2.105	322	331	345	rVB	368450	533575	27.82%	3.590%
4	2.449	435	438	440	rBV4	2204	1303	0.07%	0.009%
5	2.757	524	534	551	rBV	153514	268132	13.98%	1.804%
6	3.082	634	635	638	rBV3	1337	633	0.03%	0.004%
7	3.172	661	663	665	rBV3	1618	829	0.04%	0.006%
8	3.198	668	671	676	rVV7	1689	1215	0.06%	0.008%
9	3.259	688	690	694	rVB4	2000	1410	0.07%	0.009%
10	3.285	694	698	701	rBV5	1616	1431	0.07%	0.010%
11	3.314	704	707	710	rBV4	1375	940	0.05%	0.006%
12	3.384	725	729	730	rBV3	964	678	0.04%	0.005%
13	3.429	739	743	746	rBV6	1643	1575	0.08%	0.011%
14	3.481	755	759	760	rBV4	1239	904	0.05%	0.006%
15	3.535	774	776	778	rBV3	1342	581	0.03%	0.004%
16	3.577	785	789	791	rBV5	1929	1338	0.07%	0.009%
17	3.622	801	803	808	rVB5	1419	1004	0.05%	0.007%
18	3.645	808	810	812	rVB3	1625	592	0.03%	0.004%
19	3.661	812	815	817	rBV3	1716	1122	0.06%	0.008%
20	3.687	820	823	824	rBV3	1365	728	0.04%	0.005%
21	3.902	872	890	924	rBV2	671444	1917619	100.00%	12.903%
22	4.343	1014	1027	1054	rVB	232418	586010	30.56%	3.943%
23	4.619	1110	1113	1117	rBV6	1732	1705	0.09%	0.011%
24	4.767	1157	1159	1161	rBV3	1099	575	0.03%	0.004%
25	4.815	1170	1174	1177	rBV5	1452	981	0.05%	0.007%
26	5.040	1228	1244	1272	rBV2	588324	1568101	81.77%	10.551%
27	5.471	1375	1378	1380	rBV3	1623	730	0.04%	0.005%
28	5.613	1410	1422	1453	rBV	505452	1032033	53.82%	6.944%
29	5.908	1502	1514	1540	rBV	594140	1164976	60.75%	7.839%
30	6.066	1551	1563	1587	rBV	361632	734614	38.31%	4.943%
31	6.500	1696	1698	1703	rVV6	1385	911	0.05%	0.006%
32	6.535	1707	1709	1715	rVB6	2172	1765	0.09%	0.012%
33	6.613	1730	1733	1736	rBV5	1532	1519	0.08%	0.010%
34	6.841	1802	1804	1809	rVB5	1189	668	0.03%	0.004%
35	6.905	1822	1824	1827	rBV4	1212	572	0.03%	0.004%
36	6.982	1837	1848	1870	rBV	166399	313840	16.37%	2.112%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028798.D
 Acq On : 31 Oct 2022 22:20
 Operator : SY/MD
 Sample : N5321-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	7.310	1939	1950	1976	rBV	669376	1159283	60.45%	7.800%
38	7.616	2036	2045	2064	rBV	104702	192220	10.02%	1.293%
39	7.940	2144	2146	2147	rBV2	1332	679	0.04%	0.005%
40	8.037	2174	2176	2178	rBV3	1272	599	0.03%	0.004%
41	8.085	2181	2191	2221	rBV	445242	861789	44.94%	5.799%
42	8.442	2298	2302	2307	rBV6	1833	1663	0.09%	0.011%
43	8.709	2382	2385	2388	rBV4	1774	1296	0.07%	0.009%
44	8.754	2396	2399	2403	rBV5	2000	1605	0.08%	0.011%
45	8.847	2417	2428	2449	rBV	740170	1211285	63.17%	8.150%
46	9.198	2535	2537	2540	rBV4	1549	708	0.04%	0.005%
47	9.243	2548	2551	2555	rVB6	2342	1542	0.08%	0.010%
48	9.317	2571	2574	2575	rBV3	1469	668	0.03%	0.004%
49	9.410	2599	2603	2605	rBV5	900	598	0.03%	0.004%
50	9.474	2620	2623	2625	rBV4	1446	960	0.05%	0.006%
51	9.603	2658	2663	2667	rBV7	2311	2337	0.12%	0.016%
52	9.844	2735	2738	2740	rBV4	1810	855	0.04%	0.006%
53	9.908	2755	2758	2763	rBV6	2034	1500	0.08%	0.010%
54	9.928	2763	2764	2768	rBV4	1225	892	0.05%	0.006%
55	10.063	2803	2806	2808	rBV4	1177	595	0.03%	0.004%
56	10.088	2808	2814	2818	rBV8	2563	3017	0.16%	0.020%
57	10.207	2841	2851	2872	rVB	465641	732867	38.22%	4.931%
58	10.407	2911	2913	2917	rVB6	1223	684	0.04%	0.005%
59	10.635	2979	2984	2987	rBV6	1767	1745	0.09%	0.012%
60	10.702	3003	3005	3007	rBV3	1965	1129	0.06%	0.008%
61	10.770	3024	3026	3027	rBV2	1685	674	0.04%	0.005%
62	10.834	3043	3046	3048	rBV4	1242	806	0.04%	0.005%
63	10.908	3065	3069	3070	rBV4	1822	1413	0.07%	0.010%
64	10.931	3071	3076	3081	rVV8	2174	2493	0.13%	0.017%
65	10.989	3091	3094	3096	rBV4	1523	907	0.05%	0.006%
66	11.001	3096	3098	3100	rBV3	2208	1016	0.05%	0.007%
67	11.046	3108	3112	3114	rBV4	2140	1495	0.08%	0.010%
68	11.239	3158	3172	3196	rBV	666861	1070646	55.83%	7.204%
69	11.616	3278	3289	3315	rBV	597571	969049	50.53%	6.520%
70	12.111	3439	3443	3444	rBV3	1919	1174	0.06%	0.008%
71	12.181	3463	3465	3468	rBV3	1190	803	0.04%	0.005%
72	12.226	3475	3479	3482	rBV6	1213	944	0.05%	0.006%
73	12.288	3495	3498	3499	rBV3	1199	620	0.03%	0.004%
74	12.413	3534	3537	3538	rBV3	1459	857	0.04%	0.006%
75	12.551	3576	3580	3581	rBV4	1984	1219	0.06%	0.008%
76	12.593	3590	3593	3596	rBV4	1100	655	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028798.D
 Acq On : 31 Oct 2022 22:20
 Operator : SY/MD
 Sample : N5321-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBWN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.625	3601	3603	3605	rBV3	1379	923	0.05%	0.006%
78	12.738	3634	3638	3639	rBV2	1316	836	0.04%	0.006%
79	12.783	3647	3652	3660	rBV2	2411	3367	0.18%	0.023%
80	12.866	3676	3678	3681	rVB3	1807	1004	0.05%	0.007%
81	12.886	3681	3684	3686	rBV4	1738	954	0.05%	0.006%
82	13.027	3726	3728	3732	rBV5	1326	846	0.04%	0.006%
83	13.088	3742	3747	3751	rBV8	2566	2562	0.13%	0.017%
84	13.130	3757	3760	3765	rBV6	1003	838	0.04%	0.006%
85	13.152	3765	3767	3769	rBV3	1347	640	0.03%	0.004%
86	13.239	3791	3794	3796	rBV4	1273	673	0.04%	0.005%
87	13.371	3832	3835	3837	rBV3	2146	1213	0.06%	0.008%
88	13.445	3854	3858	3859	rBV3	2367	1597	0.08%	0.011%
89	13.516	3877	3880	3882	rBV4	2224	1796	0.09%	0.012%
90	13.580	3897	3900	3901	rBV3	1924	983	0.05%	0.007%
91	13.718	3942	3943	3946	rBV3	1081	780	0.04%	0.005%
92	13.828	3970	3977	3980	rBV8	2148	2909	0.15%	0.020%
93	13.963	4016	4019	4021	rBV3	1594	1323	0.07%	0.009%
94	14.011	4032	4034	4036	rBV3	1459	970	0.05%	0.007%
95	14.226	4099	4101	4104	rVB4	2047	1130	0.06%	0.008%
96	14.368	4138	4145	4150	rVB9	2714	3163	0.16%	0.021%
97	14.442	4166	4168	4172	rVB5	1886	864	0.05%	0.006%
98	14.670	4237	4239	4240	rBV3	1872	831	0.04%	0.006%
99	14.876	4300	4303	4304	rBV3	1660	831	0.04%	0.006%
100	14.969	4330	4332	4333	rBV2	1734	648	0.03%	0.004%




Sum of corrected areas: 14861662

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028798.D
Acq On : 31 Oct 2022 22:20
Operator : SY/MD
Sample : N5321-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

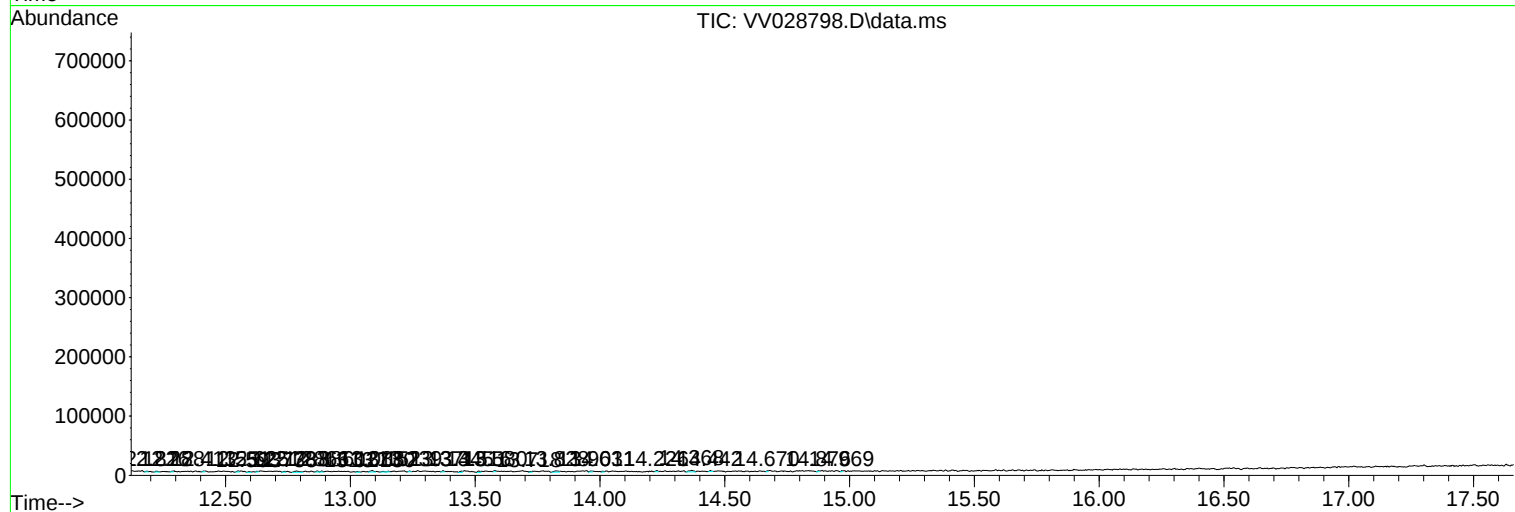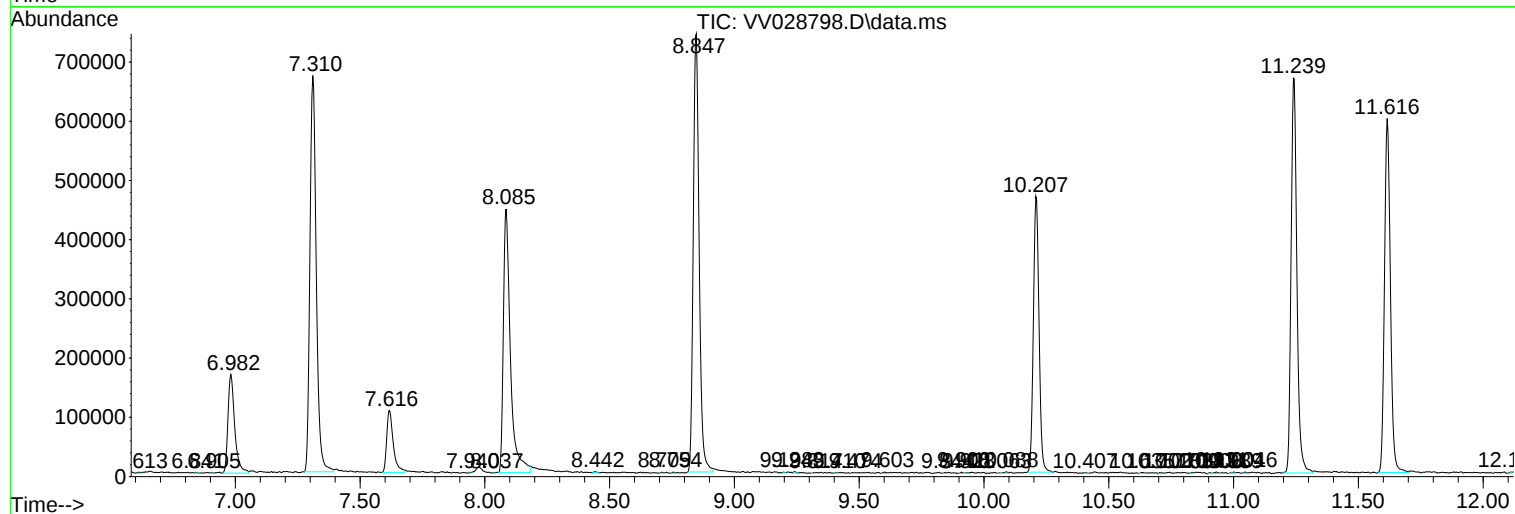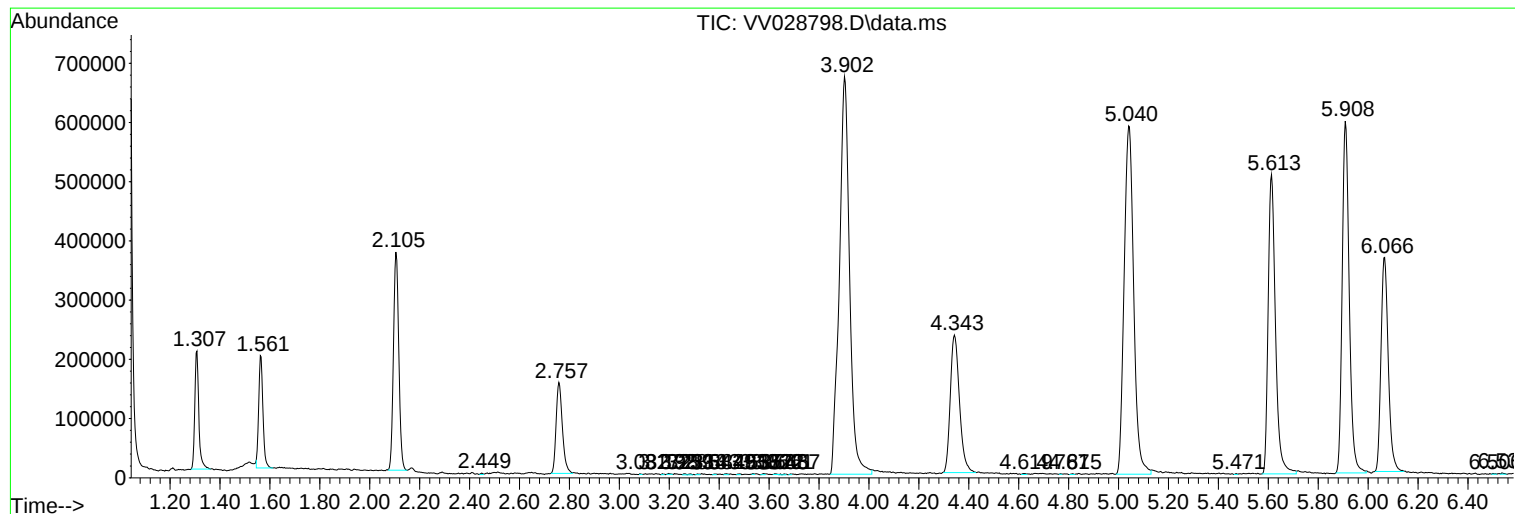

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028798.D
Acq On : 31 Oct 2022 22:20
Operator : SY/MD
Sample : N5321-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028798.D
Acq On : 31 Oct 2022 22:20
Operator : SY/MD
Sample : N5321-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc