

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028800.D
 Acq On : 31 Oct 2022 23:08
 Operator : SY/MD
 Sample : VIBLK304
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK304

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028800.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	77	82	101	rVB	181733	197021	12.87%	1.668%
2	1.561	156	162	181	rVB	183568	222592	14.55%	1.884%
3	2.105	322	331	347	rVB	369442	522115	34.12%	4.419%
4	2.433	431	433	435	rBV4	1564	562	0.04%	0.005%
5	2.503	448	455	468	rVB	41915	67481	4.41%	0.571%
6	2.703	513	517	525	rBV9	1866	2666	0.17%	0.023%
7	2.735	525	527	529	rBV3	1331	642	0.04%	0.005%
8	2.860	564	566	568	rBV3	1370	665	0.04%	0.006%
9	2.941	589	591	592	rBV2	1057	410	0.03%	0.003%
10	3.008	610	612	615	rBV4	1236	764	0.05%	0.006%
11	3.085	632	636	639	rBV5	1586	1488	0.10%	0.013%
12	3.285	696	698	700	rVB2	1431	641	0.04%	0.005%
13	3.297	700	702	704	rBV3	1375	944	0.06%	0.008%
14	3.349	716	718	720	rBV3	992	475	0.03%	0.004%
15	3.381	726	728	731	rVB4	1361	632	0.04%	0.005%
16	3.397	731	733	735	rBV3	1427	809	0.05%	0.007%
17	3.433	743	744	746	rBV2	776	363	0.02%	0.003%
18	3.555	780	782	784	rBV3	1644	629	0.04%	0.005%
19	3.590	790	793	794	rBV3	1172	830	0.05%	0.007%
20	3.748	841	842	844	rBV2	926	394	0.03%	0.003%
21	3.789	853	855	858	rBV4	1428	1104	0.07%	0.009%
22	3.870	872	880	919	rBV	146760	430489	28.13%	3.643%
23	4.342	1013	1027	1049	rBV	230966	575203	37.59%	4.868%
24	4.802	1165	1170	1171	rBV5	2171	1612	0.11%	0.014%
25	4.931	1209	1210	1213	rVB3	1323	552	0.04%	0.005%
26	4.953	1215	1217	1220	rBV4	1138	753	0.05%	0.006%
27	5.040	1228	1244	1276	rBV2	583761	1530287	100.00%	12.952%
28	5.613	1410	1422	1450	rBV	508162	1038303	67.85%	8.788%
29	6.066	1551	1563	1588	rBV	359826	729945	47.70%	6.178%
30	6.410	1668	1670	1672	rBV3	1141	591	0.04%	0.005%
31	6.577	1719	1722	1726	rBV6	2024	1897	0.12%	0.016%
32	6.915	1825	1827	1828	rBV2	955	451	0.03%	0.004%
33	6.982	1838	1848	1870	rBV	157851	295661	19.32%	2.502%
34	7.310	1938	1950	1970	rBV	650636	1142484	74.66%	9.670%
35	7.619	2037	2046	2066	rBV	101874	179157	11.71%	1.516%
36	7.863	2120	2122	2124	rBV3	1361	631	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028800.D
 Acq On : 31 Oct 2022 23:08
 Operator : SY/MD
 Sample : VIBLK304
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK304

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	7.892	2130	2131	2134	rVB2	1187	432	0.03%	0.004%
38	7.915	2134	2138	2139	rBV4	1396	820	0.05%	0.007%
39	8.085	2181	2191	2230	rBV	447779	864134	56.47%	7.314%
40	8.506	2319	2322	2323	rBV3	1087	607	0.04%	0.005%
41	8.847	2416	2428	2452	rBV	731574	1232203	80.52%	10.429%
42	9.072	2496	2498	2502	rVB5	2464	1251	0.08%	0.011%
43	9.114	2507	2511	2513	rBV5	2330	1684	0.11%	0.014%
44	9.394	2596	2598	2600	rBV2	1724	842	0.06%	0.007%
45	9.439	2611	2612	2618	rVB6	778	572	0.04%	0.005%
46	9.471	2618	2622	2626	rBV6	1984	1739	0.11%	0.015%
47	9.538	2642	2643	2644	rBV	1484	517	0.03%	0.004%
48	9.828	2731	2733	2735	rBV3	1799	953	0.06%	0.008%
49	9.847	2736	2739	2740	rVV3	1578	857	0.06%	0.007%
50	9.908	2755	2758	2760	rBV4	1662	1128	0.07%	0.010%
51	9.995	2782	2785	2787	rBV4	1417	785	0.05%	0.007%
52	10.017	2790	2792	2795	rBV4	1193	924	0.06%	0.008%
53	10.050	2800	2802	2805	rBV4	1748	1130	0.07%	0.010%
54	10.082	2811	2812	2816	rVB4	1373	446	0.03%	0.004%
55	10.104	2816	2819	2821	rBV4	1538	885	0.06%	0.007%
56	10.207	2840	2851	2874	rBV	448841	719016	46.99%	6.085%
57	10.567	2960	2963	2967	rBV5	1634	1709	0.11%	0.014%
58	10.680	2996	2998	3000	rBV3	1137	574	0.04%	0.005%
59	10.776	3026	3028	3029	rBV2	808	436	0.03%	0.004%
60	10.947	3080	3081	3083	rBV2	1280	568	0.04%	0.005%
61	10.992	3092	3095	3097	rBV3	1567	1063	0.07%	0.009%
62	11.030	3102	3107	3108	rBV5	1602	1424	0.09%	0.012%
63	11.159	3143	3147	3149	rBV4	1982	1301	0.09%	0.011%
64	11.188	3153	3156	3159	rBV4	2169	1913	0.13%	0.016%
65	11.239	3162	3172	3198	rVV	652320	1052076	68.75%	8.904%
66	11.615	3278	3289	3312	rBV	587578	940419	61.45%	7.959%
67	11.947	3390	3392	3394	rBV3	1766	902	0.06%	0.008%
68	12.046	3422	3423	3425	rBV2	1125	565	0.04%	0.005%
69	12.162	3456	3459	3463	rBV5	2280	1672	0.11%	0.014%
70	12.191	3466	3468	3471	rBV3	1475	1019	0.07%	0.009%
71	12.233	3478	3481	3483	rBV4	924	652	0.04%	0.006%
72	12.332	3511	3512	3516	rBV4	1041	746	0.05%	0.006%
73	12.416	3536	3538	3540	rBV3	984	457	0.03%	0.004%
74	12.442	3540	3546	3550	rVB9	1718	2054	0.13%	0.017%
75	12.471	3550	3555	3556	rBV4	1517	1065	0.07%	0.009%
76	12.564	3581	3584	3586	rBV4	1998	1113	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
 Data File : VV028800.D
 Acq On : 31 Oct 2022 23:08
 Operator : SY/MD
 Sample : VIBLK304
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK304

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.651	3608	3611	3613	rBV4	1743	1144	0.07%	0.010%
78	12.731	3632	3636	3637	rBV4	1334	1019	0.07%	0.009%
79	12.808	3658	3660	3661	rBV2	850	351	0.02%	0.003%
80	12.853	3672	3674	3675	rBV2	1191	489	0.03%	0.004%
81	12.992	3714	3717	3719	rBV4	1883	1245	0.08%	0.011%
82	13.101	3749	3751	3754	rBV3	1705	1039	0.07%	0.009%
83	13.117	3754	3756	3760	rVB5	1933	1456	0.10%	0.012%
84	13.149	3762	3766	3767	rBV4	1869	1197	0.08%	0.010%
85	13.185	3775	3777	3784	rBV8	881	715	0.05%	0.006%
86	13.242	3793	3795	3798	rBV3	1028	635	0.04%	0.005%
87	13.287	3805	3809	3811	rBV4	1436	1061	0.07%	0.009%
88	13.371	3833	3835	3838	rBV5	1074	729	0.05%	0.006%
89	13.477	3866	3868	3870	rBV3	1028	589	0.04%	0.005%
90	13.715	3939	3942	3945	rBV3	1075	968	0.06%	0.008%
91	13.738	3948	3949	3953	rVV3	1536	825	0.05%	0.007%
92	13.853	3982	3985	3986	rBV3	2278	1155	0.08%	0.010%
93	13.959	4016	4018	4020	rBV3	1271	553	0.04%	0.005%
94	14.001	4029	4031	4034	rVB3	1874	945	0.06%	0.008%
95	14.024	4034	4038	4039	rBV4	1397	931	0.06%	0.008%
96	14.287	4119	4120	4122	rBV2	1191	609	0.04%	0.005%
97	14.339	4134	4136	4139	rBV4	1206	758	0.05%	0.006%
98	14.358	4140	4142	4146	rBV5	2092	1139	0.07%	0.010%
99	14.532	4194	4196	4199	rBV4	1330	908	0.06%	0.008%
100	14.866	4298	4300	4302	rBV3	1648	916	0.06%	0.008%




Sum of corrected areas: 11815272

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028800.D
Acq On : 31 Oct 2022 23:08
Operator : SY/MD
Sample : VIBLK304
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK304

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

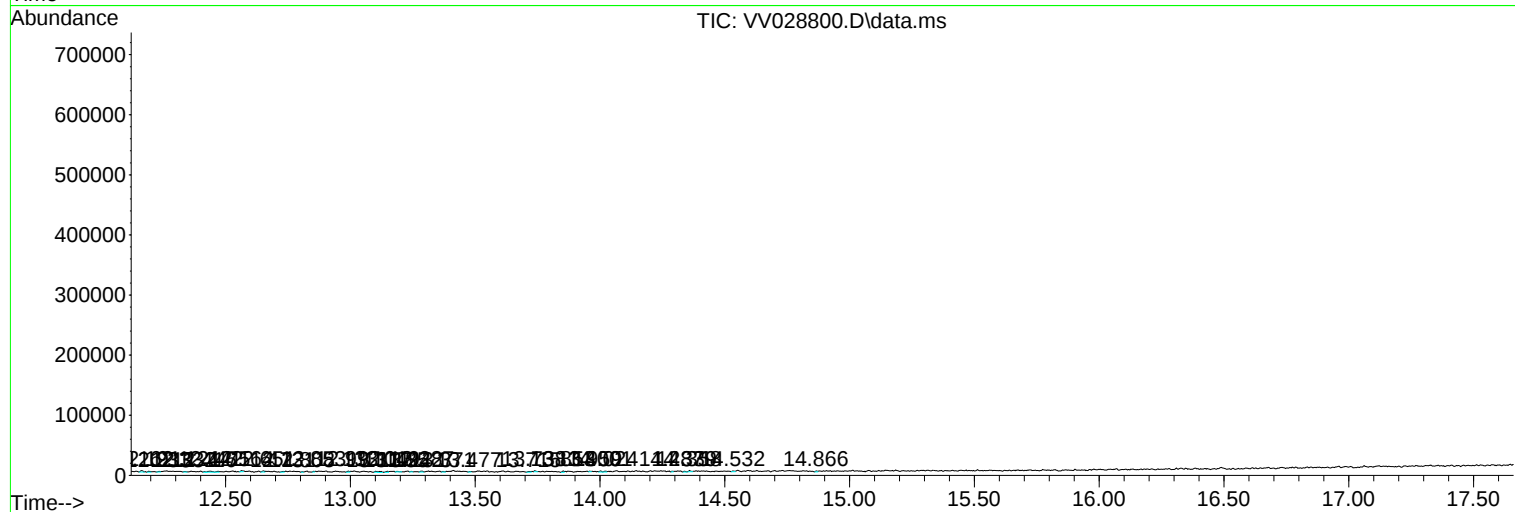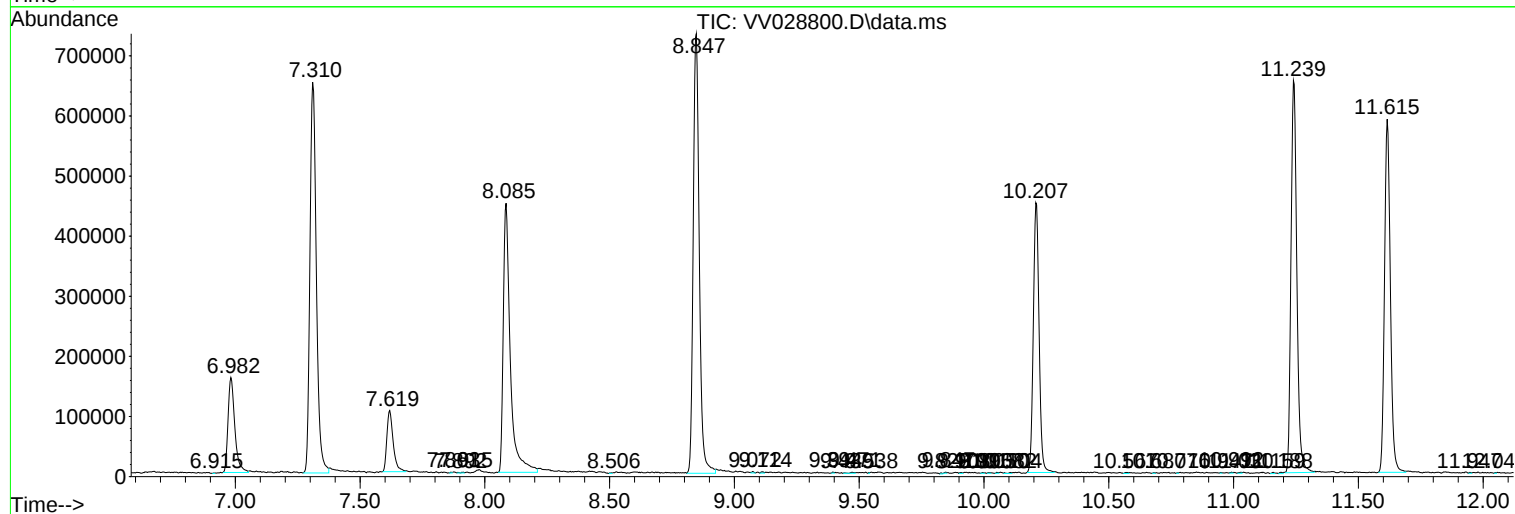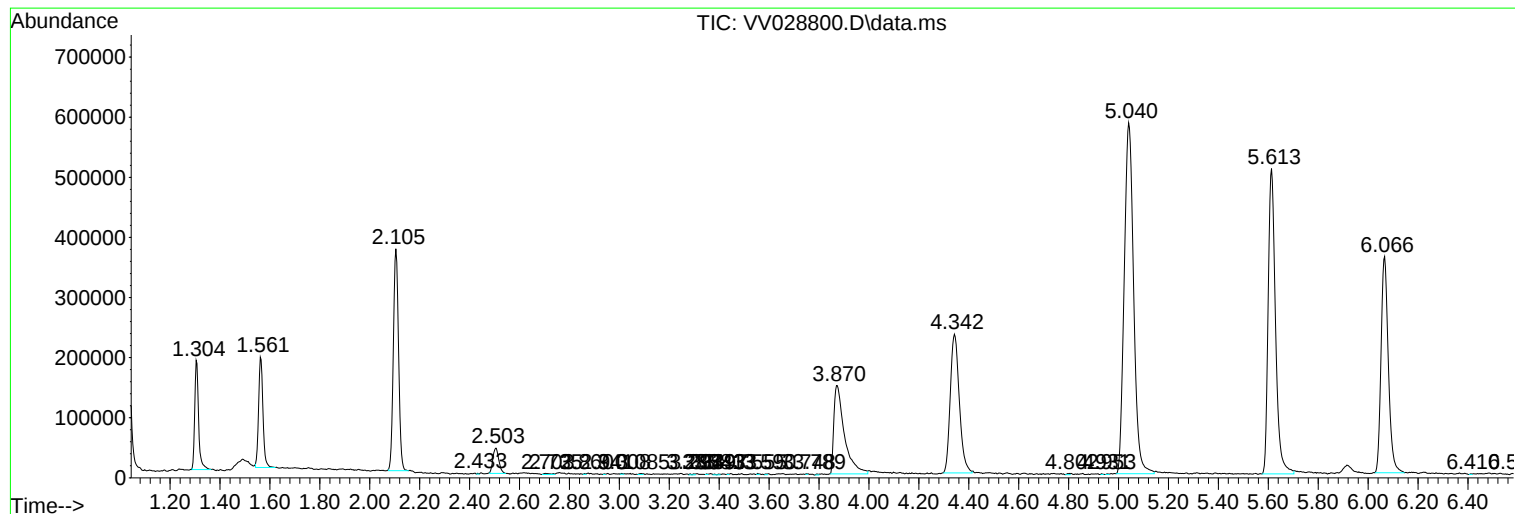

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028800.D
Acq On : 31 Oct 2022 23:08
Operator : SY/MD
Sample : VIBLK304
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK304

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103122\
Data File : VV028800.D
Acq On : 31 Oct 2022 23:08
Operator : SY/MD
Sample : VIBLK304
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK304

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc