

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW103123\
 Data File : VW032796.D
 Acq On : 31 Oct 2023 14:17
 Operator : SY/MD
 Sample : 05105-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 01 05:48:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 01 05:44:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	339773	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	374565	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	163606	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	146812	45.429	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.860%		
7) Chloroethane-d5	1.532	69	122301	45.249	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	90.500%		
11) 1,1-Dichloroethene-d2	2.060	65	58722	43.992	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.980%		
21) 2-Butanone-d5	3.786	46	131294	93.664	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	93.660%		
24) Chloroform-d	4.252	84	229251	44.443	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.880%		
26) 1,2-Dichloroethane-d4	4.944	65	146238	45.614	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.220%		
32) Benzene-d6	4.963	84	457983	47.555	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.100%		
36) 1,2-Dichloropropane-d6	5.992	67	139385	47.639	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.280%		
41) Toluene-d8	7.246	98	434496	45.819	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.640%		
43) trans-1,3-Dichloroprop...	7.554	79	70082	45.991	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.980%		
47) 2-Hexanone-d5	8.027	63	94870	88.818	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	88.820%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	196241	44.199	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.400%		
66) 1,2-Dichlorobenzene-d4	11.564	152	167594	53.157	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.320%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.551	75	3427	0.844	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032796.D
Acq On : 31 Oct 2023 14:17
Operator : SY/MD
Sample : 05105-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 01 05:48:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 01 05:44:49 2023
Response via : Initial Calibration

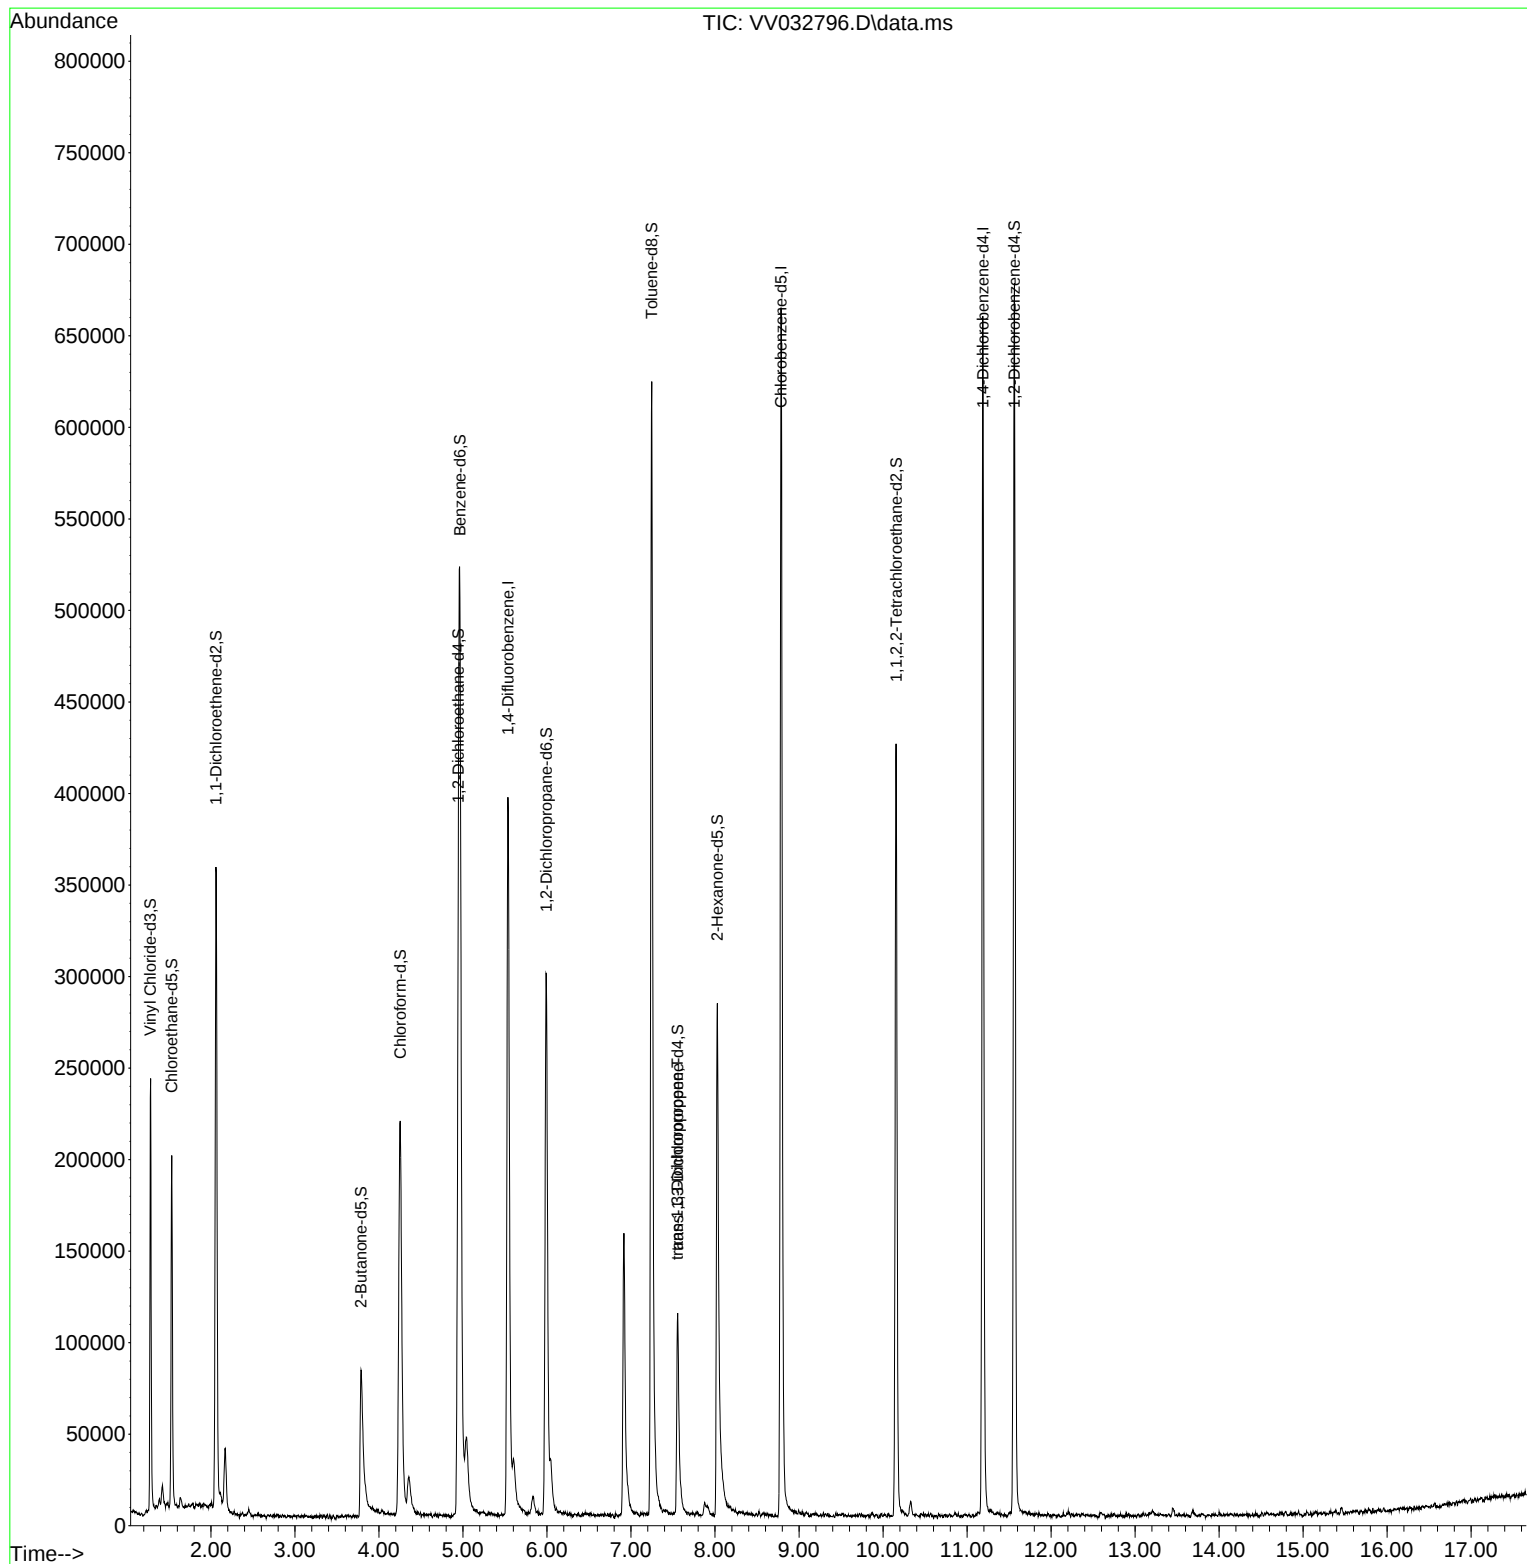

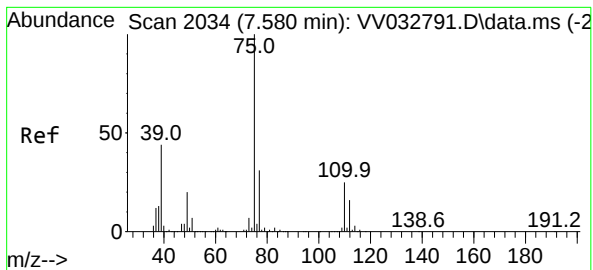

#44
 trans-1,3-Dichloropropene
 Concen: 0.844 ug/L
 RT: 7.551 min Scan# 20
 Delta R.T. -0.029 min
 Lab File: VV032796.D
 Acq: 31 Oct 2023 14:17

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 3427
 Ion Ratio Lower Upper
 75 100
 77 34.6 22.0 40.8

