

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032792.D
 Acq On : 31 Oct 2023 12:37
 Operator : SY/MD
 Sample : VV1031MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK207

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rVB	257937	261465	18.34%	2.295%
2	1.532	146	153	166	rBV	201755	236835	16.61%	2.079%
3	2.060	309	317	329	rBV	367827	532985	37.39%	4.678%
4	2.291	387	389	395	rVB7	1776	1084	0.08%	0.010%
5	2.789	542	544	548	rBV5	1620	1295	0.09%	0.011%
6	2.818	550	553	556	rVV5	1297	842	0.06%	0.007%
7	2.834	556	558	560	rVV3	1216	467	0.03%	0.004%
8	2.857	560	565	569	rVB7	1434	1599	0.11%	0.014%
9	2.883	569	573	577	rBV7	1414	1389	0.10%	0.012%
10	2.902	577	579	583	rBV4	1057	676	0.05%	0.006%
11	2.989	604	606	612	rVV6	1450	1142	0.08%	0.010%
12	3.015	612	614	616	rBV3	1038	482	0.03%	0.004%
13	3.027	616	618	620	rBV3	1430	717	0.05%	0.006%
14	3.056	625	627	628	rBV	1244	543	0.04%	0.005%
15	3.095	634	639	641	rBV6	1473	1553	0.11%	0.014%
16	3.121	643	647	657	rVV6	2282	3662	0.26%	0.032%
17	3.326	709	711	712	rBV2	1337	601	0.04%	0.005%
18	3.355	716	720	724	rBV7	2470	2287	0.16%	0.020%
19	3.397	732	733	736	rVB3	1430	597	0.04%	0.005%
20	3.420	739	740	743	rVB3	1353	634	0.04%	0.006%
21	3.442	743	747	750	rBV6	1938	1470	0.10%	0.013%
22	3.471	755	756	761	rVV5	936	562	0.04%	0.005%
23	3.519	769	771	774	rVB4	1614	798	0.06%	0.007%
24	3.590	789	793	795	rBV6	1144	944	0.07%	0.008%
25	3.687	820	823	824	rBV3	1792	765	0.05%	0.007%
26	3.696	824	826	829	rVV4	1012	697	0.05%	0.006%
27	3.789	846	855	880	rBV2	87120	242752	17.03%	2.131%
28	4.252	984	999	1021	rBV	226332	587664	41.22%	5.158%
29	4.494	1071	1074	1076	rBV4	1764	1319	0.09%	0.012%
30	4.564	1093	1096	1099	rBV5	1813	1330	0.09%	0.012%
31	4.706	1138	1140	1142	rBV3	1461	699	0.05%	0.006%
32	4.744	1148	1152	1157	rBV7	2138	2921	0.20%	0.026%
33	4.960	1203	1219	1236	rBV2	546924	1425655	100.00%	12.514%
34	5.535	1387	1398	1414	rBV	419167	859534	60.29%	7.545%
35	5.947	1522	1526	1528	rBV5	2318	1997	0.14%	0.018%
36	5.989	1528	1539	1554	rBV	309432	643916	45.17%	5.652%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032792.D
 Acq On : 31 Oct 2023 12:37
 Operator : SY/MD
 Sample : VV1031MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK207

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.288	1628	1632	1636	rBV6	1977	1868	0.13%	0.016%
38	6.387	1662	1663	1666	rBV3	1388	497	0.03%	0.004%
39	6.564	1716	1718	1720	rBV3	1923	874	0.06%	0.008%
40	6.632	1737	1739	1740	rBV2	1465	603	0.04%	0.005%
41	6.654	1744	1746	1747	rBV2	1716	612	0.04%	0.005%
42	6.760	1777	1779	1784	rBV5	1118	927	0.07%	0.008%
43	6.915	1817	1827	1860	rBV	165782	343519	24.10%	3.015%
44	7.124	1888	1892	1896	rBV6	2440	2812	0.20%	0.025%
45	7.246	1919	1930	1959	rBV	670139	1227532	86.10%	10.775%
46	7.555	2017	2026	2047	rBV	120809	230616	16.18%	2.024%
47	8.027	2163	2173	2207	rBV	287960	599186	42.03%	5.259%
48	8.519	2323	2326	2327	rBV3	1391	562	0.04%	0.005%
49	8.641	2362	2364	2367	rBV4	1115	482	0.03%	0.004%
50	8.696	2378	2381	2383	rBV4	1256	808	0.06%	0.007%
51	8.786	2398	2409	2434	rBV	705759	1190252	83.49%	10.448%
52	9.397	2597	2599	2600	rBV2	1052	389	0.03%	0.003%
53	9.429	2606	2609	2610	rBV3	1532	731	0.05%	0.006%
54	9.587	2656	2658	2660	rBV3	1132	734	0.05%	0.006%
55	9.645	2671	2676	2680	rVB8	2162	1942	0.14%	0.017%
56	9.667	2680	2683	2684	rBV3	2249	1125	0.08%	0.010%
57	9.715	2695	2698	2699	rBV3	1161	707	0.05%	0.006%
58	9.818	2727	2730	2734	rBV6	1599	1446	0.10%	0.013%
59	9.837	2734	2736	2738	rBV3	798	344	0.02%	0.003%
60	10.072	2805	2809	2811	rBV5	1034	694	0.05%	0.006%
61	10.156	2821	2835	2853	rBV	442634	720329	50.53%	6.323%
62	10.468	2930	2932	2934	rBV3	1978	995	0.07%	0.009%
63	10.609	2975	2976	2978	rVB2	1267	423	0.03%	0.004%
64	10.625	2978	2981	2986	rBV6	1408	1228	0.09%	0.011%
65	10.850	3048	3051	3054	rBV4	2486	2193	0.15%	0.019%
66	10.982	3090	3092	3094	rBV2	1666	806	0.06%	0.007%
67	11.188	3145	3156	3180	rBV	668574	1060104	74.36%	9.305%
68	11.474	3244	3245	3248	rVB2	1763	786	0.06%	0.007%
69	11.561	3261	3272	3290	rBV	688887	1093052	76.67%	9.594%
70	11.892	3374	3375	3380	rBV4	1631	1392	0.10%	0.012%
71	11.943	3388	3391	3393	rBV4	1370	985	0.07%	0.009%
72	11.985	3402	3404	3406	rBV4	1149	593	0.04%	0.005%
73	12.056	3422	3426	3433	rBV9	2017	2315	0.16%	0.020%
74	12.140	3449	3452	3453	rBV3	1601	746	0.05%	0.007%
75	12.445	3545	3547	3548	rBV2	2194	795	0.06%	0.007%
76	12.474	3554	3556	3558	rBV3	1896	613	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032792.D
 Acq On : 31 Oct 2023 12:37
 Operator : SY/MD
 Sample : VV1031MBL01
 Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK207

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.632	3603	3605	3608	rBV4	1305	458	0.03%	0.004%
78	12.699	3622	3626	3628	rBV5	1903	1404	0.10%	0.012%
79	12.715	3628	3631	3634	rBV5	1833	1340	0.09%	0.012%
80	12.789	3652	3654	3655	rBV2	1710	600	0.04%	0.005%
81	12.841	3667	3670	3673	rVB5	2208	1376	0.10%	0.012%
82	12.866	3676	3678	3682	rVV5	1251	857	0.06%	0.008%
83	12.953	3703	3705	3709	rBV5	2124	1548	0.11%	0.014%
84	12.985	3713	3715	3716	rBV2	1719	616	0.04%	0.005%
85	13.143	3762	3764	3766	rBV3	1089	688	0.05%	0.006%
86	13.355	3826	3830	3832	rBV5	1585	1265	0.09%	0.011%
87	13.384	3835	3839	3842	rBV6	1757	1362	0.10%	0.012%
88	13.448	3849	3859	3872	rBV	18623	34474	2.42%	0.303%
89	13.599	3903	3906	3909	rBV4	1254	1199	0.08%	0.011%
90	13.689	3926	3934	3939	rBV9	8546	14472	1.02%	0.127%
91	13.863	3986	3988	3990	rBV3	1336	559	0.04%	0.005%
92	13.882	3990	3994	3997	rBV6	1241	1185	0.08%	0.010%
93	13.934	4008	4010	4011	rBV2	1478	565	0.04%	0.005%
94	13.969	4019	4021	4023	rBV3	1155	580	0.04%	0.005%
95	14.204	4089	4094	4098	rBV8	3110	2526	0.18%	0.022%
96	14.461	4170	4174	4177	rBV6	1785	1594	0.11%	0.014%
97	14.586	4212	4213	4214	rBV	1342	459	0.03%	0.004%
98	14.670	4237	4239	4241	rBV3	1833	907	0.06%	0.008%
99	14.760	4265	4267	4271	rBV5	1781	1247	0.09%	0.011%
100	14.828	4286	4288	4290	rBV3	1815	762	0.05%	0.007%




Sum of corrected areas: 11392538

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032792.D
Acq On : 31 Oct 2023 12:37
Operator : SY/MD
Sample : VV1031MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK207

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

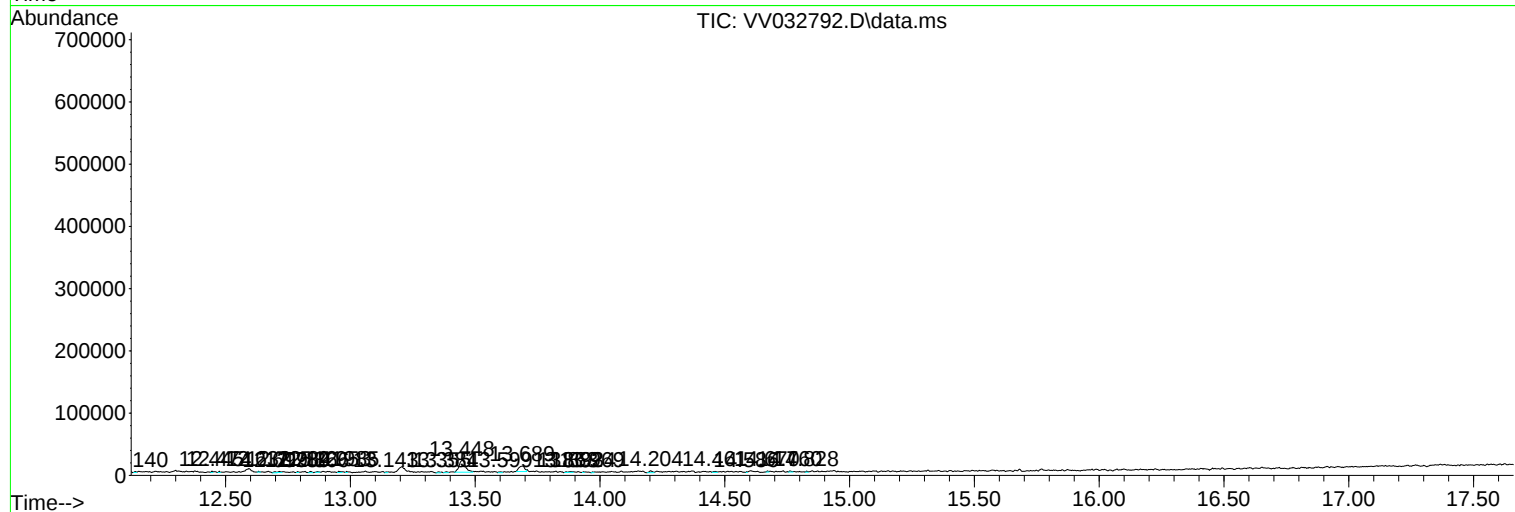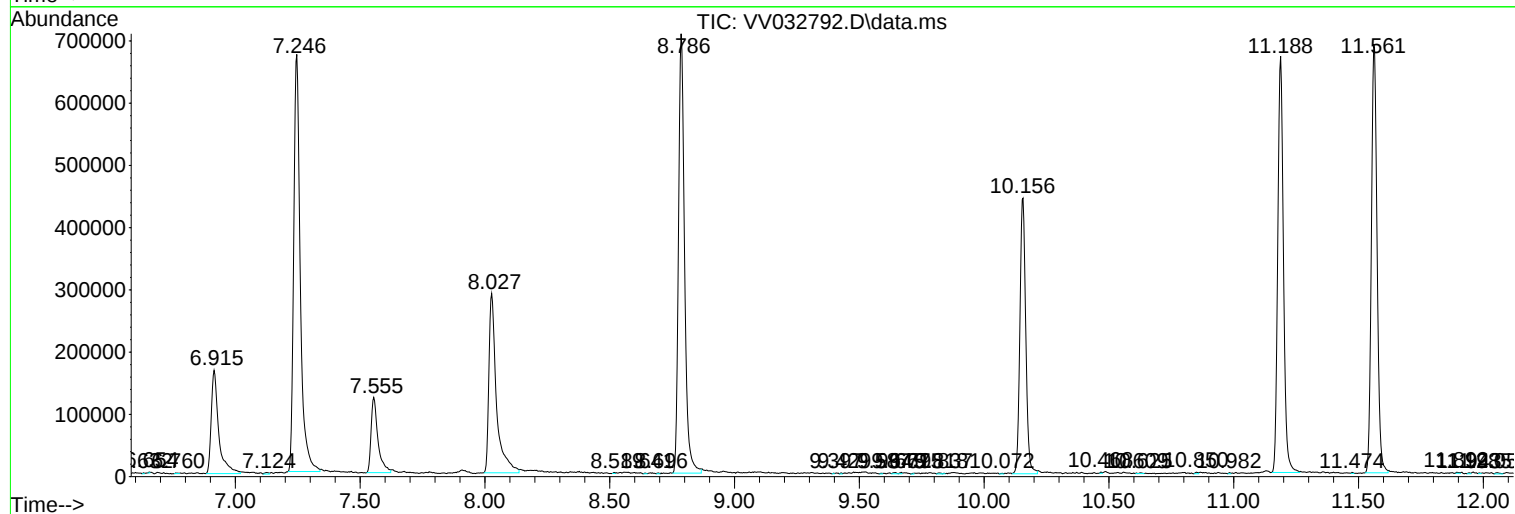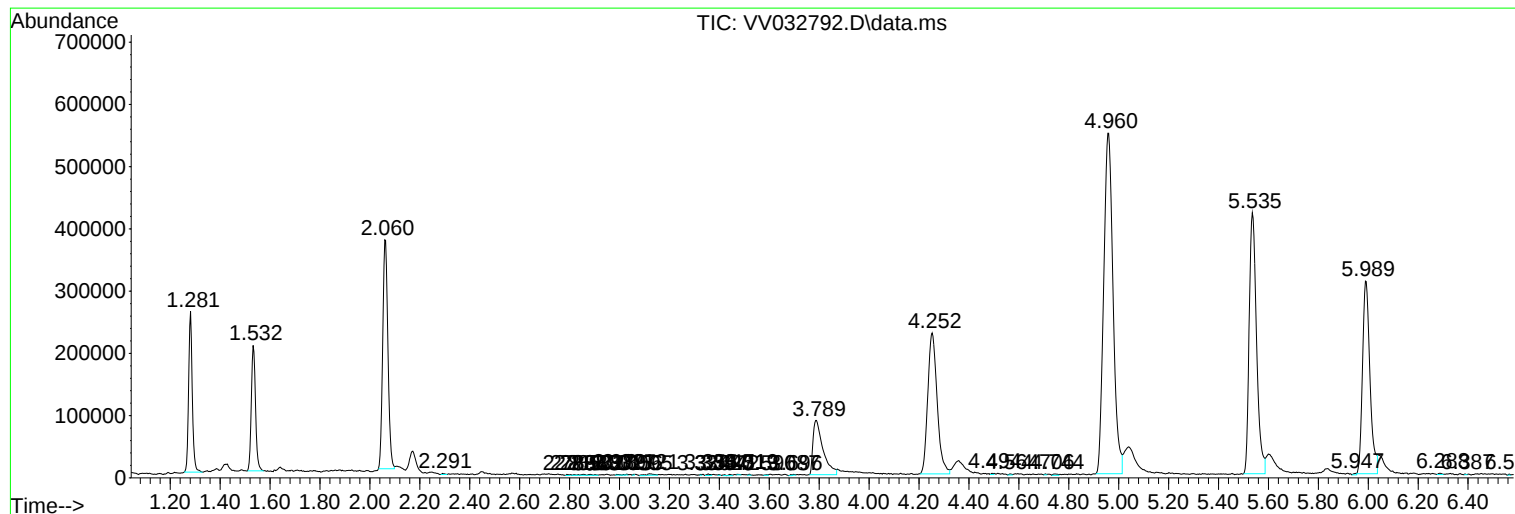

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032792.D
Acq On : 31 Oct 2023 12:37
Operator : SY/MD
Sample : VV1031MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK207

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032792.D
Acq On : 31 Oct 2023 12:37
Operator : SY/MD
Sample : VV1031MBL01
Misc : 5.00g/5.0mL/100ul/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK207

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc