

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032793.D
 Acq On : 31 Oct 2023 13:00
 Operator : SY/MD
 Sample : VV1031WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK208

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032793.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rVB	239987	251444	17.74%	2.220%
2	1.532	147	153	166	rVB	194991	229285	16.18%	2.024%
3	2.063	309	318	331	rBV	375041	533979	37.68%	4.715%
4	2.423	428	430	432	rBV3	1897	927	0.07%	0.008%
5	2.619	487	491	493	rBV4	1720	1556	0.11%	0.014%
6	2.703	515	517	518	rBV2	1796	752	0.05%	0.007%
7	2.751	527	532	535	rBV7	1458	1675	0.12%	0.015%
8	2.783	539	542	545	rVB5	1857	1298	0.09%	0.011%
9	2.806	545	549	553	rVB6	1448	1099	0.08%	0.010%
10	2.831	555	557	561	rVB4	1338	756	0.05%	0.007%
11	2.876	569	571	574	rBV4	1022	810	0.06%	0.007%
12	2.912	579	582	584	rBV4	1478	807	0.06%	0.007%
13	3.047	621	624	628	rVB6	1785	1579	0.11%	0.014%
14	3.066	628	630	633	rVB4	1166	548	0.04%	0.005%
15	3.092	633	638	644	rBV8	1906	2773	0.20%	0.024%
16	3.114	644	645	648	rBV3	966	580	0.04%	0.005%
17	3.153	653	657	662	rBV7	1557	1675	0.12%	0.015%
18	3.191	667	669	672	rVB4	1134	576	0.04%	0.005%
19	3.211	672	675	679	rBV5	1559	1478	0.10%	0.013%
20	3.336	712	714	718	rVB6	1404	616	0.04%	0.005%
21	3.359	718	721	725	rBV5	2267	1974	0.14%	0.017%
22	3.433	742	744	746	rBV3	1241	847	0.06%	0.007%
23	3.478	756	758	762	rBV4	1095	917	0.06%	0.008%
24	3.555	778	782	786	rVV6	1316	1265	0.09%	0.011%
25	3.597	793	795	799	rVB5	2263	1342	0.09%	0.012%
26	3.642	803	809	811	rBV8	1998	1746	0.12%	0.015%
27	3.706	826	829	832	rBV6	882	762	0.05%	0.007%
28	3.751	839	843	844	rBV4	1422	1001	0.07%	0.009%
29	3.789	846	855	884	rBV	89612	248312	17.52%	2.192%
30	4.172	972	974	976	rBV3	1356	620	0.04%	0.005%
31	4.252	985	999	1020	rBV	222507	575061	40.58%	5.077%
32	4.658	1121	1125	1127	rBV4	1753	1425	0.10%	0.013%
33	4.741	1149	1151	1153	rBV3	1635	964	0.07%	0.009%
34	4.960	1203	1219	1236	rBV2	542185	1417124	100.00%	12.512%
35	5.535	1387	1398	1414	rBV	415722	856599	60.45%	7.563%
36	5.992	1528	1540	1557	rBV	312740	661062	46.65%	5.837%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032793.D
 Acq On : 31 Oct 2023 13:00
 Operator : SY/MD
 Sample : VV1031WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK208

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.439	1673	1679	1681	rBV6	3430	3609	0.25%	0.032%
38	6.580	1718	1723	1725	rBV6	1785	1624	0.11%	0.014%
39	6.738	1768	1772	1773	rBV4	1591	1142	0.08%	0.010%
40	6.828	1796	1800	1801	rBV3	1669	1249	0.09%	0.011%
41	6.915	1817	1827	1850	rBV	165152	329684	23.26%	2.911%
42	7.246	1919	1930	1958	rBV	655551	1216208	85.82%	10.738%
43	7.555	2018	2026	2049	rBV2	118003	217195	15.33%	1.918%
44	8.027	2164	2173	2203	rBV	295302	604930	42.69%	5.341%
45	8.638	2359	2363	2366	rBV5	1319	1051	0.07%	0.009%
46	8.654	2366	2368	2370	rBV3	1264	700	0.05%	0.006%
47	8.786	2399	2409	2433	rBV	705662	1177462	83.09%	10.396%
48	9.117	2508	2512	2517	rBV6	1803	1788	0.13%	0.016%
49	9.233	2545	2548	2552	rBV5	1739	1631	0.12%	0.014%
50	9.490	2625	2628	2630	rBV3	1914	1059	0.07%	0.009%
51	9.632	2669	2672	2674	rBV4	1560	969	0.07%	0.009%
52	9.783	2716	2719	2722	rBV5	1678	1165	0.08%	0.010%
53	9.796	2722	2723	2726	rVV3	1241	564	0.04%	0.005%
54	9.834	2733	2735	2737	rBV3	1891	967	0.07%	0.009%
55	10.153	2823	2834	2854	rBV	447354	724437	51.12%	6.396%
56	10.407	2911	2913	2914	rBV2	1718	897	0.06%	0.008%
57	10.577	2963	2966	2967	rBV3	1718	812	0.06%	0.007%
58	10.603	2971	2974	2979	rVB7	1896	1690	0.12%	0.015%
59	10.689	2996	3001	3002	rBV5	1776	1552	0.11%	0.014%
60	10.837	3045	3047	3049	rBV3	1122	623	0.04%	0.006%
61	11.050	3110	3113	3114	rBV4	1166	692	0.05%	0.006%
62	11.188	3145	3156	3176	rBV	676716	1064171	75.09%	9.396%
63	11.381	3214	3216	3218	rVB3	1488	538	0.04%	0.005%
64	11.564	3261	3273	3291	rBV	693536	1107549	78.15%	9.779%
65	11.879	3369	3371	3373	rBV4	1336	927	0.07%	0.008%
66	11.998	3406	3408	3410	rVB3	2001	891	0.06%	0.008%
67	12.185	3464	3466	3474	rBV9	1743	1762	0.12%	0.016%
68	12.220	3474	3477	3478	rBV3	1304	671	0.05%	0.006%
69	12.249	3484	3486	3489	rVB4	1149	502	0.04%	0.004%
70	12.271	3489	3493	3494	rBV3	1364	949	0.07%	0.008%
71	12.297	3499	3501	3502	rBV2	2155	704	0.05%	0.006%
72	12.419	3536	3539	3540	rBV3	1460	921	0.06%	0.008%
73	12.525	3568	3572	3575	rBV6	1361	1471	0.10%	0.013%
74	12.757	3642	3644	3646	rBV3	1153	754	0.05%	0.007%
75	12.789	3649	3654	3656	rBV5	2222	1913	0.13%	0.017%
76	12.931	3693	3698	3702	rBV8	1728	1728	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032793.D
 Acq On : 31 Oct 2023 13:00
 Operator : SY/MD
 Sample : VV1031WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK208

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.947	3702	3703	3707	rVB4	1602	932	0.07%	0.008%
78	13.027	3724	3728	3731	rBV5	1474	1244	0.09%	0.011%
79	13.117	3754	3756	3759	rBV4	1014	717	0.05%	0.006%
80	13.204	3778	3783	3785	rBV5	6355	5642	0.40%	0.050%
81	13.278	3802	3806	3808	rBV5	1392	978	0.07%	0.009%
82	13.291	3808	3810	3816	rVV7	1380	1160	0.08%	0.010%
83	13.513	3877	3879	3882	rBV3	1515	1002	0.07%	0.009%
84	13.586	3901	3902	3904	rBV2	1216	570	0.04%	0.005%
85	13.622	3910	3913	3915	rBV4	1248	841	0.06%	0.007%
86	13.654	3921	3923	3926	rBV4	1548	659	0.05%	0.006%
87	13.686	3926	3933	3944	rVB4	7389	12380	0.87%	0.109%
88	13.738	3947	3949	3951	rBV3	1154	643	0.05%	0.006%
89	13.750	3951	3953	3956	rBV3	1846	1013	0.07%	0.009%
90	13.860	3985	3987	3990	rBV4	1534	1012	0.07%	0.009%
91	14.021	4035	4037	4041	rBV4	2102	1431	0.10%	0.013%
92	14.226	4096	4101	4104	rBV7	2301	2410	0.17%	0.021%
93	14.294	4120	4122	4124	rBV3	1660	705	0.05%	0.006%
94	14.413	4157	4159	4160	rBV2	1678	824	0.06%	0.007%
95	14.442	4166	4168	4172	rBV5	1807	1017	0.07%	0.009%
96	14.525	4191	4194	4197	rBV3	1468	1284	0.09%	0.011%
97	14.673	4238	4240	4243	rBV4	1694	1231	0.09%	0.011%
98	14.715	4250	4253	4255	rBV4	2197	1545	0.11%	0.014%
99	14.747	4261	4263	4265	rBV3	1929	1150	0.08%	0.010%
100	15.156	4386	4390	4391	rBV3	1863	1414	0.10%	0.012%




Sum of corrected areas: 11326189

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032793.D
Acq On : 31 Oct 2023 13:00
Operator : SY/MD
Sample : VV1031WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK208

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

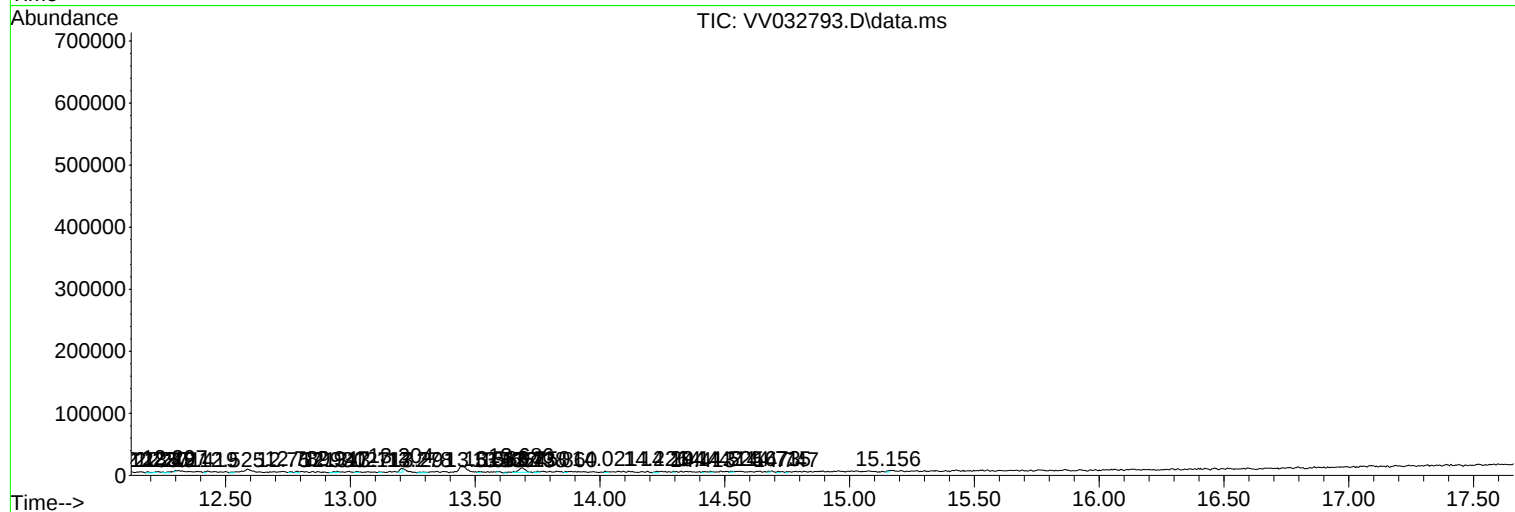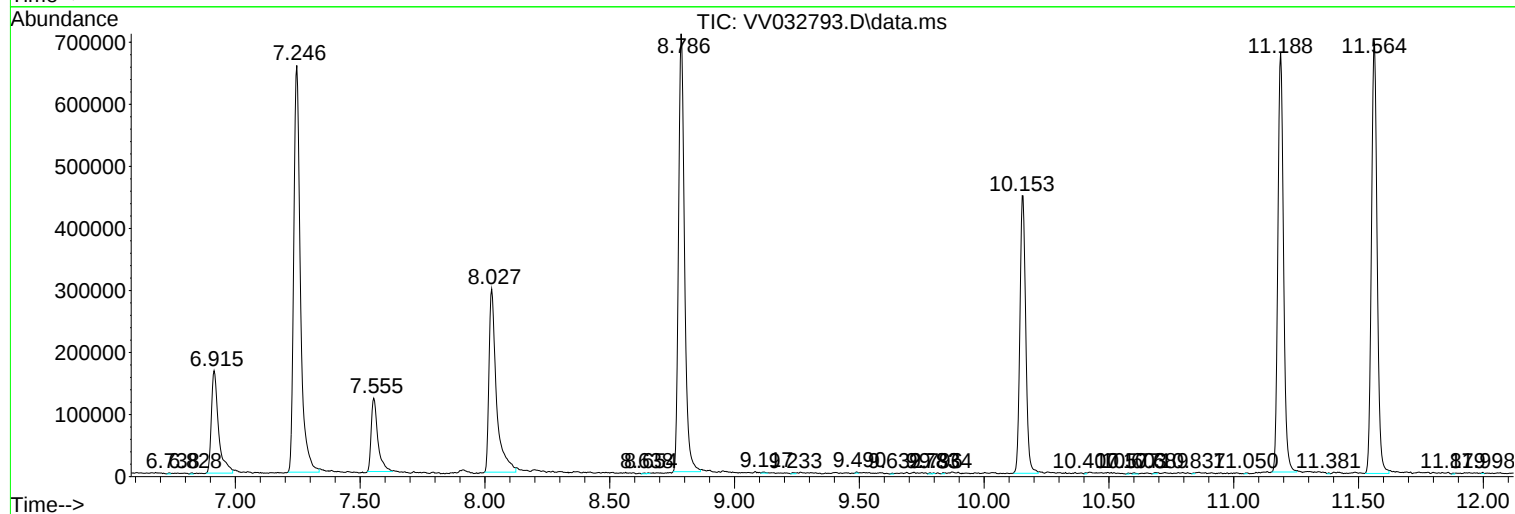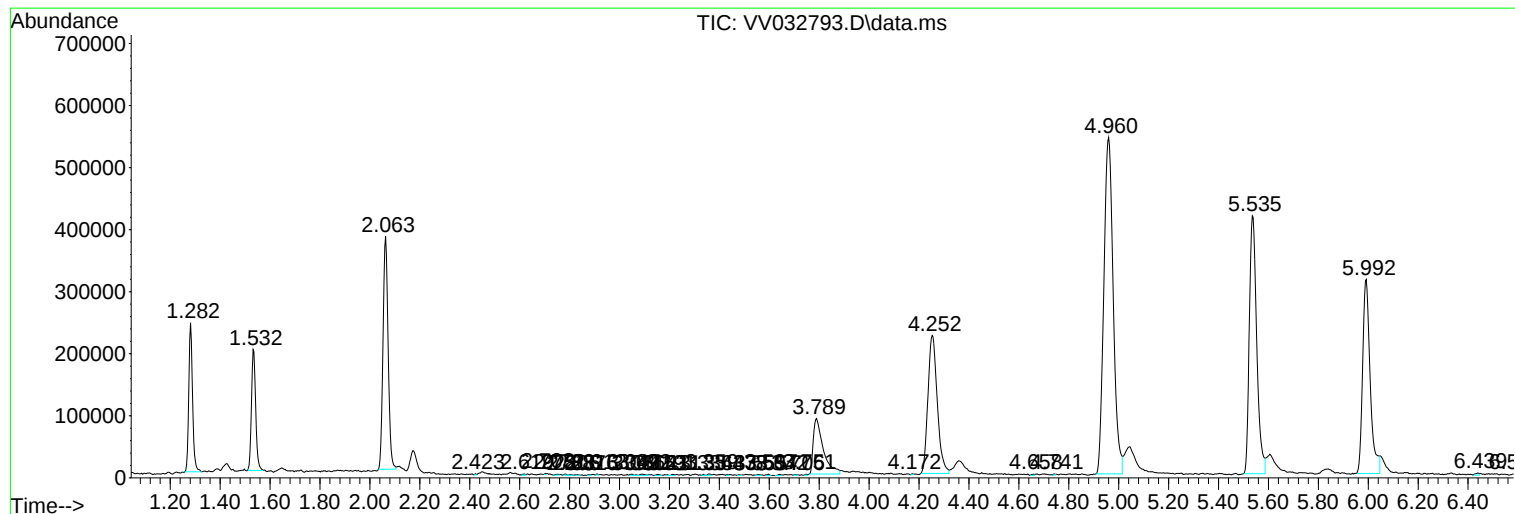

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032793.D
Acq On : 31 Oct 2023 13:00
Operator : SY/MD
Sample : VV1031WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK208

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032793.D
Acq On : 31 Oct 2023 13:00
Operator : SY/MD
Sample : VV1031WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK208

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------