

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032797.D
 Acq On : 31 Oct 2023 14:41
 Operator : SY/MD
 Sample : 05105-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0005

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.182	40	44	46	rBV5	2272	1815	0.13%	0.017%
2	1.282	68	75	91	rBV	236217	246414	17.69%	2.340%
3	1.532	146	153	168	rVB	194239	229031	16.44%	2.175%
4	2.060	309	317	331	rBV	360793	509681	36.59%	4.839%
5	2.452	430	439	441	rBV10	3948	5268	0.38%	0.050%
6	2.503	452	455	456	rBV3	1450	590	0.04%	0.006%
7	2.542	464	467	471	rBV5	2270	1793	0.13%	0.017%
8	2.616	488	490	491	rBV2	1137	638	0.05%	0.006%
9	2.754	531	533	535	rBV2	1456	921	0.07%	0.009%
10	2.786	541	543	544	rBV2	1088	438	0.03%	0.004%
11	3.050	622	625	626	rBV3	929	436	0.03%	0.004%
12	3.143	651	654	656	rBV3	1478	885	0.06%	0.008%
13	3.156	656	658	662	rVB4	1552	783	0.06%	0.007%
14	3.172	662	663	664	rBV	1589	492	0.04%	0.005%
15	3.240	682	684	687	rVV4	1161	522	0.04%	0.005%
16	3.310	703	706	707	rBV2	711	415	0.03%	0.004%
17	3.320	707	709	713	rVB4	1323	484	0.03%	0.005%
18	3.339	713	715	717	rBV3	1614	805	0.06%	0.008%
19	3.355	717	720	722	rBV4	970	540	0.04%	0.005%
20	3.400	732	734	735	rBV2	1217	547	0.04%	0.005%
21	3.442	745	747	748	rBV2	996	456	0.03%	0.004%
22	3.471	751	756	757	rBV5	1581	1084	0.08%	0.010%
23	3.561	781	784	785	rBV2	1515	795	0.06%	0.008%
24	3.625	802	804	805	rBV2	833	421	0.03%	0.004%
25	3.706	826	829	831	rBV3	1994	1350	0.10%	0.013%
26	3.751	840	843	844	rBV2	1634	1028	0.07%	0.010%
27	3.786	846	854	877	rVV	83884	223728	16.06%	2.124%
28	4.252	985	999	1021	rBV	216609	561094	40.29%	5.328%
29	4.764	1154	1158	1161	rBV5	1417	1118	0.08%	0.011%
30	4.777	1161	1162	1165	rBV3	1316	653	0.05%	0.006%
31	4.818	1173	1175	1176	rBV2	879	440	0.03%	0.004%
32	4.960	1202	1219	1236	rBV3	532089	1392810	100.00%	13.225%
33	5.304	1324	1326	1330	rBV5	1784	1005	0.07%	0.010%
34	5.535	1384	1398	1414	rBV	340493	703424	50.50%	6.679%
35	5.992	1528	1540	1553	rBV2	301675	616720	44.28%	5.856%
36	6.371	1655	1658	1660	rBV4	1451	828	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032797.D
 Acq On : 31 Oct 2023 14:41
 Operator : SY/MD
 Sample : 05105-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0005

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.426	1673	1675	1677	rBV3	1747	1098	0.08%	0.010%
38	6.490	1692	1695	1697	rBV4	1626	995	0.07%	0.009%
39	6.529	1705	1707	1709	rVB2	1348	461	0.03%	0.004%
40	6.571	1716	1720	1725	rBV7	1542	1984	0.14%	0.019%
41	6.706	1760	1762	1765	rBV4	1237	711	0.05%	0.007%
42	6.915	1818	1827	1847	rBV	152918	306341	21.99%	2.909%
43	7.169	1904	1906	1908	rBV3	2078	1310	0.09%	0.012%
44	7.246	1918	1930	1954	rBV	641934	1189772	85.42%	11.297%
45	7.555	2017	2026	2052	rBV	113233	218803	15.71%	2.078%
46	7.979	2157	2158	2161	rBV3	1076	625	0.04%	0.006%
47	8.027	2164	2173	2203	rVV	302276	614867	44.15%	5.838%
48	8.436	2296	2300	2302	rBV4	1912	1777	0.13%	0.017%
49	8.561	2337	2339	2340	rBV2	1736	724	0.05%	0.007%
50	8.673	2372	2374	2377	rVB3	1263	571	0.04%	0.005%
51	8.786	2397	2409	2433	rBV	572425	982019	70.51%	9.324%
52	9.188	2531	2534	2536	rBV4	1467	1106	0.08%	0.011%
53	9.262	2555	2557	2561	rBV5	1463	764	0.05%	0.007%
54	9.458	2615	2618	2622	rVV6	1870	1415	0.10%	0.013%
55	9.477	2622	2624	2627	rVB4	1615	1037	0.07%	0.010%
56	9.580	2653	2656	2660	rBV6	1652	1258	0.09%	0.012%
57	9.654	2677	2679	2681	rBV2	1639	974	0.07%	0.009%
58	9.683	2686	2688	2692	rVB5	1317	629	0.05%	0.006%
59	9.702	2692	2694	2697	rBV3	1050	834	0.06%	0.008%
60	9.821	2728	2731	2733	rBV4	1765	1122	0.08%	0.011%
61	9.934	2764	2766	2769	rBV3	1685	705	0.05%	0.007%
62	9.985	2780	2782	2784	rBV3	1427	752	0.05%	0.007%
63	10.053	2799	2803	2808	rBV7	1958	2063	0.15%	0.020%
64	10.091	2811	2815	2817	rBV5	1686	1126	0.08%	0.011%
65	10.156	2824	2835	2861	rVB	450753	706881	50.75%	6.712%
66	10.323	2880	2887	2889	rBV8	6083	6328	0.45%	0.060%
67	10.587	2967	2969	2972	rVB4	1738	801	0.06%	0.008%
68	10.606	2972	2975	2976	rBV3	1554	724	0.05%	0.007%
69	10.796	3031	3034	3037	rBV4	1947	1437	0.10%	0.014%
70	10.828	3042	3044	3046	rBV3	961	439	0.03%	0.004%
71	10.908	3066	3069	3071	rBV3	1645	1052	0.08%	0.010%
72	10.979	3089	3091	3093	rBV3	1275	513	0.04%	0.005%
73	11.188	3145	3156	3183	rBV	563875	884608	63.51%	8.399%
74	11.500	3250	3253	3256	rBV5	1786	1301	0.09%	0.012%
75	11.564	3262	3273	3290	rBV	669707	1053216	75.62%	10.000%
76	11.870	3364	3368	3370	rBV5	1450	1402	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032797.D
 Acq On : 31 Oct 2023 14:41
 Operator : SY/MD
 Sample : 05105-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0005

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	11.882	3370	3372	3377	rVB4	2105	1410	0.10%	0.013%
78	12.040	3419	3421	3424	rBV5	1770	1042	0.07%	0.010%
79	12.088	3434	3436	3439	rVB4	2326	1266	0.09%	0.012%
80	12.255	3485	3488	3489	rBV3	1433	870	0.06%	0.008%
81	12.509	3566	3567	3570	rBV3	1096	538	0.04%	0.005%
82	12.567	3582	3585	3588	rBV5	1839	1194	0.09%	0.011%
83	12.657	3611	3613	3614	rBV2	780	430	0.03%	0.004%
84	12.667	3614	3616	3620	rVV5	1870	1056	0.08%	0.010%
85	12.712	3628	3630	3631	rBV2	1306	435	0.03%	0.004%
86	12.734	3636	3637	3639	rBV2	1092	508	0.04%	0.005%
87	12.934	3696	3699	3701	rBV4	1388	908	0.07%	0.009%
88	13.114	3753	3755	3758	rBV4	2011	1109	0.08%	0.011%
89	13.136	3758	3762	3768	rVB8	2406	2055	0.15%	0.020%
90	13.165	3768	3771	3773	rBV3	1582	970	0.07%	0.009%
91	13.201	3777	3782	3786	rBV8	2854	3423	0.25%	0.033%
92	13.259	3798	3800	3803	rBV3	1308	666	0.05%	0.006%
93	13.580	3896	3900	3902	rBV4	1687	1225	0.09%	0.012%
94	13.802	3968	3969	3971	rBV	1246	457	0.03%	0.004%
95	13.834	3974	3979	3980	rBV5	1395	1317	0.09%	0.013%
96	13.905	3997	4001	4003	rVB5	951	706	0.05%	0.007%
97	14.149	4075	4077	4080	rBV4	1303	589	0.04%	0.006%
98	14.432	4160	4165	4167	rBV6	2387	1755	0.13%	0.017%
99	14.471	4175	4177	4178	rBV2	1137	460	0.03%	0.004%
100	15.136	4382	4384	4391	rBV9	3097	3303	0.24%	0.031%




Sum of corrected areas: 10531689

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032797.D
Acq On : 31 Oct 2023 14:41
Operator : SY/MD
Sample : 05105-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

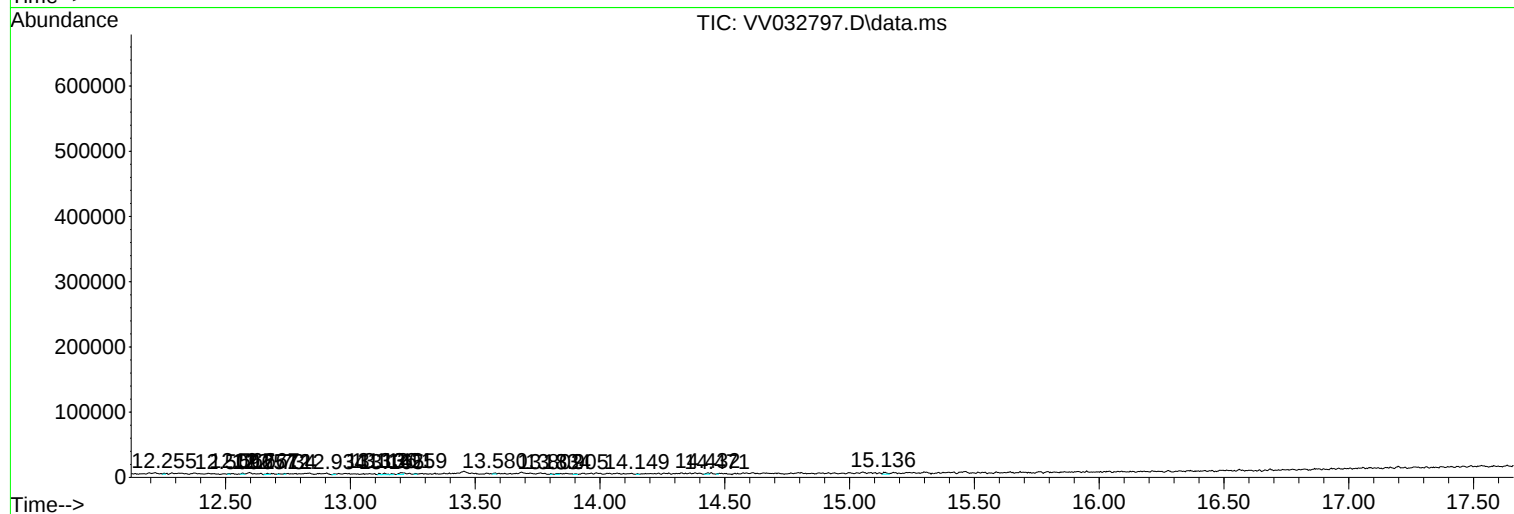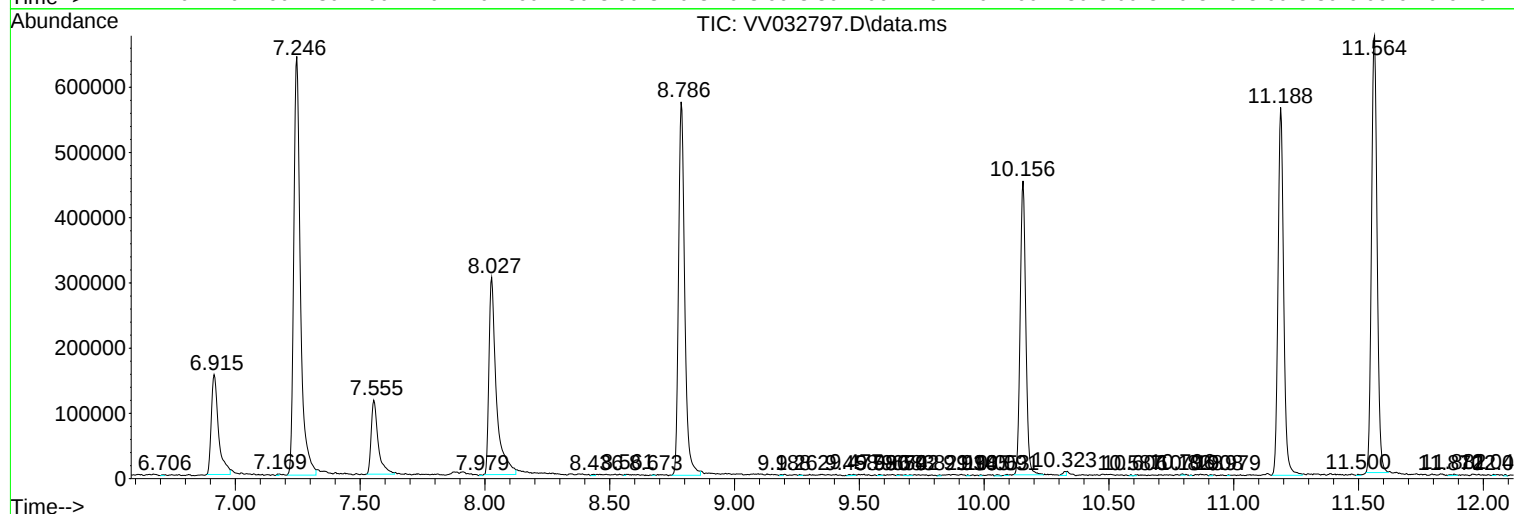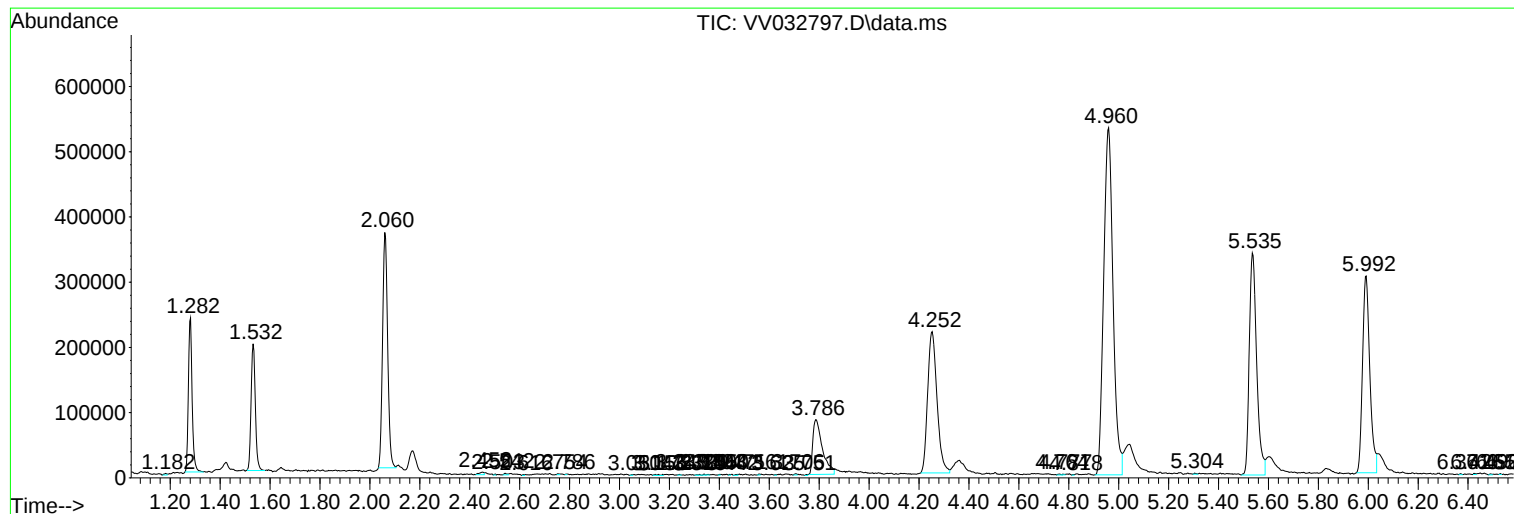

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032797.D
Acq On : 31 Oct 2023 14:41
Operator : SY/MD
Sample : 05105-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032797.D
Acq On : 31 Oct 2023 14:41
Operator : SY/MD
Sample : 05105-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0005

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc