

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032798.D
 Acq On : 31 Oct 2023 15:04
 Operator : SY/MD
 Sample : 05105-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0009

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032798.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rVB	226650	236381	17.85%	2.160%
2	1.532	146	153	168	rVB	187446	217058	16.39%	1.983%
3	2.060	308	317	332	rBV	350924	510582	38.56%	4.665%
4	2.494	450	452	454	rBV3	1155	576	0.04%	0.005%
5	2.548	467	469	473	rBV5	1623	1111	0.08%	0.010%
6	2.571	473	476	479	rVB5	2135	1403	0.11%	0.013%
7	2.645	497	499	502	rBV4	2188	1615	0.12%	0.015%
8	2.780	539	541	545	rVB5	1415	762	0.06%	0.007%
9	2.812	547	551	554	rVB6	2373	1491	0.11%	0.014%
10	2.828	554	556	558	rBV3	1382	729	0.06%	0.007%
11	3.098	638	640	643	rBV4	1484	748	0.06%	0.007%
12	3.127	645	649	653	rVV6	1245	1106	0.08%	0.010%
13	3.147	653	655	660	rVB4	2259	1492	0.11%	0.014%
14	3.169	660	662	665	rBV3	1141	625	0.05%	0.006%
15	3.262	688	691	694	rBV5	2121	1720	0.13%	0.016%
16	3.307	702	705	706	rBV3	730	422	0.03%	0.004%
17	3.333	712	713	715	rBV2	819	395	0.03%	0.004%
18	3.388	726	730	733	rBV6	2725	2441	0.18%	0.022%
19	3.449	746	749	751	rVB4	1727	909	0.07%	0.008%
20	3.610	794	799	800	rBV5	1761	1575	0.12%	0.014%
21	3.664	813	816	817	rBV2	731	476	0.04%	0.004%
22	3.706	825	829	832	rBV6	2294	1963	0.15%	0.018%
23	3.738	837	839	843	rVB4	1979	1003	0.08%	0.009%
24	3.786	846	854	879	rBV	72844	200247	15.12%	1.829%
25	4.140	962	964	967	rBV3	1110	659	0.05%	0.006%
26	4.249	985	998	1019	rBV	208149	536887	40.55%	4.905%
27	4.661	1123	1126	1129	rVB5	1306	827	0.06%	0.008%
28	4.780	1160	1163	1167	rBV6	1472	1213	0.09%	0.011%
29	4.867	1188	1190	1197	rVB7	1159	825	0.06%	0.008%
30	4.892	1197	1198	1200	rBV2	1003	521	0.04%	0.005%
31	4.960	1203	1219	1235	rBV2	507767	1324058	100.00%	12.097%
32	5.400	1354	1356	1359	rBV4	1332	596	0.05%	0.005%
33	5.455	1371	1373	1376	rBV5	2006	1228	0.09%	0.011%
34	5.535	1387	1398	1413	rBV	378756	787978	59.51%	7.199%
35	5.838	1481	1492	1505	rBV	183943	376571	28.44%	3.440%
36	5.989	1529	1539	1554	rBV	284848	585334	44.21%	5.348%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032798.D
 Acq On : 31 Oct 2023 15:04
 Operator : SY/MD
 Sample : 05105-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0009

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.214	1607	1609	1611	rBV3	1914	962	0.07%	0.009%
38	6.388	1660	1663	1667	rVB5	1731	1158	0.09%	0.011%
39	6.426	1672	1675	1676	rBV3	1595	644	0.05%	0.006%
40	6.445	1676	1681	1685	rBV8	2505	2795	0.21%	0.026%
41	6.738	1770	1772	1773	rBV2	1595	595	0.04%	0.005%
42	6.786	1785	1787	1789	rBV3	1501	933	0.07%	0.009%
43	6.915	1818	1827	1852	rBV	150641	304369	22.99%	2.781%
44	7.140	1895	1897	1900	rBV4	1632	1285	0.10%	0.012%
45	7.246	1918	1930	1964	rBV	614456	1160491	87.65%	10.602%
46	7.394	1975	1976	1979	rBV3	2028	1300	0.10%	0.012%
47	7.555	2017	2026	2047	rBV	113746	213079	16.09%	1.947%
48	8.027	2164	2173	2204	rBV	267204	554795	41.90%	5.069%
49	8.317	2261	2263	2267	rBV4	1894	1373	0.10%	0.013%
50	8.683	2375	2377	2380	rBV3	2039	1137	0.09%	0.010%
51	8.786	2398	2409	2438	rBV	657586	1115619	84.26%	10.192%
52	9.027	2482	2484	2485	rBV2	1669	597	0.05%	0.005%
53	9.079	2498	2500	2504	rBV5	2185	1155	0.09%	0.011%
54	9.313	2569	2573	2576	rBV5	2000	1710	0.13%	0.016%
55	9.381	2592	2594	2595	rBV2	1150	551	0.04%	0.005%
56	9.484	2621	2626	2628	rBV5	2888	2374	0.18%	0.022%
57	9.539	2641	2643	2647	rBV4	1622	1298	0.10%	0.012%
58	9.616	2664	2667	2668	rBV3	860	490	0.04%	0.004%
59	9.748	2706	2708	2709	rBV2	1679	643	0.05%	0.006%
60	9.802	2722	2725	2727	rBV4	1766	1103	0.08%	0.010%
61	9.902	2754	2756	2757	rBV2	1204	495	0.04%	0.005%
62	10.021	2790	2793	2796	rBV4	1793	1245	0.09%	0.011%
63	10.082	2810	2812	2815	rBV4	1323	1070	0.08%	0.010%
64	10.156	2823	2835	2856	rBV	424086	684660	51.71%	6.255%
65	10.326	2877	2888	2896	rBV	6782	11935	0.90%	0.109%
66	10.378	2902	2904	2907	rVB4	1297	589	0.04%	0.005%
67	10.426	2915	2919	2922	rBV6	1563	1253	0.09%	0.011%
68	10.458	2927	2929	2931	rBV3	1870	851	0.06%	0.008%
69	10.539	2952	2954	2956	rBV3	1294	605	0.05%	0.006%
70	10.564	2960	2962	2966	rVV4	1251	803	0.06%	0.007%
71	10.629	2980	2982	2985	rVB4	1183	766	0.06%	0.007%
72	10.648	2985	2988	2991	rVB5	1364	925	0.07%	0.008%
73	10.670	2994	2995	2997	rBV2	1201	671	0.05%	0.006%
74	10.760	3021	3023	3024	rBV2	1194	458	0.03%	0.004%
75	10.796	3027	3034	3040	rVV2	1938	2656	0.20%	0.024%
76	10.838	3045	3047	3051	rVB4	1496	866	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032798.D
 Acq On : 31 Oct 2023 15:04
 Operator : SY/MD
 Sample : 05105-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0009

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	10.911	3068	3070	3072	rBV3	1347	684	0.05%	0.006%
78	10.992	3091	3095	3096	rBV4	1523	866	0.07%	0.008%
79	11.188	3144	3156	3175	rBV	652908	1008205	76.15%	9.211%
80	11.564	3262	3273	3287	rBV	650183	1031739	77.92%	9.426%
81	11.918	3382	3383	3385	rBV2	1324	564	0.04%	0.005%
82	12.127	3445	3448	3449	rBV3	1212	668	0.05%	0.006%
83	12.214	3473	3475	3477	rBV3	1909	1061	0.08%	0.010%
84	12.268	3489	3492	3496	rBV6	1973	1693	0.13%	0.015%
85	12.349	3514	3517	3520	rBV4	1754	1234	0.09%	0.011%
86	12.481	3556	3558	3560	rBV4	1162	464	0.04%	0.004%
87	12.667	3614	3616	3617	rBV2	824	392	0.03%	0.004%
88	12.715	3629	3631	3634	rBV4	1407	1020	0.08%	0.009%
89	12.799	3654	3657	3660	rBV5	1334	1386	0.10%	0.013%
90	13.079	3742	3744	3745	rBV2	1505	497	0.04%	0.005%
91	13.101	3748	3751	3752	rBV2	1642	832	0.06%	0.008%
92	13.133	3758	3761	3765	rBV6	2967	2396	0.18%	0.022%
93	13.387	3838	3840	3842	rBV3	1260	783	0.06%	0.007%
94	13.413	3844	3848	3849	rBV4	1870	1062	0.08%	0.010%
95	13.619	3910	3912	3916	rVB5	1848	1103	0.08%	0.010%
96	13.664	3923	3926	3928	rBV3	1583	1155	0.09%	0.011%
97	13.847	3981	3983	3985	rBV3	2184	1149	0.09%	0.010%
98	14.043	4042	4044	4045	rBV	1327	566	0.04%	0.005%
99	14.178	4081	4086	4087	rBV5	1830	1847	0.14%	0.017%
100	14.262	4110	4112	4113	rBV2	1207	438	0.03%	0.004%




Sum of corrected areas: 10945635

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032798.D
Acq On : 31 Oct 2023 15:04
Operator : SY/MD
Sample : 05105-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0009

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

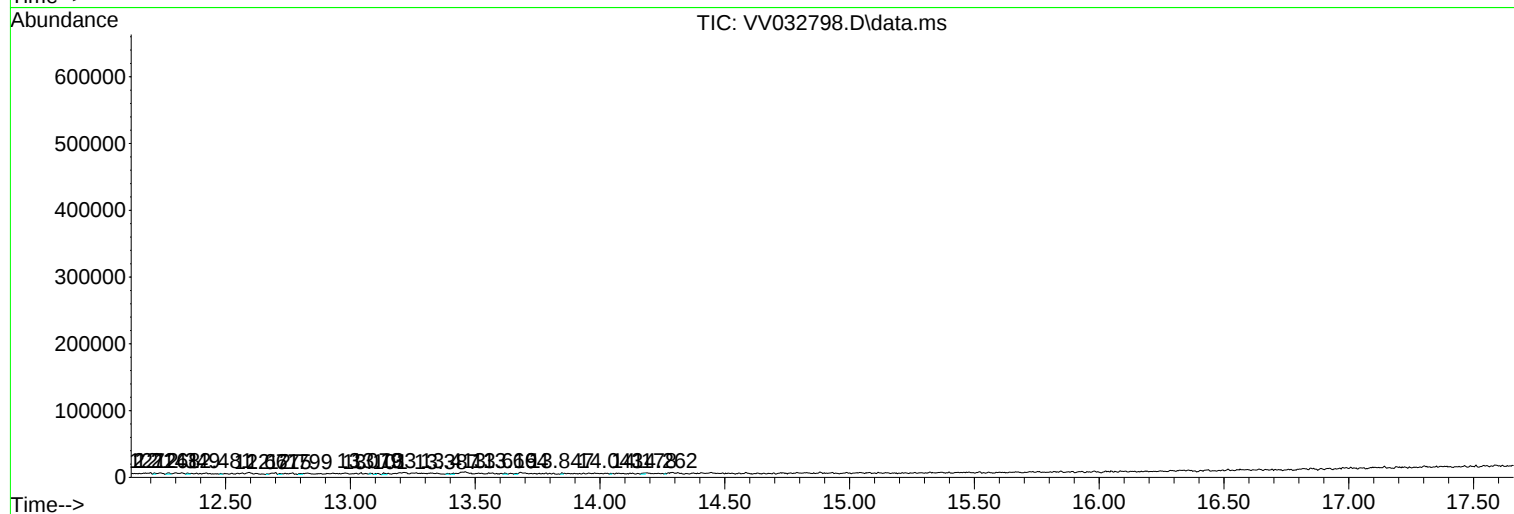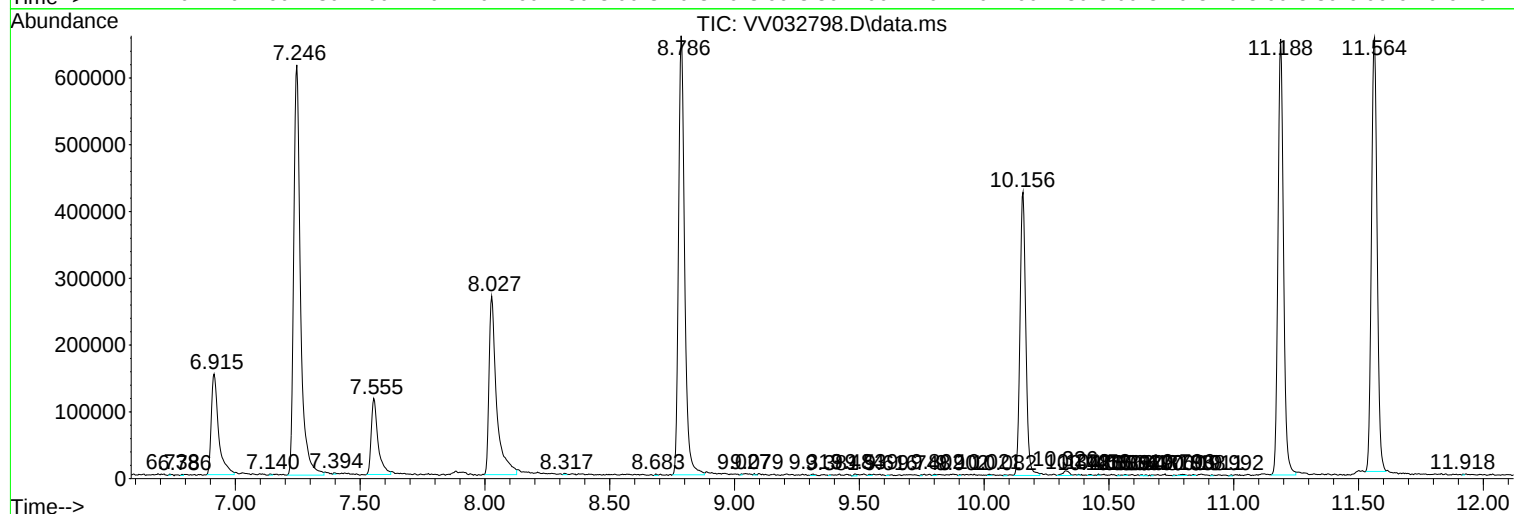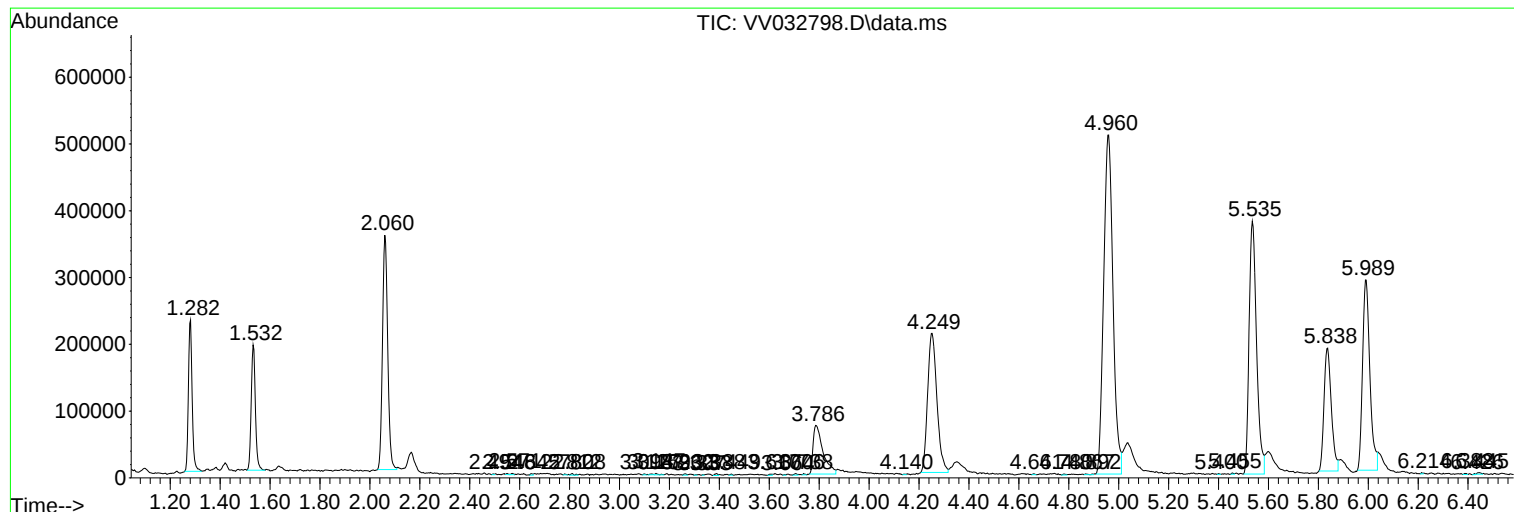

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032798.D
Acq On : 31 Oct 2023 15:04
Operator : SY/MD
Sample : 05105-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0009

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032798.D
Acq On : 31 Oct 2023 15:04
Operator : SY/MD
Sample : 05105-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0009

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------