

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032799.D
 Acq On : 31 Oct 2023 15:27
 Operator : SY/MD
 Sample : 05105-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0010

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032799.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rBV	221936	231966	17.33%	2.189%
2	1.532	147	153	163	rVB	184005	207619	15.51%	1.959%
3	2.060	308	317	329	rBV	352927	509537	38.07%	4.808%
4	2.362	409	411	413	rBV3	1255	520	0.04%	0.005%
5	2.513	454	458	462	rBV6	1617	1485	0.11%	0.014%
6	2.539	464	466	468	rBV3	1826	867	0.06%	0.008%
7	2.587	479	481	485	rVB5	1599	737	0.06%	0.007%
8	2.638	494	497	498	rBV2	1010	469	0.04%	0.004%
9	2.661	502	504	506	rBV3	1161	622	0.05%	0.006%
10	2.741	526	529	531	rBV4	1194	619	0.05%	0.006%
11	2.770	534	538	540	rBV5	1577	1211	0.09%	0.011%
12	2.783	540	542	543	rBV2	1270	403	0.03%	0.004%
13	2.828	553	556	557	rBV2	966	494	0.04%	0.005%
14	2.863	562	567	570	rBV7	2207	2190	0.16%	0.021%
15	2.963	595	598	599	rBV2	848	487	0.04%	0.005%
16	3.031	617	619	620	rBV2	788	386	0.03%	0.004%
17	3.163	659	660	664	rVB3	2196	927	0.07%	0.009%
18	3.182	664	666	668	rBV3	1661	849	0.06%	0.008%
19	3.211	671	675	677	rBV5	1338	890	0.07%	0.008%
20	3.262	690	691	692	rBV	1249	416	0.03%	0.004%
21	3.298	700	702	704	rVB4	1356	434	0.03%	0.004%
22	3.336	713	714	719	rBV4	1152	793	0.06%	0.007%
23	3.362	719	722	726	rVB6	1894	1191	0.09%	0.011%
24	3.381	726	728	729	rBV2	779	394	0.03%	0.004%
25	3.388	729	730	732	rVB2	1652	494	0.04%	0.005%
26	3.407	734	736	740	rBV5	1174	708	0.05%	0.007%
27	3.426	740	742	744	rBV4	1328	674	0.05%	0.006%
28	3.497	762	764	766	rBV3	1506	760	0.06%	0.007%
29	3.535	774	776	778	rBV3	1136	551	0.04%	0.005%
30	3.654	809	813	816	rBV6	1012	920	0.07%	0.009%
31	3.687	821	823	827	rBV5	1354	880	0.07%	0.008%
32	3.786	846	854	881	rBV	76456	209797	15.68%	1.980%
33	4.253	985	999	1019	rBV	213570	538723	40.25%	5.084%
34	4.625	1113	1115	1117	rBV3	1209	606	0.05%	0.006%
35	4.716	1141	1143	1147	rVB4	2054	1265	0.09%	0.012%
36	4.777	1160	1162	1164	rBV3	1501	911	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032799.D
 Acq On : 31 Oct 2023 15:27
 Operator : SY/MD
 Sample : 05105-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0010

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	4.815	1173	1174	1177	rBV2	1264	436	0.03%	0.004%
38	4.841	1180	1182	1184	rBV3	1426	699	0.05%	0.007%
39	4.957	1202	1218	1236	rBV2	508770	1338289	100.00%	12.629%
40	5.535	1385	1398	1413	rBV	385557	785187	58.67%	7.409%
41	5.992	1528	1540	1566	rBV	289526	649798	48.55%	6.132%
42	6.269	1625	1626	1627	rBV	1143	419	0.03%	0.004%
43	6.506	1696	1700	1703	rBV5	1945	1604	0.12%	0.015%
44	6.523	1703	1705	1706	rBV2	1270	428	0.03%	0.004%
45	6.706	1759	1762	1766	rBV6	2011	1569	0.12%	0.015%
46	6.793	1786	1789	1792	rVB5	1403	835	0.06%	0.008%
47	6.812	1792	1795	1800	rBV7	2425	1916	0.14%	0.018%
48	6.834	1800	1802	1803	rBV2	1103	561	0.04%	0.005%
49	6.915	1817	1827	1857	rBV	152238	313996	23.46%	2.963%
50	7.246	1918	1930	1961	rBV	611100	1157214	86.47%	10.920%
51	7.555	2017	2026	2048	rBV2	110384	209434	15.65%	1.976%
52	7.873	2121	2125	2131	rBV8	4978	6831	0.51%	0.064%
53	8.027	2161	2173	2201	rBV	271811	563891	42.14%	5.321%
54	8.317	2261	2263	2264	rBV2	1528	513	0.04%	0.005%
55	8.522	2324	2327	2329	rBV3	1622	900	0.07%	0.008%
56	8.786	2399	2409	2433	rBV	641804	1083000	80.92%	10.220%
57	9.050	2489	2491	2494	rBV3	2224	1407	0.11%	0.013%
58	9.378	2592	2593	2596	rBV3	926	364	0.03%	0.003%
59	9.471	2620	2622	2624	rBV3	1730	935	0.07%	0.009%
60	9.510	2632	2634	2637	rBV4	2235	1334	0.10%	0.013%
61	9.921	2760	2762	2763	rBV2	971	230	0.02%	0.002%
62	10.069	2806	2808	2810	rBV2	1397	688	0.05%	0.006%
63	10.101	2810	2818	2820	rVV9	2061	2366	0.18%	0.022%
64	10.156	2823	2835	2852	rVV	422415	681078	50.89%	6.427%
65	10.416	2912	2916	2919	rBV7	1941	1265	0.09%	0.012%
66	10.471	2931	2933	2936	rBV4	1504	758	0.06%	0.007%
67	10.490	2936	2939	2940	rBV3	1561	941	0.07%	0.009%
68	10.538	2952	2954	2957	rBV3	1887	1178	0.09%	0.011%
69	10.587	2967	2969	2970	rBV2	1132	412	0.03%	0.004%
70	10.825	3038	3043	3046	rBV6	1444	1495	0.11%	0.014%
71	10.998	3093	3097	3100	rBV5	2196	1899	0.14%	0.018%
72	11.027	3103	3106	3107	rBV3	1223	536	0.04%	0.005%
73	11.079	3119	3122	3126	rVB6	2411	2054	0.15%	0.019%
74	11.108	3126	3131	3132	rBV4	2621	2312	0.17%	0.022%
75	11.188	3145	3156	3178	rBV	641800	985949	73.67%	9.304%
76	11.493	3247	3251	3252	rBV4	3822	2292	0.17%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032799.D
 Acq On : 31 Oct 2023 15:27
 Operator : SY/MD
 Sample : 05105-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0010

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	11.564	3262	3273	3295	rVB	663320	1047309	78.26%	9.883%
78	11.818	3350	3352	3353	rBV2	1159	444	0.03%	0.004%
79	11.934	3385	3388	3389	rBV3	1825	1038	0.08%	0.010%
80	11.982	3398	3403	3404	rBV5	1746	1332	0.10%	0.013%
81	12.169	3458	3461	3463	rBV3	1465	1102	0.08%	0.010%
82	12.345	3513	3516	3517	rBV3	1940	947	0.07%	0.009%
83	12.448	3541	3548	3549	rBV6	1618	1615	0.12%	0.015%
84	12.632	3600	3605	3607	rBV5	2100	1957	0.15%	0.018%
85	12.709	3627	3629	3631	rVB3	1177	363	0.03%	0.003%
86	12.731	3633	3636	3639	rBV6	1531	1240	0.09%	0.012%
87	13.124	3756	3758	3761	rVB4	1564	746	0.06%	0.007%
88	13.143	3761	3764	3766	rBV4	1030	565	0.04%	0.005%
89	13.291	3807	3810	3812	rBV3	1322	579	0.04%	0.005%
90	13.316	3815	3818	3820	rVV4	1563	842	0.06%	0.008%
91	13.406	3844	3846	3849	rBV3	1410	790	0.06%	0.007%
92	13.519	3880	3881	3883	rBV2	1450	563	0.04%	0.005%
93	13.625	3909	3914	3916	rBV6	1779	1759	0.13%	0.017%
94	13.956	4015	4017	4020	rBV4	1318	906	0.07%	0.009%
95	14.493	4182	4184	4189	rBV6	2014	2099	0.16%	0.020%
96	14.705	4247	4250	4251	rBV3	1626	911	0.07%	0.009%
97	14.760	4265	4267	4271	rBV4	1836	1218	0.09%	0.011%




Sum of corrected areas: 10597133

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032799.D
Acq On : 31 Oct 2023 15:27
Operator : SY/MD
Sample : 05105-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0010

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

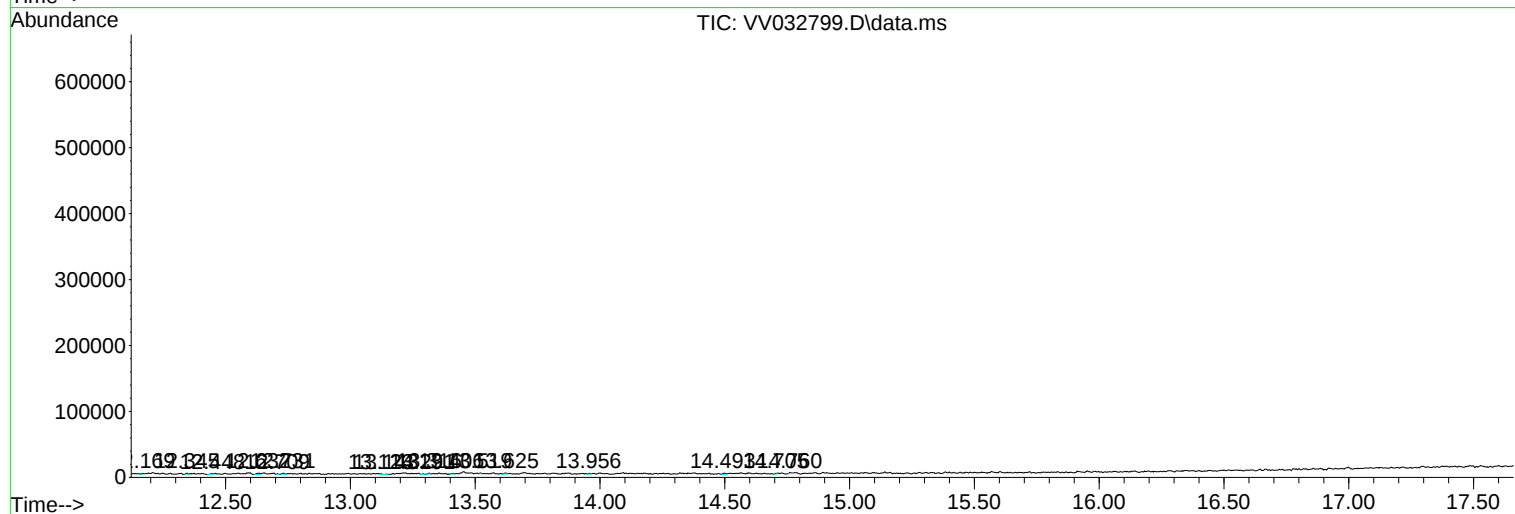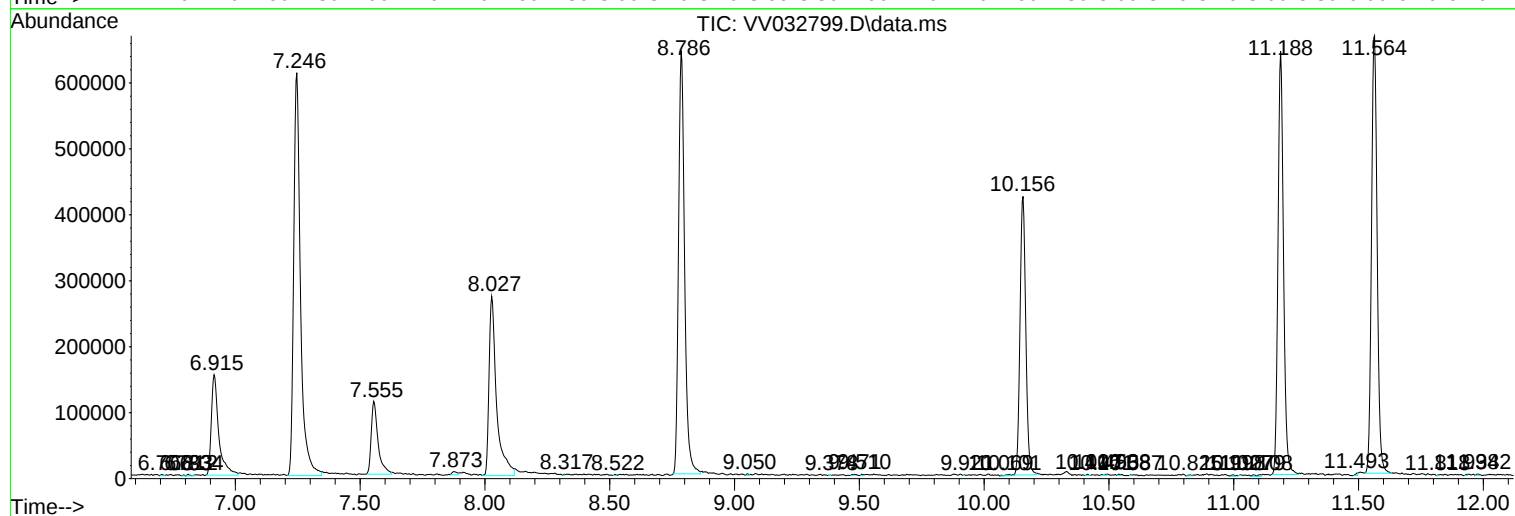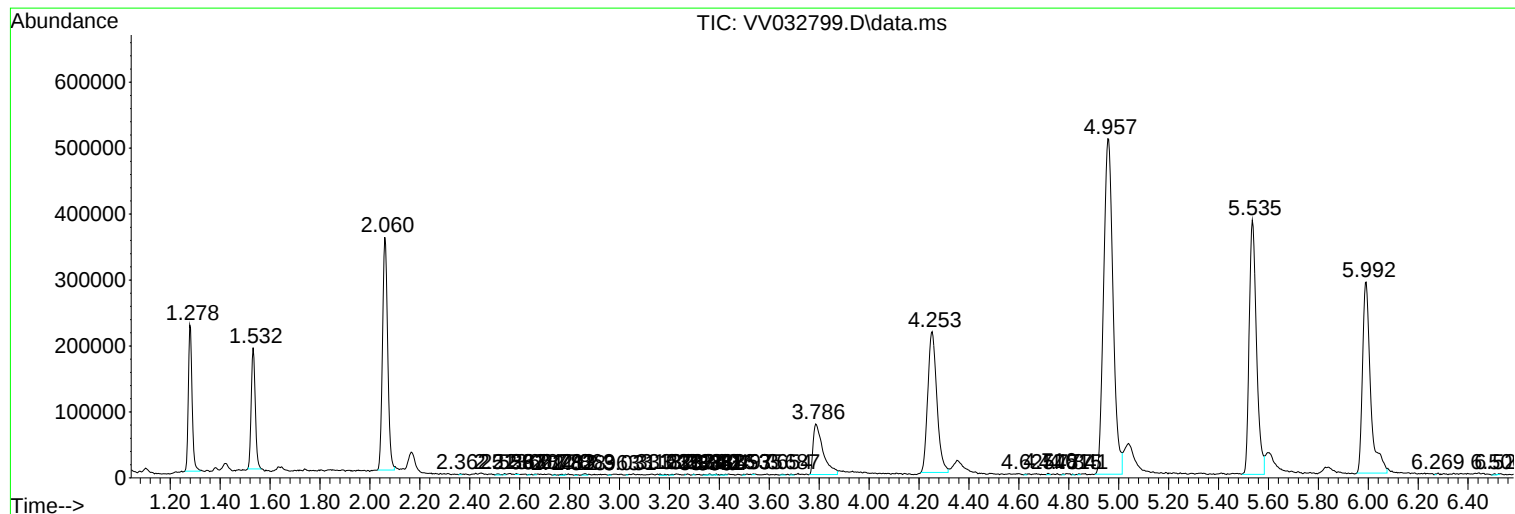

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032799.D
Acq On : 31 Oct 2023 15:27
Operator : SY/MD
Sample : 05105-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0010

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032799.D
Acq On : 31 Oct 2023 15:27
Operator : SY/MD
Sample : 05105-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0010

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc