

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032800.D
 Acq On : 31 Oct 2023 15:51
 Operator : SY/MD
 Sample : 05105-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0011

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032800.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rBV	207911	220017	17.43%	2.122%
2	1.532	146	153	166	rVB	177703	204582	16.21%	1.973%
3	2.060	308	317	334	rBV	337708	492802	39.05%	4.753%
4	2.532	460	464	467	rBV6	1666	1655	0.13%	0.016%
5	2.667	504	506	507	rBV2	1247	483	0.04%	0.005%
6	2.828	554	556	557	rBV2	1635	594	0.05%	0.006%
7	2.931	585	588	593	rBV7	1452	1393	0.11%	0.013%
8	2.953	593	595	597	rBV4	1321	744	0.06%	0.007%
9	2.966	597	599	603	rVB5	1780	1215	0.10%	0.012%
10	3.015	611	614	617	rVB4	1770	1083	0.09%	0.010%
11	3.085	632	636	638	rBV4	1852	1074	0.09%	0.010%
12	3.211	673	675	678	rBV4	1599	925	0.07%	0.009%
13	3.252	683	688	690	rVB6	1533	1280	0.10%	0.012%
14	3.272	690	694	697	rVB7	1859	1407	0.11%	0.014%
15	3.291	697	700	702	rBV4	1631	937	0.07%	0.009%
16	3.420	738	740	746	rBV6	1291	1075	0.09%	0.010%
17	3.503	763	766	768	rBV4	1134	722	0.06%	0.007%
18	3.577	787	789	791	rBV3	1401	788	0.06%	0.008%
19	3.741	836	840	845	rBV8	1322	859	0.07%	0.008%
20	3.789	846	855	883	rBV	74060	204384	16.19%	1.971%
21	4.172	972	974	976	rBV3	1514	694	0.05%	0.007%
22	4.252	985	999	1020	rBV	202267	525406	41.63%	5.068%
23	4.789	1163	1166	1170	rBV7	1752	1659	0.13%	0.016%
24	4.960	1203	1219	1236	rBV2	481580	1262056	100.00%	12.173%
25	5.233	1302	1304	1308	rBV5	1775	1186	0.09%	0.011%
26	5.535	1386	1398	1413	rBV	406643	827397	65.56%	7.981%
27	5.757	1465	1467	1469	rBV4	2173	973	0.08%	0.009%
28	5.992	1529	1540	1553	rBV	274117	562780	44.59%	5.428%
29	6.301	1634	1636	1637	rBV2	1572	508	0.04%	0.005%
30	6.342	1644	1649	1652	rBV6	2332	1928	0.15%	0.019%
31	6.375	1655	1659	1661	rBV6	1542	1000	0.08%	0.010%
32	6.574	1716	1721	1722	rBV5	1456	1010	0.08%	0.010%
33	6.693	1756	1758	1762	rVB5	1721	1175	0.09%	0.011%
34	6.825	1796	1799	1800	rBV2	1274	816	0.06%	0.008%
35	6.915	1817	1827	1852	rBV	141257	290276	23.00%	2.800%
36	7.246	1919	1930	1959	rBV	574139	1083602	85.86%	10.452%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032800.D
 Acq On : 31 Oct 2023 15:51
 Operator : SY/MD
 Sample : 05105-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0011

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	7.555	2017	2026	2043	rBV	105851	199712	15.82%	1.926%
38	7.805	2102	2104	2108	rBV5	1804	827	0.07%	0.008%
39	7.969	2153	2155	2156	rBV2	2793	1334	0.11%	0.013%
40	8.027	2164	2173	2210	rBV	256014	534490	42.35%	5.155%
41	8.735	2391	2393	2395	rVV3	1673	875	0.07%	0.008%
42	8.786	2399	2409	2434	rVV	684181	1165322	92.34%	11.240%
43	9.024	2480	2483	2486	rVB5	2031	1407	0.11%	0.014%
44	9.043	2487	2489	2491	rBV2	2129	1103	0.09%	0.011%
45	9.188	2531	2534	2536	rBV4	1476	1024	0.08%	0.010%
46	9.458	2617	2618	2621	rVV3	995	489	0.04%	0.005%
47	9.641	2673	2675	2677	rBV3	1279	594	0.05%	0.006%
48	9.763	2709	2713	2714	rBV4	1511	829	0.07%	0.008%
49	9.776	2714	2717	2718	rBV3	1621	917	0.07%	0.009%
50	9.825	2729	2732	2735	rBV4	1205	681	0.05%	0.007%
51	9.850	2735	2740	2744	rVB8	1603	1758	0.14%	0.017%
52	9.873	2744	2747	2750	rBV5	1620	1193	0.09%	0.012%
53	10.001	2785	2787	2789	rBV4	1151	474	0.04%	0.005%
54	10.085	2810	2813	2814	rBV3	946	630	0.05%	0.006%
55	10.156	2824	2835	2857	rVB	407743	640708	50.77%	6.180%
56	10.513	2944	2946	2949	rVB4	1431	675	0.05%	0.007%
57	10.561	2957	2961	2963	rVB5	1419	925	0.07%	0.009%
58	10.574	2963	2965	2966	rBV2	1401	498	0.04%	0.005%
59	10.728	3010	3013	3014	rBV3	925	626	0.05%	0.006%
60	10.857	3050	3053	3056	rBV5	2673	2259	0.18%	0.022%
61	10.892	3061	3064	3066	rVV4	1973	1207	0.10%	0.012%
62	10.927	3073	3075	3078	rVB4	2005	837	0.07%	0.008%
63	10.956	3080	3084	3087	rBV5	2134	1760	0.14%	0.017%
64	11.027	3104	3106	3110	rVB5	1725	1058	0.08%	0.010%
65	11.046	3110	3112	3116	rBV4	1446	879	0.07%	0.008%
66	11.107	3128	3131	3133	rBV4	1743	1177	0.09%	0.011%
67	11.188	3145	3156	3179	rBV	670406	1052688	83.41%	10.154%
68	11.513	3253	3257	3260	rBV5	2410	2049	0.16%	0.020%
69	11.564	3261	3273	3293	rVV	626915	1004978	79.63%	9.693%
70	11.905	3377	3379	3383	rVB5	1746	881	0.07%	0.008%
71	11.947	3390	3392	3396	rBV4	1546	1326	0.11%	0.013%
72	12.040	3415	3421	3426	rBV8	2937	3405	0.27%	0.033%
73	12.201	3466	3471	3473	rBV4	2614	2328	0.18%	0.022%
74	12.252	3484	3487	3494	rVB9	1317	1182	0.09%	0.011%
75	12.329	3509	3511	3516	rVB6	1998	1790	0.14%	0.017%
76	12.358	3516	3520	3522	rBV5	1842	1183	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032800.D
 Acq On : 31 Oct 2023 15:51
 Operator : SY/MD
 Sample : 05105-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0011

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.480	3555	3558	3559	rBV3	1202	681	0.05%	0.007%
78	12.529	3571	3573	3577	rBV5	1556	1137	0.09%	0.011%
79	12.667	3614	3616	3618	rBV3	1132	594	0.05%	0.006%
80	12.802	3655	3658	3659	rBV3	1382	860	0.07%	0.008%
81	12.963	3706	3708	3712	rBV5	1071	785	0.06%	0.008%
82	13.053	3732	3736	3738	rBV4	1694	973	0.08%	0.009%
83	13.069	3738	3741	3742	rBV3	1012	560	0.04%	0.005%
84	13.194	3776	3780	3783	rBV5	1854	1705	0.14%	0.016%
85	13.268	3800	3803	3808	rVB6	2579	2021	0.16%	0.019%
86	13.294	3808	3811	3813	rBV4	1234	744	0.06%	0.007%
87	13.394	3837	3842	3847	rBV9	1676	2053	0.16%	0.020%
88	13.419	3847	3850	3851	rBV4	1248	560	0.04%	0.005%
89	13.429	3851	3853	3854	rBV2	1391	558	0.04%	0.005%
90	13.558	3889	3893	3895	rBV5	1769	1353	0.11%	0.013%
91	13.622	3911	3913	3917	rVB5	2113	992	0.08%	0.010%
92	13.821	3972	3975	3977	rBV4	2240	1472	0.12%	0.014%
93	13.850	3982	3984	3987	rVB4	2050	948	0.08%	0.009%
94	13.966	4018	4020	4024	rBV5	1666	1033	0.08%	0.010%
95	14.133	4069	4072	4076	rBV6	1813	1590	0.13%	0.015%
96	14.400	4153	4155	4157	rVB3	1707	632	0.05%	0.006%
97	14.419	4157	4161	4162	rBV4	1800	1331	0.11%	0.013%
98	14.590	4212	4214	4217	rBV4	1398	777	0.06%	0.007%
99	15.075	4358	4365	4369	rBV10	3296	4481	0.36%	0.043%
100	15.223	4408	4411	4412	rBV3	1954	1273	0.10%	0.012%




Sum of corrected areas: 10367676

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032800.D
Acq On : 31 Oct 2023 15:51
Operator : SY/MD
Sample : 05105-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0011

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

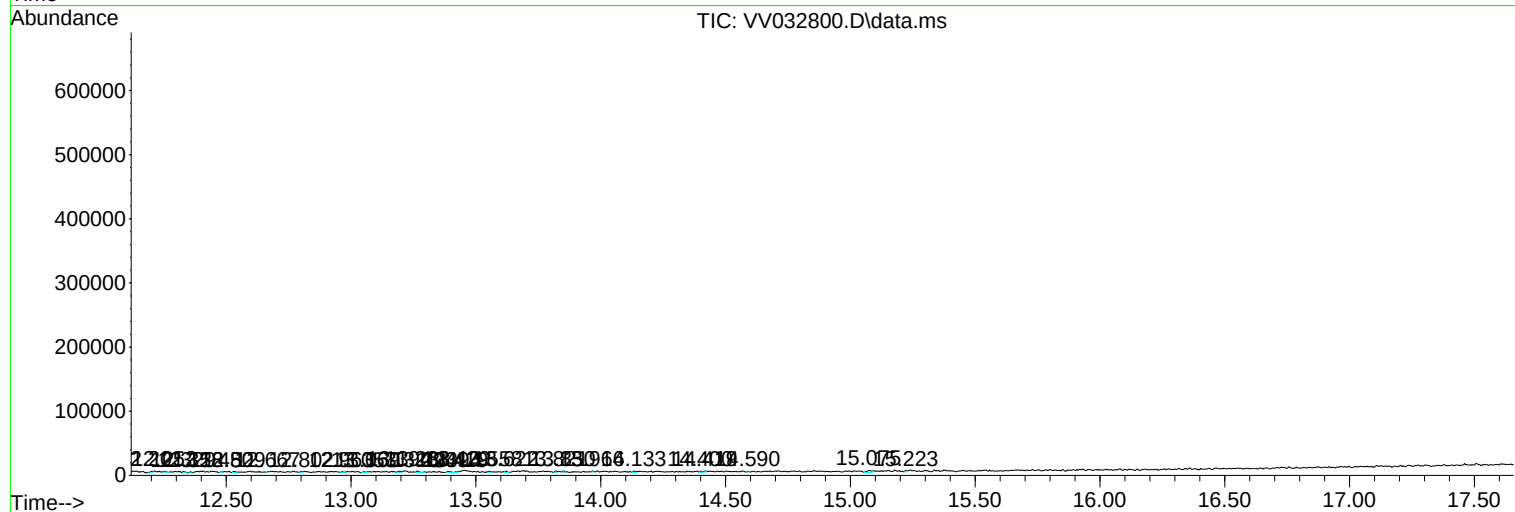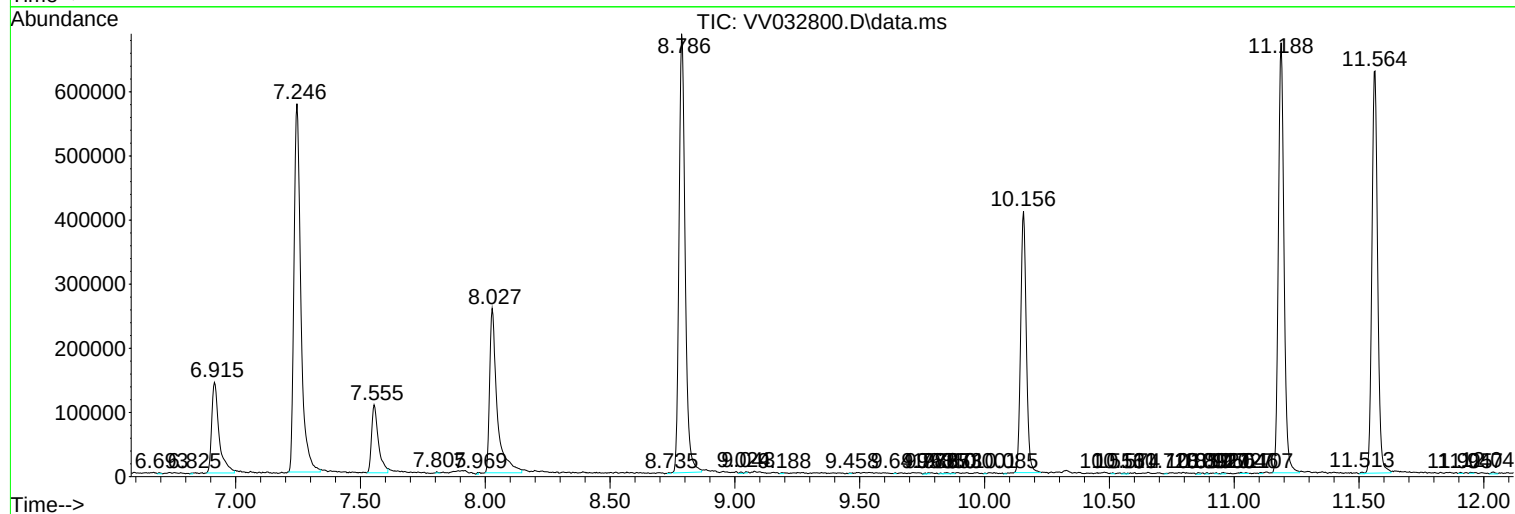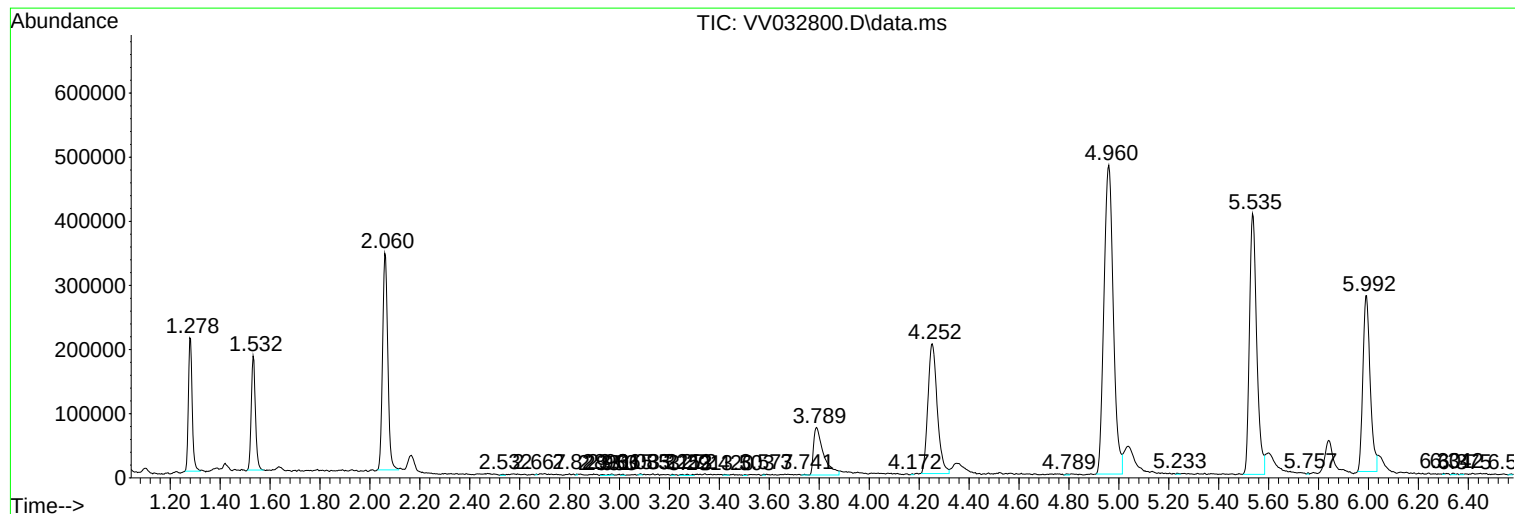

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032800.D
Acq On : 31 Oct 2023 15:51
Operator : SY/MD
Sample : 05105-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0011

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032800.D
Acq On : 31 Oct 2023 15:51
Operator : SY/MD
Sample : 05105-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0011

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------