

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032805.D
 Acq On : 31 Oct 2023 17:48
 Operator : SY/MD
 Sample : 05105-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0006

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032805.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	88	rBV	230896	239432	17.64%	2.168%
2	1.532	146	153	167	rVB	203427	227051	16.72%	2.055%
3	2.060	309	317	334	rVB	356359	510842	37.63%	4.625%
4	2.622	491	492	494	rVB2	737	262	0.02%	0.002%
5	2.635	494	496	497	rBV2	1362	569	0.04%	0.005%
6	2.661	501	504	506	rBV4	2272	1714	0.13%	0.016%
7	2.818	550	553	555	rBV4	1639	1014	0.07%	0.009%
8	2.886	572	574	579	rVB6	1385	805	0.06%	0.007%
9	2.921	583	585	590	rVB6	1531	1020	0.08%	0.009%
10	2.950	591	594	597	rBV5	1374	1089	0.08%	0.010%
11	3.056	623	627	629	rBV4	1396	1048	0.08%	0.009%
12	3.162	658	660	663	rVB4	1585	640	0.05%	0.006%
13	3.208	672	674	677	rBV3	1255	828	0.06%	0.007%
14	3.233	680	682	684	rBV3	1026	536	0.04%	0.005%
15	3.269	690	693	695	rBV3	1169	777	0.06%	0.007%
16	3.314	704	707	709	rBV4	1166	652	0.05%	0.006%
17	3.343	714	716	717	rBV3	889	345	0.03%	0.003%
18	3.352	717	719	721	rBV3	1068	413	0.03%	0.004%
19	3.397	731	733	735	rBV2	1871	1013	0.07%	0.009%
20	3.439	744	746	751	rVB5	2379	1534	0.11%	0.014%
21	3.462	751	753	755	rBV2	1060	616	0.05%	0.006%
22	3.474	755	757	758	rBV2	1263	631	0.05%	0.006%
23	3.523	770	772	774	rBV3	1438	891	0.07%	0.008%
24	3.558	781	783	785	rBV3	999	325	0.02%	0.003%
25	3.606	796	798	799	rBV2	913	329	0.02%	0.003%
26	3.632	803	806	807	rBV4	1002	536	0.04%	0.005%
27	3.690	823	824	827	rVB2	1144	586	0.04%	0.005%
28	3.712	829	831	832	rBV2	1378	720	0.05%	0.007%
29	3.789	842	855	880	rBV	82706	229302	16.89%	2.076%
30	4.252	985	999	1021	rBV	216588	558073	41.11%	5.052%
31	4.609	1108	1110	1111	rBV2	1491	544	0.04%	0.005%
32	4.687	1132	1134	1138	rVB4	2290	1566	0.12%	0.014%
33	4.709	1138	1141	1142	rBV3	1813	893	0.07%	0.008%
34	4.770	1158	1160	1161	rBV2	1528	707	0.05%	0.006%
35	4.809	1170	1172	1173	rBV2	1279	458	0.03%	0.004%
36	4.851	1183	1185	1188	rBV4	1318	647	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032805.D
 Acq On : 31 Oct 2023 17:48
 Operator : SY/MD
 Sample : 05105-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0006

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	4.896	1196	1199	1200	rBV3	1953	1123	0.08%	0.010%
38	4.957	1203	1218	1235	rBV2	518770	1357579	100.00%	12.290%
39	5.535	1387	1398	1413	rBV	391981	802626	59.12%	7.266%
40	5.989	1527	1539	1571	rBV	292048	686314	50.55%	6.213%
41	6.503	1696	1699	1700	rBV3	1592	995	0.07%	0.009%
42	6.577	1720	1722	1725	rVB4	1985	1011	0.07%	0.009%
43	6.658	1745	1747	1751	rBV5	1632	1011	0.07%	0.009%
44	6.748	1773	1775	1777	rBV3	2143	906	0.07%	0.008%
45	6.915	1818	1827	1857	rBV	154766	315736	23.26%	2.858%
46	7.246	1918	1930	1967	rBV	630863	1205405	88.79%	10.912%
47	7.555	2018	2026	2049	rBV	114963	211478	15.58%	1.914%
48	8.027	2164	2173	2202	rBV	298031	592384	43.64%	5.363%
49	8.397	2286	2288	2292	rBV5	1619	965	0.07%	0.009%
50	8.574	2341	2343	2346	rBV4	1783	764	0.06%	0.007%
51	8.690	2377	2379	2380	rBV2	1197	307	0.02%	0.003%
52	8.786	2399	2409	2436	rBV	667766	1148515	84.60%	10.397%
53	9.252	2551	2554	2557	rBV5	1644	1547	0.11%	0.014%
54	9.776	2714	2717	2719	rBV2	1962	1109	0.08%	0.010%
55	9.931	2763	2765	2767	rBV3	1689	1006	0.07%	0.009%
56	10.021	2791	2793	2798	rVB5	1431	898	0.07%	0.008%
57	10.156	2823	2835	2849	rBV	445537	710626	52.35%	6.433%
58	10.474	2930	2934	2935	rBV3	1640	1171	0.09%	0.011%
59	10.773	3024	3027	3028	rBV3	1388	929	0.07%	0.008%
60	10.841	3045	3048	3049	rBV3	2333	1118	0.08%	0.010%
61	10.924	3070	3074	3078	rVB6	2169	1791	0.13%	0.016%
62	10.947	3079	3081	3083	rBV3	1332	760	0.06%	0.007%
63	11.091	3123	3126	3127	rBV3	964	491	0.04%	0.004%
64	11.114	3130	3133	3135	rBV4	2068	1277	0.09%	0.012%
65	11.127	3135	3137	3138	rBV	1851	771	0.06%	0.007%
66	11.188	3144	3156	3173	rBV	687914	1076236	79.28%	9.743%
67	11.455	3237	3239	3242	rBV3	2070	990	0.07%	0.009%
68	11.564	3261	3273	3293	rBV	705407	1109667	81.74%	10.045%
69	12.104	3437	3441	3442	rBV4	1225	818	0.06%	0.007%
70	12.181	3463	3465	3467	rBV3	2310	1291	0.10%	0.012%
71	12.226	3477	3479	3481	rBV3	1431	674	0.05%	0.006%
72	12.320	3506	3508	3509	rBV2	1256	625	0.05%	0.006%
73	12.570	3585	3586	3587	rBV	1360	471	0.03%	0.004%
74	12.812	3659	3661	3663	rBV4	1130	615	0.05%	0.006%
75	12.853	3672	3674	3675	rBV2	1239	383	0.03%	0.003%
76	12.915	3687	3693	3695	rBV6	2245	2385	0.18%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032805.D
 Acq On : 31 Oct 2023 17:48
 Operator : SY/MD
 Sample : 05105-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0006

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M

Title : VOC Analysis

77	13.124	3756	3758	3761	rVB3	993	406	0.03%	0.004%
78	13.275	3800	3805	3807	rBV6	2553	2532	0.19%	0.023%
79	13.329	3820	3822	3824	rBV2	1415	955	0.07%	0.009%
80	13.545	3887	3889	3892	rBV4	1460	926	0.07%	0.008%
81	13.587	3900	3902	3905	rBV4	1401	626	0.05%	0.006%
82	13.808	3967	3971	3976	rBV8	2536	2697	0.20%	0.024%
83	14.088	4056	4058	4059	rBV2	1998	591	0.04%	0.005%
84	14.622	4220	4224	4228	rBV7	2664	2539	0.19%	0.023%
85	15.564	4514	4517	4519	rBV3	2641	1963	0.14%	0.018%




Sum of corrected areas: 11046411

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032805.D
Acq On : 31 Oct 2023 17:48
Operator : SY/MD
Sample : 05105-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0006

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

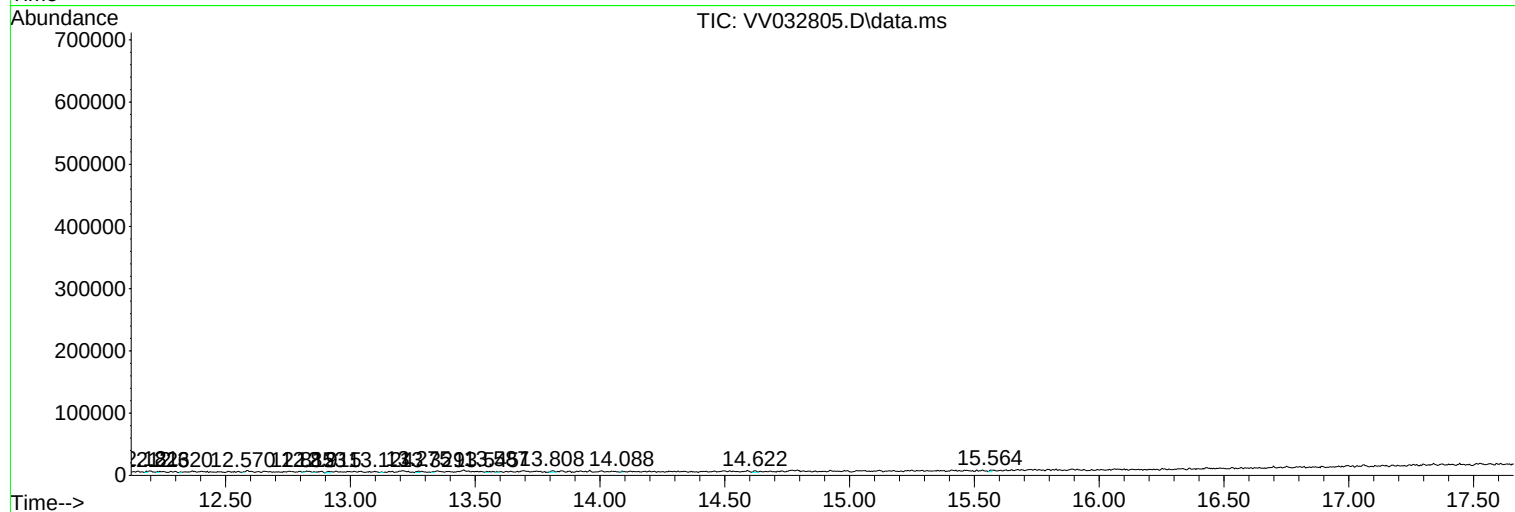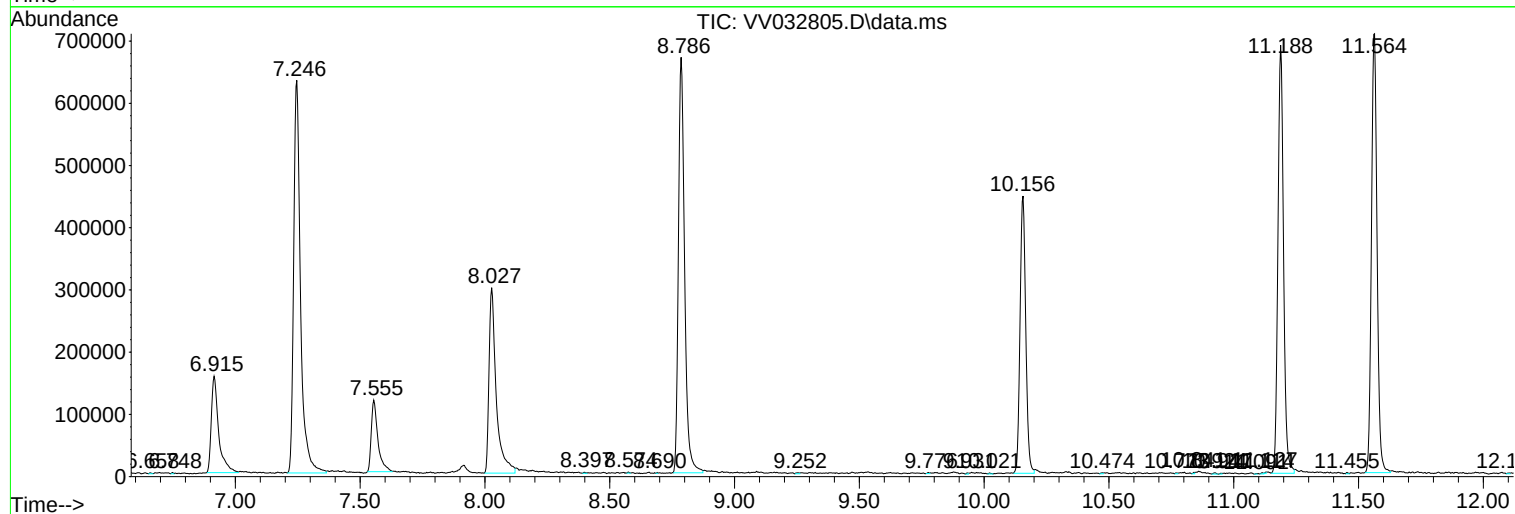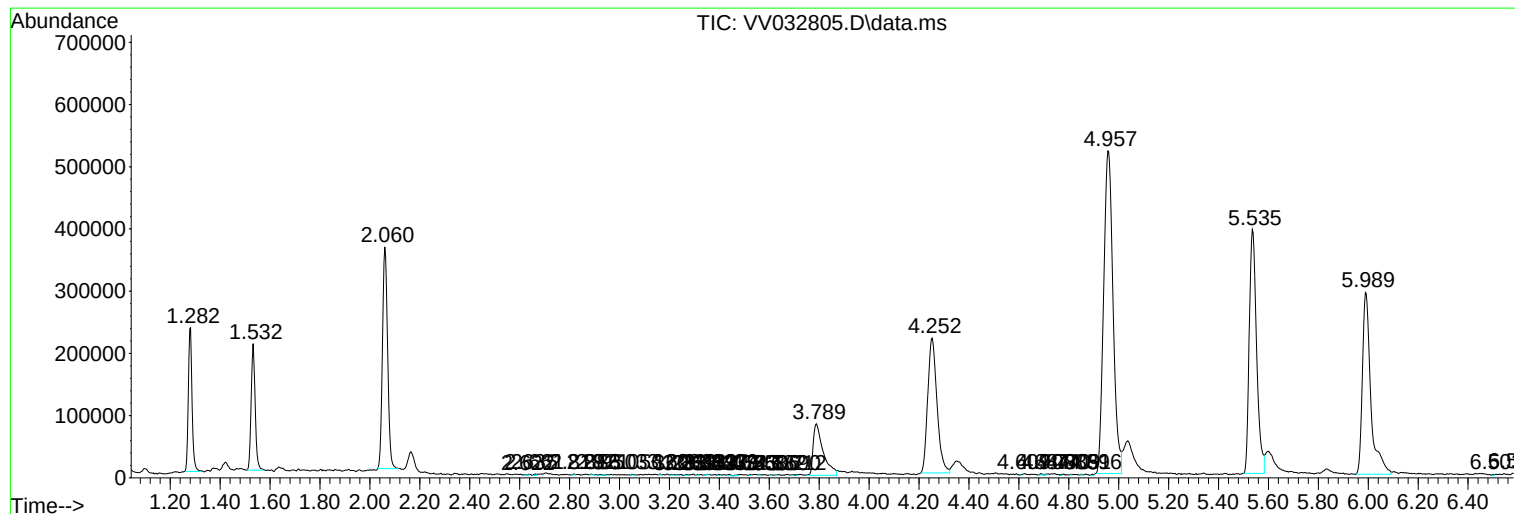

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032805.D
Acq On : 31 Oct 2023 17:48
Operator : SY/MD
Sample : 05105-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0006

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032805.D
Acq On : 31 Oct 2023 17:48
Operator : SY/MD
Sample : 05105-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0006

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------