

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032807.D
 Acq On : 31 Oct 2023 18:35
 Operator : SY/MD
 Sample : 05105-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0012

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032807.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	51	55	56	rBV4	2779	1977	0.15%	0.017%
2	1.278	68	74	89	rBV	216704	231692	17.16%	2.038%
3	1.532	146	153	163	rBV	188214	212979	15.77%	1.874%
4	2.060	308	317	331	rBV	352694	508940	37.69%	4.477%
5	2.310	393	395	400	rVV6	2446	1498	0.11%	0.013%
6	2.330	400	401	405	rVB4	1475	821	0.06%	0.007%
7	2.404	421	424	425	rBV3	1252	809	0.06%	0.007%
8	2.487	448	450	457	rVB8	2575	2374	0.18%	0.021%
9	2.513	457	458	460	rBV2	1409	757	0.06%	0.007%
10	2.616	488	490	492	rBV3	1231	543	0.04%	0.005%
11	2.706	515	518	519	rBV2	1064	488	0.04%	0.004%
12	2.886	573	574	575	rBV	1569	531	0.04%	0.005%
13	2.912	580	582	584	rBV3	1128	586	0.04%	0.005%
14	2.963	596	598	602	rBV6	1319	941	0.07%	0.008%
15	3.133	650	651	656	rVB5	1388	976	0.07%	0.009%
16	3.182	664	666	668	rBV2	856	596	0.04%	0.005%
17	3.269	691	693	696	rBV2	1582	852	0.06%	0.007%
18	3.285	696	698	699	rVB2	1679	557	0.04%	0.005%
19	3.301	701	703	705	rBV3	1210	526	0.04%	0.005%
20	3.346	715	717	718	rBV2	1163	553	0.04%	0.005%
21	3.436	743	745	747	rBV3	961	495	0.04%	0.004%
22	3.494	761	763	766	rVV4	1374	941	0.07%	0.008%
23	3.548	779	780	783	rBV3	1090	679	0.05%	0.006%
24	3.606	794	798	800	rBV5	1309	1229	0.09%	0.011%
25	3.683	814	822	825	rBV9	2344	2877	0.21%	0.025%
26	3.703	825	828	830	rVV3	1170	634	0.05%	0.006%
27	3.754	837	844	845	rBV6	2252	1978	0.15%	0.017%
28	3.786	847	854	873	rBV	76254	186904	13.84%	1.644%
29	4.252	985	999	1020	rBV	214966	550962	40.81%	4.847%
30	4.770	1158	1160	1163	rVB4	2044	953	0.07%	0.008%
31	4.960	1200	1219	1235	rBV2	518867	1350222	100.00%	11.878%
32	5.535	1387	1398	1413	rBV	403481	821859	60.87%	7.230%
33	5.834	1480	1491	1506	rBV	240336	496975	36.81%	4.372%
34	5.989	1529	1539	1570	rVB	290776	650988	48.21%	5.727%
35	6.532	1704	1708	1711	rBV6	1663	1404	0.10%	0.012%
36	6.680	1752	1754	1756	rBV3	1166	703	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW103123\
 Data File : VW032807.D
 Acq On : 31 Oct 2023 18:35
 Operator : SY/MD
 Sample : 05105-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0012

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.754	1773	1777	1779	rBV4	1975	1197	0.09%	0.011%
38	6.915	1817	1827	1851	rBV	154579	312530	23.15%	2.749%
39	7.246	1919	1930	1965	rBV	612642	1171089	86.73%	10.302%
40	7.555	2017	2026	2049	rBV2	109058	212753	15.76%	1.872%
41	7.828	2109	2111	2113	rBV3	1856	1104	0.08%	0.010%
42	8.027	2164	2173	2202	rBV	278319	568484	42.10%	5.001%
43	8.693	2376	2380	2381	rBV3	1250	623	0.05%	0.005%
44	8.718	2386	2388	2391	rBV4	1653	648	0.05%	0.006%
45	8.786	2399	2409	2437	rBV	688979	1156195	85.63%	10.171%
46	9.259	2555	2556	2558	rBV2	1123	509	0.04%	0.004%
47	9.429	2607	2609	2612	rVB4	1570	825	0.06%	0.007%
48	9.529	2639	2640	2644	rVB4	1559	712	0.05%	0.006%
49	9.548	2644	2646	2651	rVB6	1554	1374	0.10%	0.012%
50	9.571	2651	2653	2657	rBV4	1595	1061	0.08%	0.009%
51	9.628	2668	2671	2674	rBV4	1526	1051	0.08%	0.009%
52	9.718	2696	2699	2704	rVB7	2174	2024	0.15%	0.018%
53	9.747	2704	2708	2709	rBV3	2018	1269	0.09%	0.011%
54	9.815	2726	2729	2731	rVB3	1143	606	0.04%	0.005%
55	9.828	2731	2733	2736	rBV4	1073	737	0.05%	0.006%
56	9.898	2753	2755	2758	rBV4	2079	1017	0.08%	0.009%
57	9.921	2758	2762	2764	rBV5	2511	1598	0.12%	0.014%
58	10.021	2790	2793	2794	rBV3	1337	782	0.06%	0.007%
59	10.156	2824	2835	2856	rBV	437226	686581	50.85%	6.040%
60	10.255	2862	2866	2870	rBV7	2338	2188	0.16%	0.019%
61	10.384	2902	2906	2909	rBV6	1781	1423	0.11%	0.013%
62	10.458	2927	2929	2934	rVB5	1781	1516	0.11%	0.013%
63	10.529	2948	2951	2954	rBV5	1762	1347	0.10%	0.012%
64	10.599	2971	2973	2975	rBV3	2103	1217	0.09%	0.011%
65	10.654	2986	2990	2992	rBV5	1324	1059	0.08%	0.009%
66	10.783	3026	3030	3032	rBV4	2786	1705	0.13%	0.015%
67	10.844	3046	3049	3050	rBV2	1811	869	0.06%	0.008%
68	10.886	3061	3062	3067	rVB3	1424	901	0.07%	0.008%
69	10.915	3067	3071	3074	rVB6	1858	1240	0.09%	0.011%
70	10.995	3092	3096	3099	rBV6	1098	991	0.07%	0.009%
71	11.056	3113	3115	3116	rBV2	1549	638	0.05%	0.006%
72	11.127	3134	3137	3141	rBV6	1958	2006	0.15%	0.018%
73	11.188	3145	3156	3175	rBV	707905	1085449	80.39%	9.549%
74	11.561	3262	3272	3288	rBV	684190	1073906	79.54%	9.447%
75	11.821	3350	3353	3354	rBV2	1879	855	0.06%	0.008%
76	12.287	3494	3498	3501	rBV6	2263	2048	0.15%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032807.D
 Acq On : 31 Oct 2023 18:35
 Operator : SY/MD
 Sample : 05105-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0012

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.313	3504	3506	3508	rVB2	1324	572	0.04%	0.005%
78	12.329	3508	3511	3512	rBV3	1671	1020	0.08%	0.009%
79	12.374	3523	3525	3527	rBV3	1450	787	0.06%	0.007%
80	12.577	3586	3588	3590	rBV3	2078	1034	0.08%	0.009%
81	12.593	3591	3593	3595	rVV3	1525	659	0.05%	0.006%
82	12.725	3632	3634	3636	rBV3	995	477	0.04%	0.004%
83	12.750	3640	3642	3645	rVB4	1477	749	0.06%	0.007%
84	12.795	3654	3656	3658	rBV3	984	478	0.04%	0.004%
85	12.850	3672	3673	3678	rVB5	1776	1125	0.08%	0.010%
86	12.959	3703	3707	3708	rBV4	1395	684	0.05%	0.006%
87	13.323	3818	3820	3822	rBV3	1125	615	0.05%	0.005%
88	13.365	3831	3833	3836	rVB4	1811	1032	0.08%	0.009%
89	13.445	3855	3858	3860	rBV3	2270	1839	0.14%	0.016%
90	13.512	3877	3879	3882	rBV4	1343	672	0.05%	0.006%
91	13.766	3955	3958	3962	rBV5	1680	1543	0.11%	0.014%
92	13.895	3996	3998	4004	rVB6	1744	1511	0.11%	0.013%
93	13.943	4011	4013	4016	rVB4	1538	809	0.06%	0.007%
94	13.963	4016	4019	4023	rVB6	1494	1158	0.09%	0.010%
95	13.998	4026	4030	4031	rBV4	1345	1088	0.08%	0.010%
96	14.168	4081	4083	4087	rBV4	1433	888	0.07%	0.008%
97	14.236	4101	4104	4108	rVB6	1926	1426	0.11%	0.013%
98	14.303	4123	4125	4129	rBV5	1737	1655	0.12%	0.015%
99	14.484	4179	4181	4185	rBV5	2006	1621	0.12%	0.014%
100	15.056	4357	4359	4362	rBV4	2049	1330	0.10%	0.012%




Sum of corrected areas: 11367698

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032807.D
Acq On : 31 Oct 2023 18:35
Operator : SY/MD
Sample : 05105-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0012

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

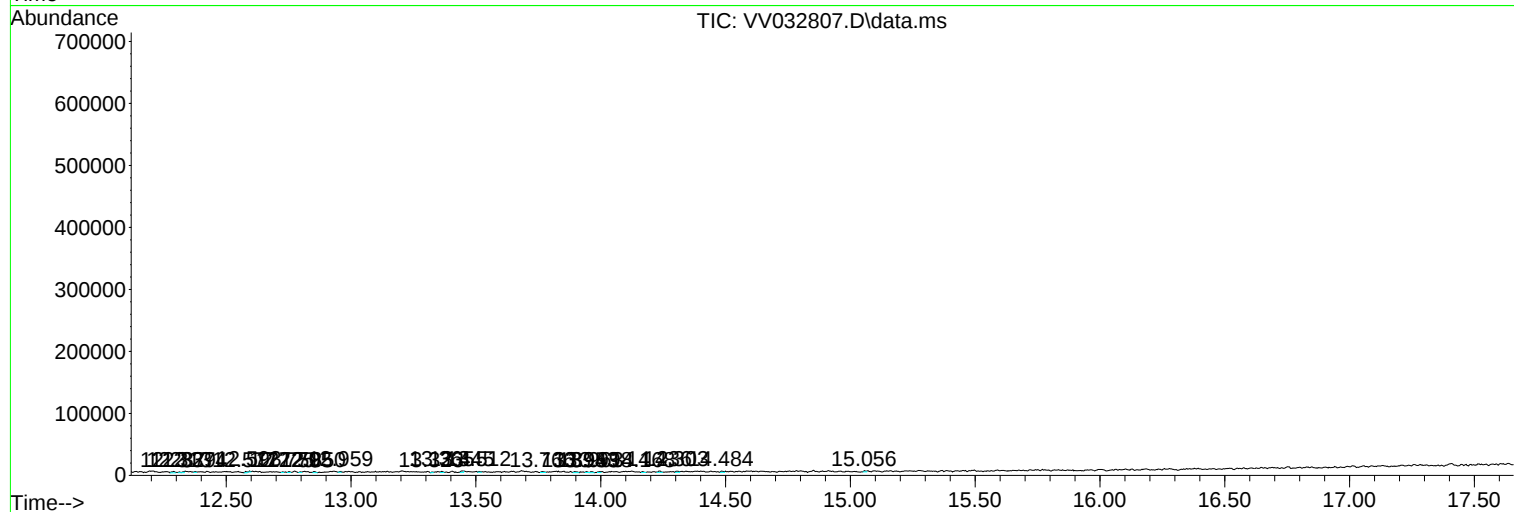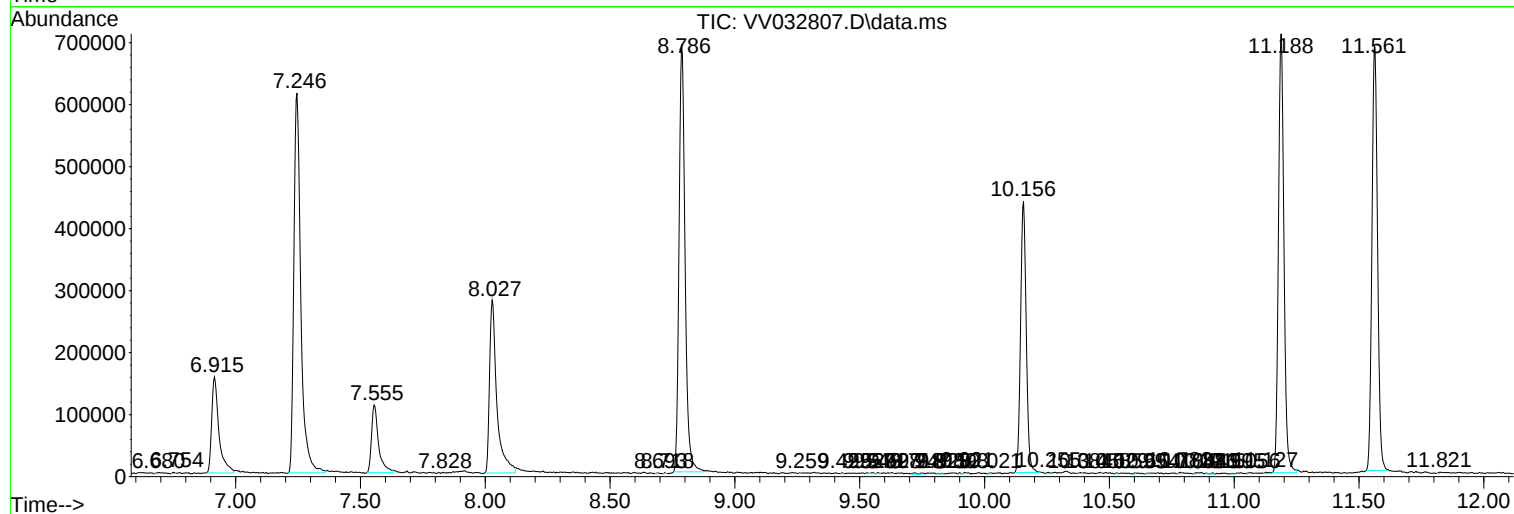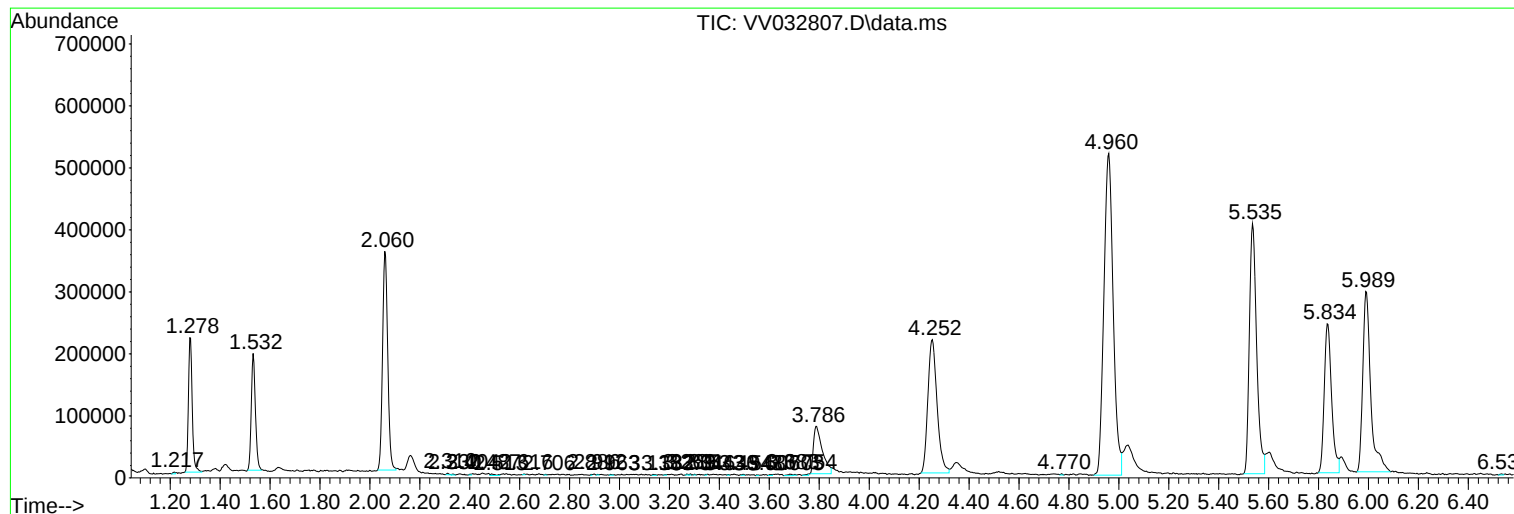

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032807.D
Acq On : 31 Oct 2023 18:35
Operator : SY/MD
Sample : 05105-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0012

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032807.D
Acq On : 31 Oct 2023 18:35
Operator : SY/MD
Sample : 05105-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0012

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------