

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032808.D
 Acq On : 31 Oct 2023 18:58
 Operator : SY/MD
 Sample : 05105-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032808.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	91	rVB	221036	229509	17.07%	2.040%
2	1.532	146	153	167	rVB	185846	215602	16.03%	1.917%
3	2.060	309	317	331	rVB	348522	493792	36.72%	4.390%
4	2.474	443	446	448	rBV4	1366	909	0.07%	0.008%
5	2.645	497	499	500	rBV2	1270	653	0.05%	0.006%
6	2.735	525	527	530	rBV4	904	284	0.02%	0.003%
7	2.806	545	549	551	rBV5	2037	1807	0.13%	0.016%
8	2.883	571	573	575	rBV3	928	237	0.02%	0.002%
9	3.015	612	614	617	rVB4	1534	608	0.05%	0.005%
10	3.031	617	619	624	rBV5	1736	1561	0.12%	0.014%
11	3.333	709	713	716	rBV6	2221	1890	0.14%	0.017%
12	3.404	734	735	738	rBV3	1200	468	0.03%	0.004%
13	3.468	753	755	757	rVB3	904	348	0.03%	0.003%
14	3.513	767	769	772	rBV4	1234	782	0.06%	0.007%
15	3.587	788	792	796	rBV7	1072	1089	0.08%	0.010%
16	3.603	796	797	801	rVB4	1000	434	0.03%	0.004%
17	3.677	817	820	822	rBV4	1928	1369	0.10%	0.012%
18	3.719	831	833	837	rVB3	1721	990	0.07%	0.009%
19	3.790	845	855	883	rBV	77787	222037	16.51%	1.974%
20	4.143	962	965	968	rBV4	1891	1673	0.12%	0.015%
21	4.253	985	999	1018	rBV	213159	550305	40.93%	4.892%
22	4.677	1128	1131	1132	rBV4	1452	973	0.07%	0.009%
23	4.841	1180	1182	1183	rBV2	1474	389	0.03%	0.003%
24	4.867	1188	1190	1194	rVB5	1971	1250	0.09%	0.011%
25	4.889	1194	1197	1199	rBV5	1318	910	0.07%	0.008%
26	4.960	1203	1219	1235	rBV2	510256	1344634	100.00%	11.954%
27	5.535	1387	1398	1412	rBV	397121	806444	59.97%	7.169%
28	5.834	1481	1491	1504	rBV	231591	467279	34.75%	4.154%
29	5.989	1528	1539	1570	rBV	292908	652110	48.50%	5.797%
30	6.696	1757	1759	1761	rBV3	1438	805	0.06%	0.007%
31	6.915	1818	1827	1854	rBV	152140	307219	22.85%	2.731%
32	7.246	1920	1930	1959	rBV	616922	1133978	84.33%	10.081%
33	7.555	2018	2026	2048	rBV	110988	210273	15.64%	1.869%
34	7.873	2121	2125	2127	rBV5	3540	2665	0.20%	0.024%
35	8.027	2164	2173	2205	rBV	276710	571562	42.51%	5.081%
36	8.786	2398	2409	2430	rBV	681127	1152346	85.70%	10.244%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032808.D
 Acq On : 31 Oct 2023 18:58
 Operator : SY/MD
 Sample : 05105-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0013

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	9.256	2553	2555	2558	rBV4	1941	1359	0.10%	0.012%
38	9.397	2596	2599	2602	rBV4	2217	1463	0.11%	0.013%
39	9.413	2602	2604	2606	rBV3	1905	940	0.07%	0.008%
40	9.638	2671	2674	2678	rBV6	1824	1462	0.11%	0.013%
41	9.657	2678	2680	2681	rBV2	1261	464	0.03%	0.004%
42	9.747	2706	2708	2711	rBV4	1375	736	0.05%	0.007%
43	9.793	2721	2722	2726	rBV4	1430	777	0.06%	0.007%
44	9.812	2726	2728	2730	rBV3	1491	732	0.05%	0.007%
45	9.976	2776	2779	2782	rVB4	2156	1473	0.11%	0.013%
46	9.998	2782	2786	2788	rBV4	1723	1244	0.09%	0.011%
47	10.156	2824	2835	2850	rBV	425243	684998	50.94%	6.090%
48	10.458	2927	2929	2931	rBV3	2069	919	0.07%	0.008%
49	10.471	2931	2933	2934	rBV2	1171	357	0.03%	0.003%
50	10.497	2938	2941	2942	rBV3	1503	728	0.05%	0.006%
51	10.593	2968	2971	2974	rBV5	780	482	0.04%	0.004%
52	10.622	2978	2980	2982	rBV3	1423	581	0.04%	0.005%
53	10.693	2995	3002	3004	rBV9	2347	2443	0.18%	0.022%
54	10.809	3036	3038	3040	rBV3	1642	794	0.06%	0.007%
55	11.130	3135	3138	3139	rBV3	1504	731	0.05%	0.006%
56	11.188	3145	3156	3176	rBV	691356	1073008	79.80%	9.539%
57	11.564	3262	3273	3291	rBV	671617	1076224	80.04%	9.567%
58	12.101	3438	3440	3442	rBV3	992	494	0.04%	0.004%
59	12.146	3451	3454	3456	rBV4	1821	1250	0.09%	0.011%
60	12.239	3481	3483	3487	rBV5	1454	1064	0.08%	0.009%
61	12.281	3495	3496	3497	rBV	1046	298	0.02%	0.003%
62	12.329	3509	3511	3515	rBV5	1866	1339	0.10%	0.012%
63	12.368	3522	3523	3524	rBV	1138	398	0.03%	0.004%
64	12.477	3556	3557	3559	rVB2	1428	433	0.03%	0.004%
65	12.532	3572	3574	3576	rVB3	2209	911	0.07%	0.008%
66	12.635	3604	3606	3608	rBV4	1210	513	0.04%	0.005%
67	12.661	3612	3614	3618	rBV5	1783	1499	0.11%	0.013%
68	12.696	3623	3625	3626	rVB2	1231	313	0.02%	0.003%
69	12.706	3626	3628	3630	rBV3	1433	690	0.05%	0.006%
70	12.931	3696	3698	3700	rBV3	1331	625	0.05%	0.006%
71	12.992	3713	3717	3721	rBV6	1952	1495	0.11%	0.013%
72	13.088	3745	3747	3749	rBV3	2075	1220	0.09%	0.011%
73	13.198	3778	3781	3782	rBV3	1776	922	0.07%	0.008%
74	13.734	3943	3948	3949	rBV5	1585	1219	0.09%	0.011%
75	13.760	3954	3956	3958	rVV2	1517	604	0.04%	0.005%
76	13.837	3976	3980	3983	rBV5	2256	1783	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032808.D
Acq On : 31 Oct 2023 18:58
Operator : SY/MD
Sample : 05105-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0013

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Title : VOC Analysis

77	14.053	4045	4047	4049	rVB2	1685	622	0.05%	0.006%
----	--------	------	------	------	------	------	-----	-------	--------




Sum of corrected areas: 11248791

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032808.D
Acq On : 31 Oct 2023 18:58
Operator : SY/MD
Sample : 05105-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

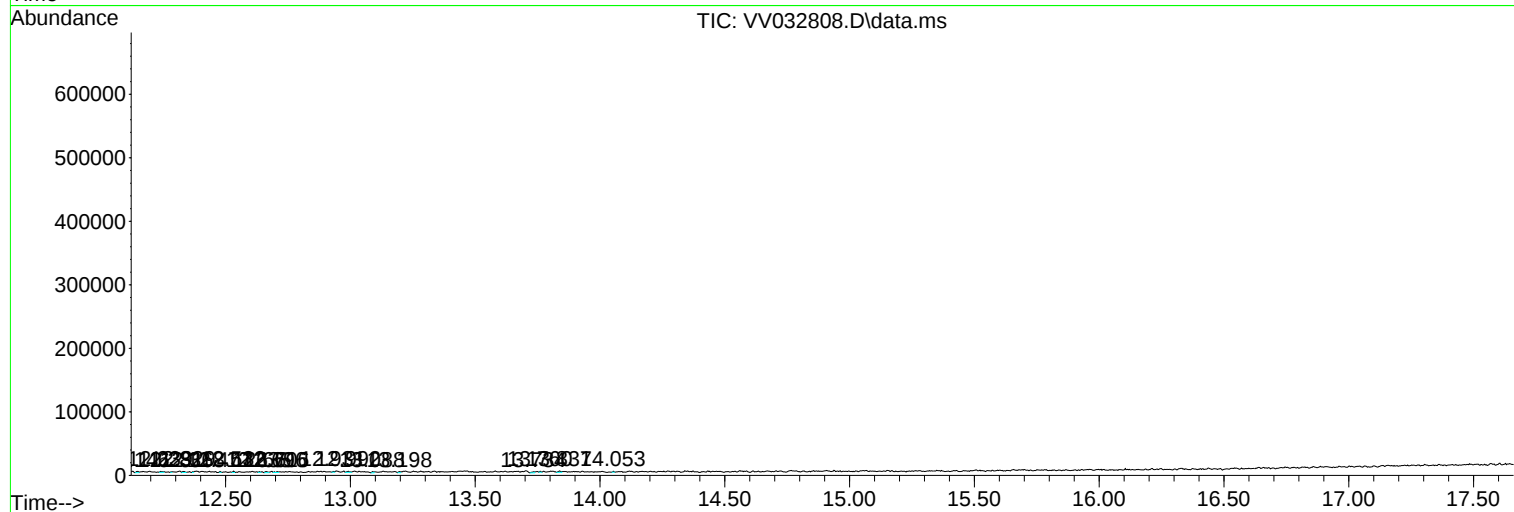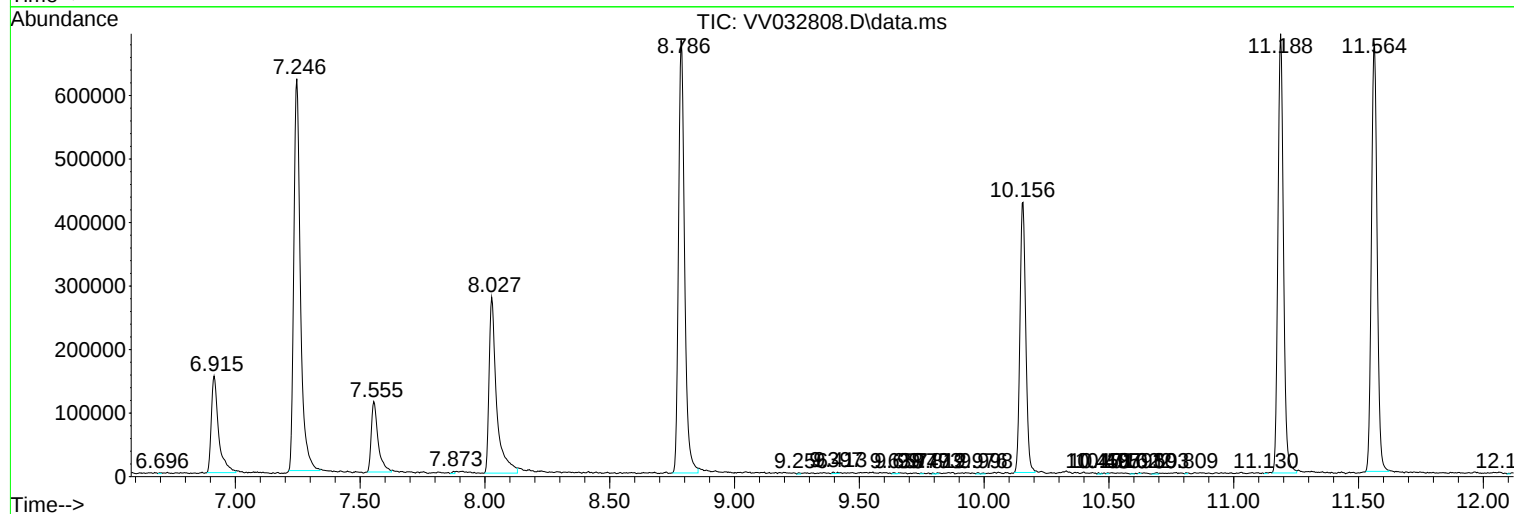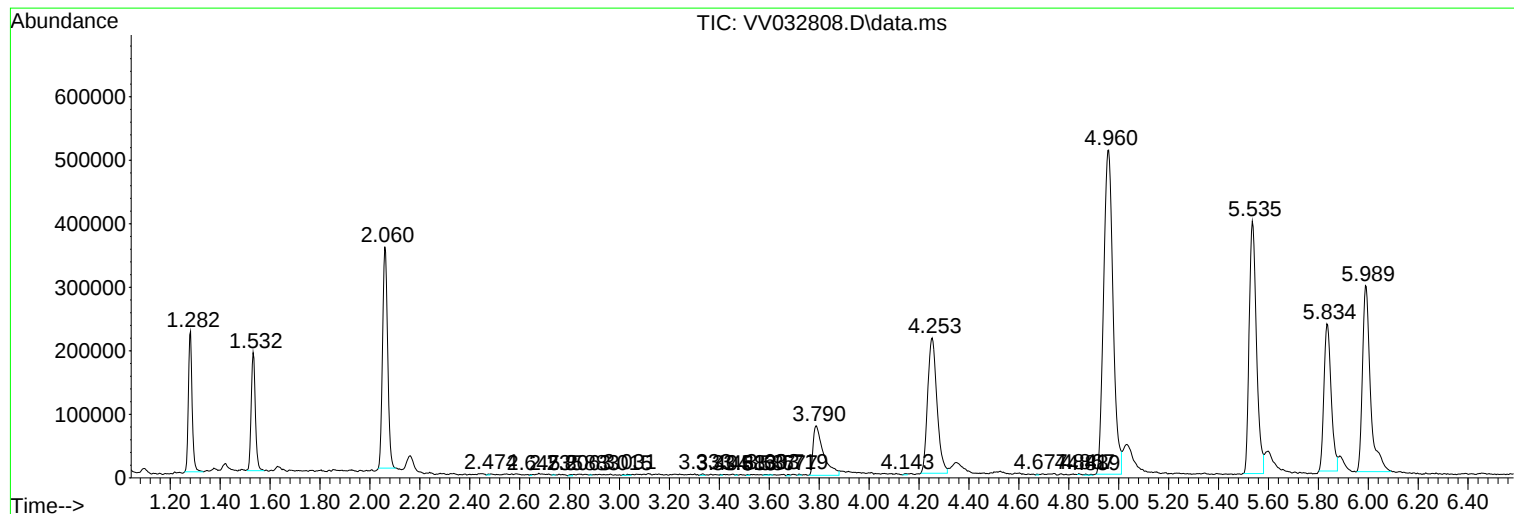

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032808.D
Acq On : 31 Oct 2023 18:58
Operator : SY/MD
Sample : 05105-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032808.D
Acq On : 31 Oct 2023 18:58
Operator : SY/MD
Sample : 05105-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0013

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------