

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032809.D
 Acq On : 31 Oct 2023 19:22
 Operator : SY/MD
 Sample : 05132-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5Q5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M

Title : VOC Analysis

Signal : TIC: VV032809.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.089	11	15	25	rVB2	13784	17668	1.30%	0.161%
2	1.278	68	74	86	rBV	219823	233137	17.10%	2.127%
3	1.532	147	153	165	rVB	188477	219149	16.07%	1.999%
4	2.060	309	317	329	rBV	351214	498978	36.59%	4.552%
5	2.343	403	405	407	rBV3	1145	425	0.03%	0.004%
6	2.606	485	487	488	rBV2	1127	418	0.03%	0.004%
7	2.680	505	510	511	rBV3	936	810	0.06%	0.007%
8	2.690	511	513	514	rBV2	1866	750	0.05%	0.007%
9	2.732	524	526	529	rBV4	1163	879	0.06%	0.008%
10	2.796	544	546	548	rBV3	806	441	0.03%	0.004%
11	2.892	572	576	577	rBV3	1221	874	0.06%	0.008%
12	2.976	598	602	603	rBV3	1165	608	0.04%	0.006%
13	3.015	609	614	615	rBV5	1299	955	0.07%	0.009%
14	3.056	625	627	629	rVB3	1685	692	0.05%	0.006%
15	3.072	629	632	636	rBV5	2343	2084	0.15%	0.019%
16	3.130	647	650	651	rBV3	2475	1550	0.11%	0.014%
17	3.230	678	681	684	rBV4	1655	1040	0.08%	0.009%
18	3.304	700	704	707	rBV7	1795	1539	0.11%	0.014%
19	3.352	717	719	720	rBV2	1098	500	0.04%	0.005%
20	3.362	720	722	724	rVB4	1400	541	0.04%	0.005%
21	3.371	724	725	726	rBV	993	348	0.03%	0.003%
22	3.433	742	744	746	rVB2	1370	486	0.04%	0.004%
23	3.465	753	754	755	rBV	990	300	0.02%	0.003%
24	3.539	772	777	779	rBV6	2865	2235	0.16%	0.020%
25	3.577	785	789	791	rVB4	1964	1411	0.10%	0.013%
26	3.600	793	796	798	rVV4	1311	740	0.05%	0.007%
27	3.613	798	800	802	rVB3	1266	534	0.04%	0.005%
28	3.648	810	811	813	rBV3	567	225	0.02%	0.002%
29	3.661	813	815	816	rVV2	1231	423	0.03%	0.004%
30	3.683	820	822	824	rVB3	2172	713	0.05%	0.007%
31	3.696	824	826	828	rBV3	1119	600	0.04%	0.005%
32	3.732	835	837	838	rBV3	660	236	0.02%	0.002%
33	3.744	838	841	843	rBV4	1189	871	0.06%	0.008%
34	3.757	843	845	846	rBV2	1370	566	0.04%	0.005%
35	3.786	846	854	882	rBV2	77925	214793	15.75%	1.960%
36	4.140	960	964	966	rBV5	1821	1440	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW103123\
 Data File : VW032809.D
 Acq On : 31 Oct 2023 19:22
 Operator : SY/MD
 Sample : 05132-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5Q5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	4.252	986	999	1019	rBV	215572	545716	40.02%	4.978%
38	4.558	1088	1094	1096	rVB7	2426	2206	0.16%	0.020%
39	4.574	1096	1099	1101	rBV4	1332	865	0.06%	0.008%
40	4.635	1115	1118	1121	rBV5	1750	1262	0.09%	0.012%
41	4.748	1150	1153	1155	rBV2	1838	1045	0.08%	0.010%
42	4.854	1184	1186	1187	rBV2	1598	718	0.05%	0.007%
43	4.957	1203	1218	1235	rBV2	521208	1363727	100.00%	12.441%
44	5.535	1387	1398	1414	rBV	394235	810210	59.41%	7.391%
45	5.989	1528	1539	1574	rBV	297245	672915	49.34%	6.139%
46	6.510	1698	1701	1702	rBV3	1449	590	0.04%	0.005%
47	6.719	1762	1766	1769	rBV6	2246	1745	0.13%	0.016%
48	6.870	1810	1813	1814	rBV3	1040	516	0.04%	0.005%
49	6.915	1817	1827	1854	rVV	157300	316375	23.20%	2.886%
50	7.246	1918	1930	1955	rBV	631323	1182229	86.69%	10.785%
51	7.555	2017	2026	2043	rBV	111060	210142	15.41%	1.917%
52	7.850	2114	2118	2119	rBV3	2010	1233	0.09%	0.011%
53	8.027	2164	2173	2209	rBV	277615	573737	42.07%	5.234%
54	8.786	2394	2409	2431	rBV	677978	1157327	84.87%	10.558%
55	9.246	2548	2552	2556	rBV5	1932	1917	0.14%	0.017%
56	9.265	2556	2558	2560	rBV2	1821	1068	0.08%	0.010%
57	9.391	2593	2597	2598	rBV3	1646	1367	0.10%	0.012%
58	9.558	2647	2649	2650	rBV2	877	322	0.02%	0.003%
59	9.616	2665	2667	2669	rBV3	1163	597	0.04%	0.005%
60	9.690	2682	2690	2694	rBV9	2037	2681	0.20%	0.024%
61	9.709	2694	2696	2698	rBV3	1271	679	0.05%	0.006%
62	9.969	2774	2777	2779	rBV4	1809	1221	0.09%	0.011%
63	10.046	2799	2801	2804	rBV4	1624	829	0.06%	0.008%
64	10.156	2823	2835	2855	rBV	437989	700092	51.34%	6.387%
65	10.471	2931	2933	2936	rBV4	1526	976	0.07%	0.009%
66	10.599	2971	2973	2974	rBV2	1110	494	0.04%	0.005%
67	10.927	3073	3075	3076	rBV2	1361	565	0.04%	0.005%
68	10.953	3081	3083	3086	rVB4	1516	579	0.04%	0.005%
69	10.969	3086	3088	3091	rBV4	1809	1237	0.09%	0.011%
70	11.001	3096	3098	3102	rBV4	1299	933	0.07%	0.009%
71	11.188	3145	3156	3179	rBV	677321	1056841	77.50%	9.641%
72	11.564	3261	3273	3294	rBV	698205	1108826	81.31%	10.116%
73	11.963	3395	3397	3399	rBV3	1540	866	0.06%	0.008%
74	12.033	3418	3419	3420	rBV	1064	243	0.02%	0.002%
75	12.088	3433	3436	3442	rVB7	1616	1712	0.13%	0.016%
76	12.220	3474	3477	3479	rBV4	1924	1074	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032809.D
 Acq On : 31 Oct 2023 19:22
 Operator : SY/MD
 Sample : 05132-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5Q5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.378	3524	3526	3534	rVB9	1930	1326	0.10%	0.012%
78	12.413	3535	3537	3539	rVB3	1813	739	0.05%	0.007%
79	12.429	3540	3542	3546	rBV5	1542	1070	0.08%	0.010%
80	12.471	3553	3555	3557	rVB3	1636	665	0.05%	0.006%
81	12.484	3557	3559	3561	rBV3	807	335	0.02%	0.003%
82	12.506	3561	3566	3568	rBV6	2166	1509	0.11%	0.014%
83	12.574	3583	3587	3589	rBV4	2139	1412	0.10%	0.013%
84	12.744	3638	3640	3642	rBV3	1805	949	0.07%	0.009%
85	12.857	3672	3675	3678	rBV4	2058	1681	0.12%	0.015%
86	12.924	3695	3696	3699	rBV3	1129	577	0.04%	0.005%
87	13.136	3756	3762	3764	rBV6	1449	1435	0.11%	0.013%
88	13.152	3764	3767	3773	rBV9	2079	2268	0.17%	0.021%
89	13.307	3813	3815	3818	rVB4	1384	671	0.05%	0.006%
90	13.326	3818	3821	3822	rBV3	1516	938	0.07%	0.009%
91	13.577	3895	3899	3901	rBV5	1427	1017	0.07%	0.009%
92	13.619	3910	3912	3914	rBV3	1076	563	0.04%	0.005%
93	13.750	3951	3953	3955	rBV3	1180	785	0.06%	0.007%
94	13.792	3964	3966	3968	rBV3	1759	942	0.07%	0.009%
95	14.014	4033	4035	4038	rBV4	2094	1085	0.08%	0.010%
96	14.091	4057	4059	4063	rBV4	1655	1267	0.09%	0.012%
97	14.162	4079	4081	4083	rBV3	1962	925	0.07%	0.008%
98	14.255	4107	4110	4112	rBV4	2723	1464	0.11%	0.013%
99	14.702	4246	4249	4251	rVB4	1832	894	0.07%	0.008%
100	14.715	4251	4253	4254	rBV2	1161	334	0.02%	0.003%




Sum of corrected areas: 10961487

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032809.D
Acq On : 31 Oct 2023 19:22
Operator : SY/MD
Sample : 05132-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5Q5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

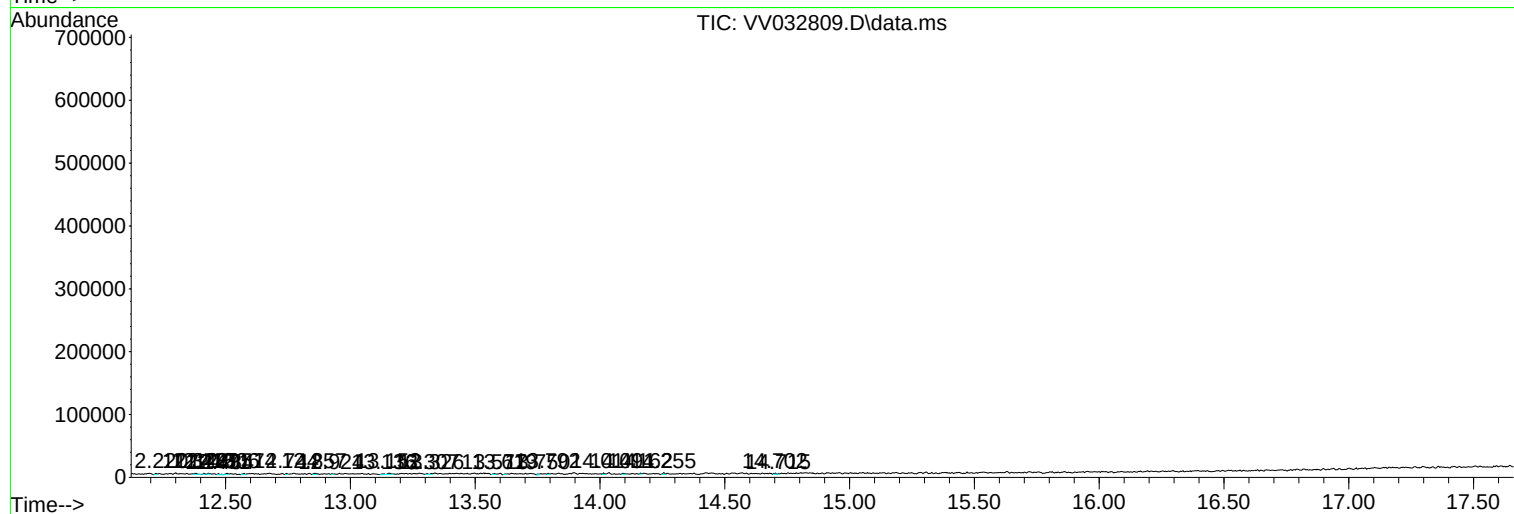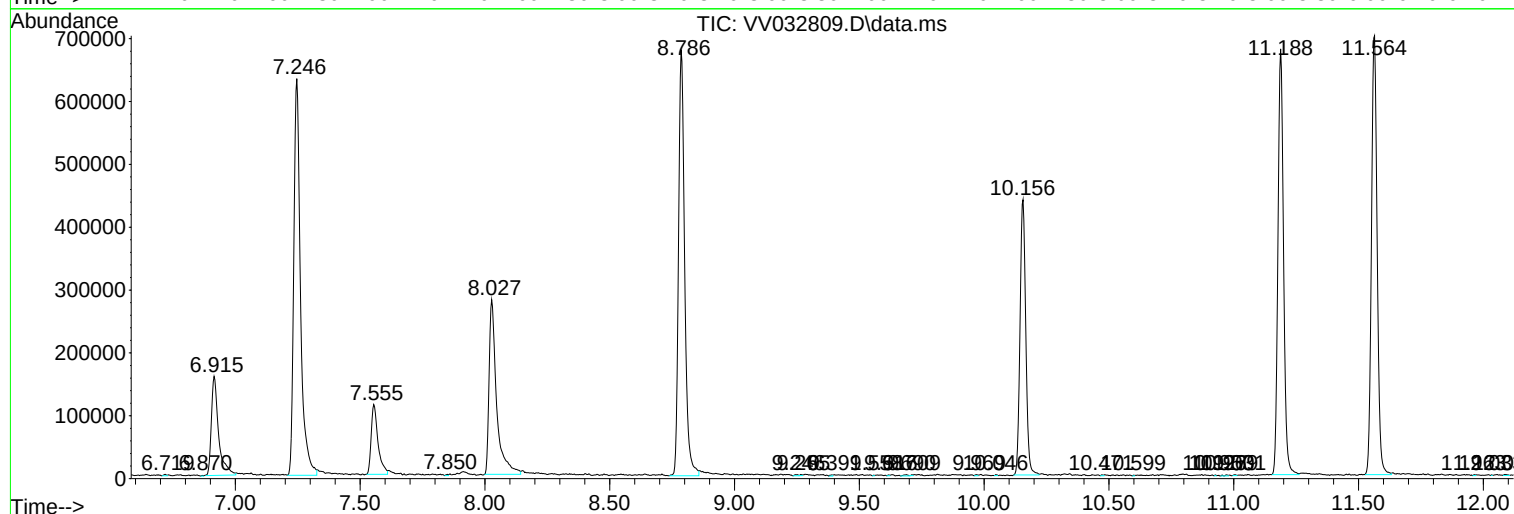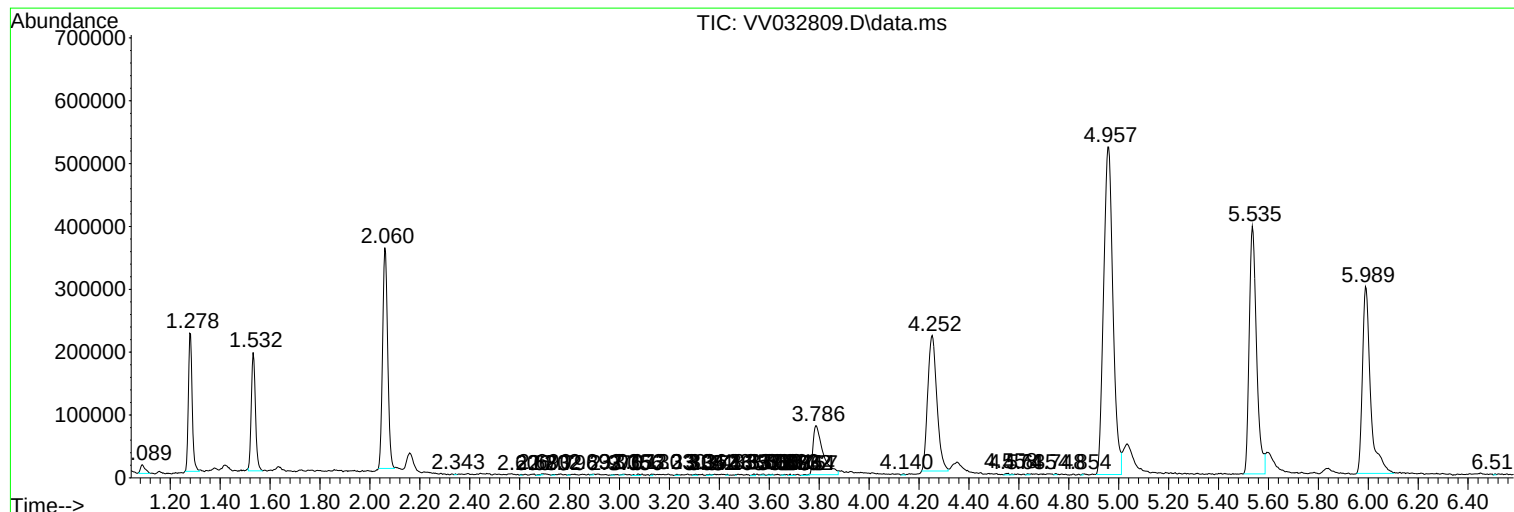

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032809.D
Acq On : 31 Oct 2023 19:22
Operator : SY/MD
Sample : 05132-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5Q5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032809.D
Acq On : 31 Oct 2023 19:22
Operator : SY/MD
Sample : 05132-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5Q5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------