

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032810.D
 Acq On : 31 Oct 2023 19:45
 Operator : SY/MD
 Sample : 05132-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5Q6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032810.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	10	14	24	rVB2	31545	33866	2.56%	0.314%
2	1.278	67	74	87	rBV	219815	242729	18.34%	2.252%
3	1.532	147	153	168	rVB	184297	209855	15.86%	1.947%
4	2.060	309	317	330	rBV	342912	490205	37.04%	4.548%
5	2.404	422	424	428	rVB5	1749	1036	0.08%	0.010%
6	2.487	448	450	451	rBV2	1489	587	0.04%	0.005%
7	2.632	489	495	497	rBV7	1469	1444	0.11%	0.013%
8	2.651	498	501	503	rBV3	1242	778	0.06%	0.007%
9	2.931	585	588	590	rBV4	1253	818	0.06%	0.008%
10	2.960	594	597	599	rBV4	1307	753	0.06%	0.007%
11	3.015	612	614	618	rBV4	1249	610	0.05%	0.006%
12	3.056	624	627	630	rVB4	1130	864	0.07%	0.008%
13	3.085	630	636	639	rBV8	1634	1337	0.10%	0.012%
14	3.172	659	663	666	rBV6	1522	1400	0.11%	0.013%
15	3.227	676	680	683	rVB4	1781	1393	0.11%	0.013%
16	3.253	683	688	689	rBV3	1060	694	0.05%	0.006%
17	3.285	695	698	699	rBV3	1342	736	0.06%	0.007%
18	3.317	703	708	710	rBV6	2247	1787	0.14%	0.017%
19	3.388	725	730	731	rBV5	1646	1219	0.09%	0.011%
20	3.433	742	744	747	rVB4	1088	599	0.05%	0.006%
21	3.523	768	772	777	rBV7	1499	1635	0.12%	0.015%
22	3.642	807	809	811	rBV3	1191	619	0.05%	0.006%
23	3.706	827	829	832	rVB4	2489	1248	0.09%	0.012%
24	3.728	832	836	838	rBV4	1642	1167	0.09%	0.011%
25	3.786	846	854	879	rBV2	75051	201849	15.25%	1.873%
26	4.163	969	971	973	rBV3	1080	603	0.05%	0.006%
27	4.253	985	999	1022	rBV	213475	553807	41.85%	5.139%
28	4.590	1102	1104	1106	rBV3	1332	596	0.05%	0.006%
29	4.667	1126	1128	1131	rBV3	1698	959	0.07%	0.009%
30	4.728	1145	1147	1152	rVB5	1598	1345	0.10%	0.012%
31	4.806	1167	1171	1175	rBV5	2226	2245	0.17%	0.021%
32	4.863	1186	1189	1192	rBV5	1083	900	0.07%	0.008%
33	4.960	1202	1219	1235	rBV2	505072	1323454	100.00%	12.280%
34	5.224	1297	1301	1302	rBV3	2441	1599	0.12%	0.015%
35	5.416	1357	1361	1363	rBV5	2604	2173	0.16%	0.020%
36	5.535	1386	1398	1413	rBV	392459	807531	61.02%	7.493%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032810.D
 Acq On : 31 Oct 2023 19:45
 Operator : SY/MD
 Sample : 05132-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5Q6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	5.989	1528	1539	1571	rBV2	287196	649839	49.10%	6.030%
38	6.387	1660	1663	1665	rBV4	2175	1172	0.09%	0.011%
39	6.429	1674	1676	1678	rBV2	1394	702	0.05%	0.007%
40	6.580	1718	1723	1726	rBV7	1748	1488	0.11%	0.014%
41	6.600	1726	1729	1732	rBV4	1798	1456	0.11%	0.014%
42	6.674	1750	1752	1754	rBV2	1614	768	0.06%	0.007%
43	6.719	1764	1766	1771	rBV5	1688	1355	0.10%	0.013%
44	6.915	1817	1827	1856	rBV	148762	304848	23.03%	2.829%
45	7.246	1918	1930	1955	rBV	601100	1140421	86.17%	10.582%
46	7.555	2018	2026	2046	rBV	107128	201279	15.21%	1.868%
47	8.027	2164	2173	2206	rBV	270715	568649	42.97%	5.276%
48	8.526	2324	2328	2329	rBV4	1488	881	0.07%	0.008%
49	8.786	2398	2409	2438	rVV	666964	1139299	86.09%	10.571%
50	9.014	2478	2480	2483	rBV4	1374	939	0.07%	0.009%
51	9.162	2522	2526	2529	rVB5	1964	1401	0.11%	0.013%
52	9.227	2540	2546	2547	rBV6	1340	1227	0.09%	0.011%
53	9.259	2553	2556	2557	rBV3	1225	663	0.05%	0.006%
54	9.317	2570	2574	2576	rBV4	1745	1069	0.08%	0.010%
55	9.381	2591	2594	2597	rBV5	1112	838	0.06%	0.008%
56	9.487	2623	2627	2630	rBV6	2200	1515	0.11%	0.014%
57	9.596	2659	2661	2665	rVB5	1712	751	0.06%	0.007%
58	9.667	2680	2683	2684	rBV3	2254	1102	0.08%	0.010%
59	9.731	2696	2703	2704	rBV7	1988	1978	0.15%	0.018%
60	9.976	2775	2779	2782	rBV5	2098	1524	0.12%	0.014%
61	10.156	2824	2835	2852	rBV	430845	685363	51.79%	6.359%
62	10.410	2912	2914	2915	rBV2	1428	652	0.05%	0.006%
63	10.522	2947	2949	2954	rVV6	1698	1303	0.10%	0.012%
64	10.545	2954	2956	2960	rVB6	2584	1463	0.11%	0.014%
65	10.638	2980	2985	2989	rBV8	1582	1496	0.11%	0.014%
66	10.776	3021	3028	3030	rBV9	2261	2606	0.20%	0.024%
67	10.847	3048	3050	3052	rBV3	2167	1018	0.08%	0.009%
68	10.931	3073	3076	3079	rBV5	1493	901	0.07%	0.008%
69	11.108	3124	3131	3138	rBV10	3117	6041	0.46%	0.056%
70	11.188	3145	3156	3178	rBV	675261	1049646	79.31%	9.739%
71	11.561	3261	3272	3291	rBV	678639	1070291	80.87%	9.931%
72	11.873	3366	3369	3370	rBV3	2364	1178	0.09%	0.011%
73	11.966	3394	3398	3400	rVB5	2145	1482	0.11%	0.014%
74	11.982	3400	3403	3404	rBV3	2026	957	0.07%	0.009%
75	12.249	3480	3486	3487	rBV6	1415	1466	0.11%	0.014%
76	12.390	3526	3530	3533	rBV5	1755	1387	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032810.D
 Acq On : 31 Oct 2023 19:45
 Operator : SY/MD
 Sample : 05132-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5Q6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.519	3568	3570	3573	rBV3	1956	935	0.07%	0.009%
78	12.574	3584	3587	3589	rBV4	1426	819	0.06%	0.008%
79	12.664	3612	3615	3618	rBV5	1820	1257	0.09%	0.012%
80	12.715	3629	3631	3633	rBV3	1595	710	0.05%	0.007%
81	12.966	3707	3709	3712	rVB4	2381	1181	0.09%	0.011%
82	12.989	3712	3716	3719	rBV6	1962	1908	0.14%	0.018%
83	13.066	3739	3740	3742	rBV2	1338	673	0.05%	0.006%
84	13.175	3771	3774	3778	rBV5	1636	1063	0.08%	0.010%
85	13.326	3816	3821	3823	rBV6	1349	1110	0.08%	0.010%
86	13.426	3850	3852	3855	rBV3	2007	1330	0.10%	0.012%
87	13.455	3855	3861	3868	rVV10	2705	3841	0.29%	0.036%
88	13.519	3878	3881	3882	rBV3	1629	1022	0.08%	0.009%
89	13.689	3932	3934	3940	rVB6	2008	1508	0.11%	0.014%
90	13.715	3940	3942	3944	rBV3	1574	801	0.06%	0.007%
91	13.741	3948	3950	3952	rBV3	1825	1018	0.08%	0.009%
92	13.886	3993	3995	3997	rBV3	1373	820	0.06%	0.008%
93	13.934	4007	4010	4016	rVB7	1961	1677	0.13%	0.016%
94	13.988	4022	4027	4031	rBV9	2690	2468	0.19%	0.023%
95	14.152	4076	4078	4081	rBV4	1126	647	0.05%	0.006%
96	14.307	4122	4126	4130	rBV7	1759	1307	0.10%	0.012%
97	14.554	4201	4203	4205	rBV3	1319	581	0.04%	0.005%
98	14.564	4205	4206	4209	rBV3	1442	838	0.06%	0.008%
99	14.699	4245	4248	4252	rBV6	2413	1889	0.14%	0.018%
100	15.262	4422	4423	4426	rBV3	1999	1083	0.08%	0.010%




Sum of corrected areas: 10777340

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032810.D
Acq On : 31 Oct 2023 19:45
Operator : SY/MD
Sample : 05132-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5Q6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

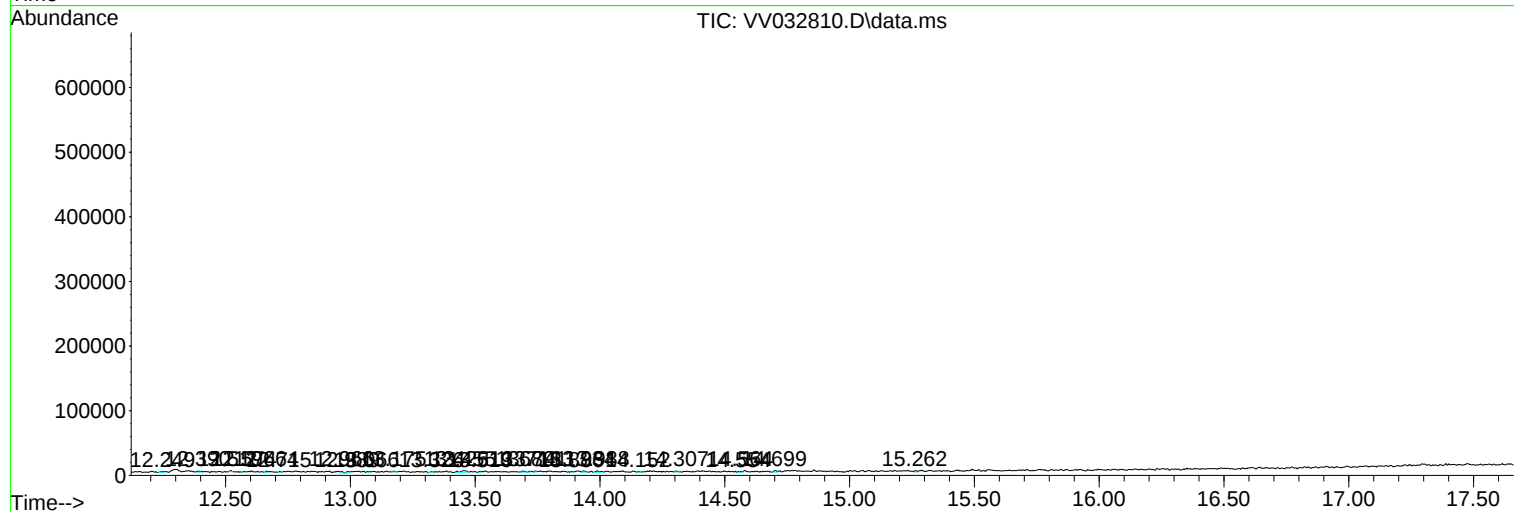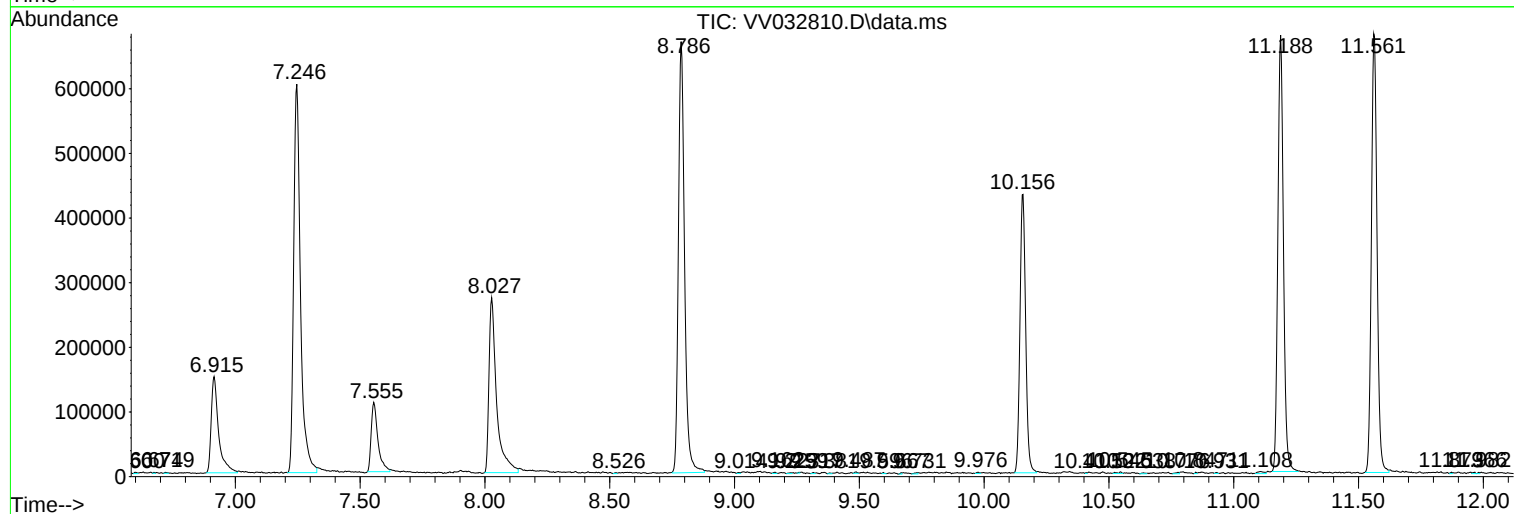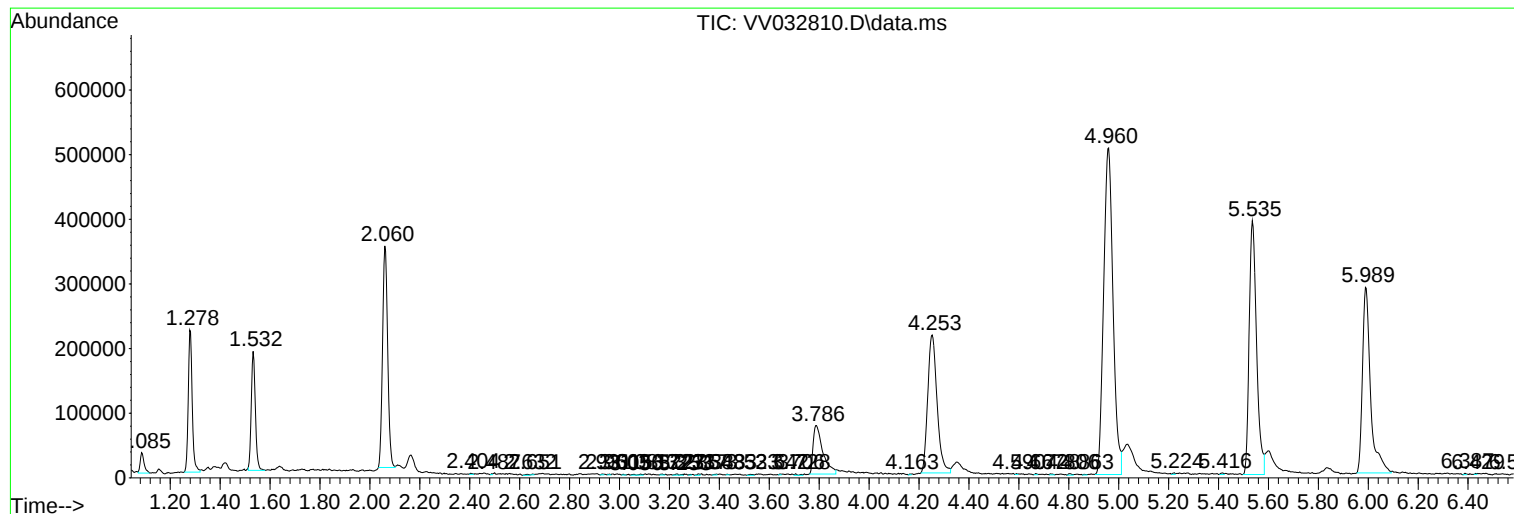

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032810.D
Acq On : 31 Oct 2023 19:45
Operator : SY/MD
Sample : 05132-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5Q6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032810.D
Acq On : 31 Oct 2023 19:45
Operator : SY/MD
Sample : 05132-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5Q6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------