

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032812.D
 Acq On : 31 Oct 2023 20:32
 Operator : SY/MD
 Sample : 05132-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5R3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032812.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	25	rBV2	35455	36319	2.65%	0.330%
2	1.153	32	35	41	rBV4	4117	4026	0.29%	0.037%
3	1.281	68	75	88	rVB	229782	244861	17.87%	2.222%
4	1.532	147	153	167	rVB	191504	218163	15.92%	1.980%
5	2.060	309	317	331	rVB	354263	500330	36.51%	4.540%
6	2.542	463	467	470	rBV4	2091	2058	0.15%	0.019%
7	2.664	500	505	507	rBV6	3238	3130	0.23%	0.028%
8	2.777	538	540	544	rBV3	1475	962	0.07%	0.009%
9	2.912	581	582	585	rVB3	1990	822	0.06%	0.007%
10	3.040	620	622	623	rVB2	1049	259	0.02%	0.002%
11	3.053	624	626	628	rBV3	1248	540	0.04%	0.005%
12	3.072	630	632	635	rBV4	1210	619	0.05%	0.006%
13	3.114	643	645	646	rBV2	889	404	0.03%	0.004%
14	3.249	685	687	691	rBV4	1585	1084	0.08%	0.010%
15	3.291	697	700	702	rBV4	1585	956	0.07%	0.009%
16	3.339	713	715	719	rVB5	2638	1780	0.13%	0.016%
17	3.362	719	722	723	rBV3	2076	1195	0.09%	0.011%
18	3.471	754	756	757	rBV2	1275	467	0.03%	0.004%
19	3.500	760	765	767	rBV6	1181	1030	0.08%	0.009%
20	3.786	846	854	882	rBV	81071	224150	16.36%	2.034%
21	4.056	936	938	941	rBV4	2031	1341	0.10%	0.012%
22	4.140	962	964	966	rBV3	1102	666	0.05%	0.006%
23	4.249	984	998	1019	rBV2	221382	574884	41.95%	5.217%
24	4.957	1202	1218	1235	rBV2	525511	1370264	100.00%	12.435%
25	5.535	1386	1398	1413	rBV	397283	815999	59.55%	7.405%
26	5.989	1527	1539	1572	rBV	295231	678119	49.49%	6.154%
27	6.381	1659	1661	1662	rBV2	1444	475	0.03%	0.004%
28	6.420	1671	1673	1674	rBV3	1361	626	0.05%	0.006%
29	6.648	1742	1744	1745	rBV3	1458	336	0.02%	0.003%
30	6.760	1774	1779	1780	rBV5	1622	1567	0.11%	0.014%
31	6.802	1790	1792	1797	rVB6	1126	498	0.04%	0.005%
32	6.854	1806	1808	1811	rBV4	1660	820	0.06%	0.007%
33	6.915	1817	1827	1853	rBV	153568	313524	22.88%	2.845%
34	7.246	1919	1930	1955	rBV	629842	1173603	85.65%	10.650%
35	7.555	2017	2026	2044	rBV	113202	215258	15.71%	1.953%
36	8.027	2164	2173	2206	rBV	277180	574506	41.93%	5.213%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
 Data File : VV032812.D
 Acq On : 31 Oct 2023 20:32
 Operator : SY/MD
 Sample : 05132-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5R3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	8.616	2354	2356	2359	rBV4	1547	846	0.06%	0.008%
38	8.786	2397	2409	2433	rBV	681244	1161245	84.75%	10.538%
39	9.452	2612	2616	2617	rBV4	1506	992	0.07%	0.009%
40	9.699	2690	2693	2697	rBV6	1961	2172	0.16%	0.020%
41	9.927	2762	2764	2768	rBV5	2174	1462	0.11%	0.013%
42	9.956	2771	2773	2776	rBV5	2351	1599	0.12%	0.015%
43	10.156	2823	2835	2853	rBV	440312	711656	51.94%	6.458%
44	10.452	2925	2927	2931	rBV5	1745	1511	0.11%	0.014%
45	10.542	2952	2955	2956	rBV2	1907	1228	0.09%	0.011%
46	10.860	3051	3054	3055	rBV3	1193	722	0.05%	0.007%
47	10.943	3078	3080	3082	rBV3	1768	706	0.05%	0.006%
48	11.188	3145	3156	3173	rBV	688212	1069412	78.04%	9.705%
49	11.564	3262	3273	3291	rVB	688511	1089967	79.54%	9.891%
50	12.011	3408	3412	3413	rBV4	1595	999	0.07%	0.009%
51	12.072	3429	3431	3434	rBV4	1218	961	0.07%	0.009%
52	12.792	3653	3655	3656	rBV2	1048	316	0.02%	0.003%
53	13.030	3727	3729	3731	rBV3	1080	485	0.04%	0.004%
54	13.078	3741	3744	3745	rBV2	1836	1005	0.07%	0.009%
55	13.123	3756	3758	3760	rVB2	1815	651	0.05%	0.006%
56	13.242	3793	3795	3798	rBV3	1511	624	0.05%	0.006%
57	13.606	3904	3908	3911	rBV6	1738	1569	0.11%	0.014%
58	13.728	3943	3946	3950	rBV5	2036	1315	0.10%	0.012%
59	13.754	3952	3954	3959	rBV6	1216	918	0.07%	0.008%
60	14.040	4041	4043	4046	rVB3	1735	842	0.06%	0.008%
61	14.332	4132	4134	4136	rBV3	1882	829	0.06%	0.008%




Sum of corrected areas: 11019673

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032812.D
Acq On : 31 Oct 2023 20:32
Operator : SY/MD
Sample : 05132-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5R3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

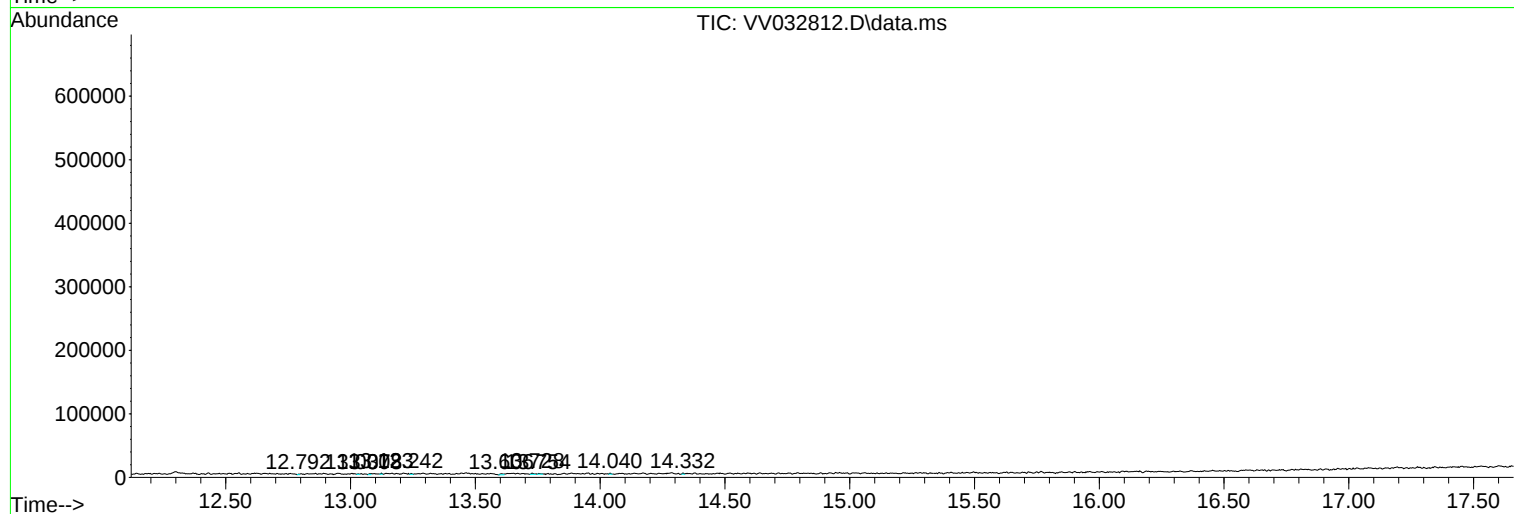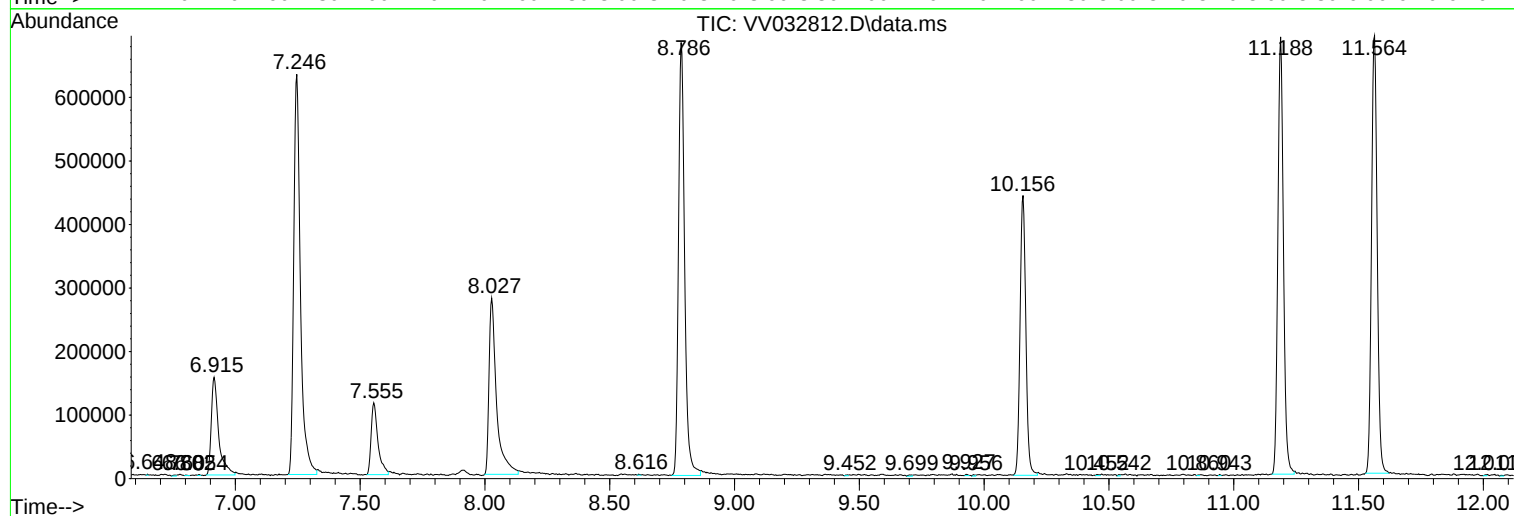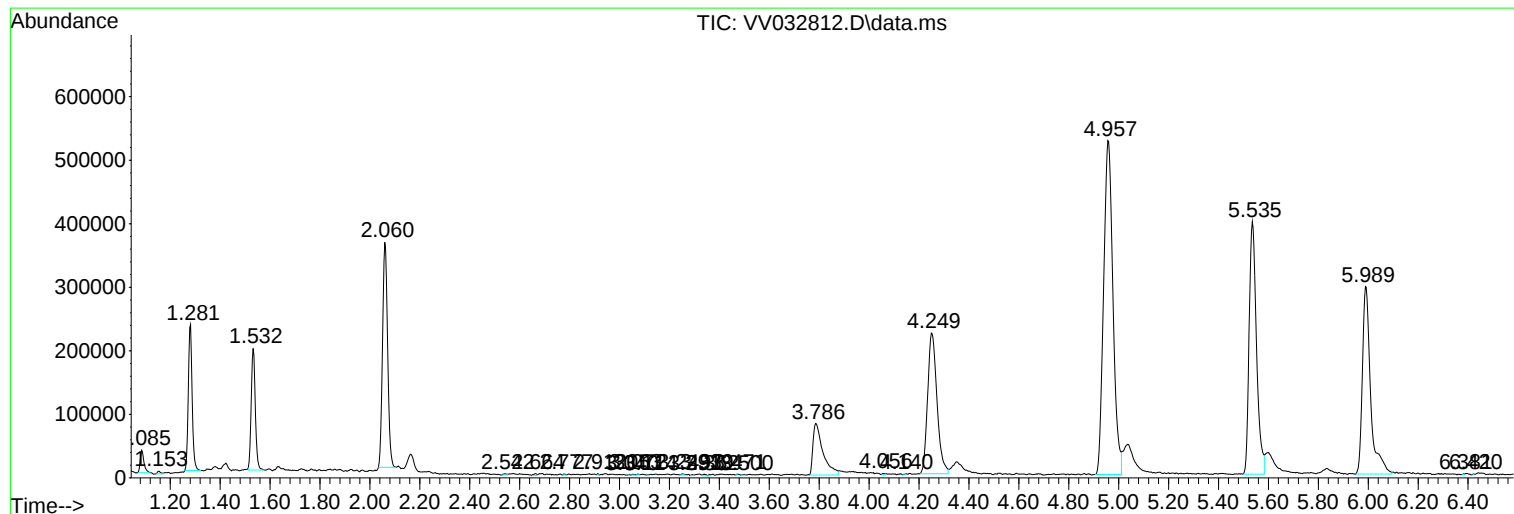

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032812.D
Acq On : 31 Oct 2023 20:32
Operator : SY/MD
Sample : 05132-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5R3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV103123\
Data File : VV032812.D
Acq On : 31 Oct 2023 20:32
Operator : SY/MD
Sample : 05132-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5R3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc