

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV110118\
 Data File : VV008509.D
 Acq On : 01 Nov 2018 13:10
 Operator : SY/MD
 Sample : J5726-05
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBX2

Quant Time: Nov 02 07:36:57 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM103118WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 02 07:10:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	206220	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	186690	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	77178	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	55964	42.68	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.36%
7) Chloroethane-d5	1.56	69	40587	55.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	111.18%
11) 1,1-Dichloroethene-d2	2.13	63	71651	34.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.02%
21) 2-Butanone-d5	3.94	46	117399	92.49	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.49%
24) Chloroform-d	4.41	84	129130	44.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.74%
26) 1,2-Dichloroethane-d4	5.09	65	89975	46.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.58%
32) Benzene-d6	5.10	84	261715	46.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.60%
36) 1,2-Dichloropropane-d6	6.12	67	89881	47.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.50%
41) Toluene-d8	7.36	98	230156	44.57	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.14%
43) trans-1,3-Dichloropropene-	7.67	79	43523	45.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.22%
47) 2-Hexanone-d5	8.14	63	89051	92.87	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.87%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	121505	46.18	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.36%
64) 1,2-Dichlorobenzene-d4	11.68	152	78901	46.64	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.28%


Target Compounds					Qvalue
13) Acetone	2.20	43	8235	7.840 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110118\
Data File : VV008509.D
Acq On : 01 Nov 2018 13:10
Operator : SY/MD
Sample : J5726-05
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBX2

Quant Time: Nov 02 07:36:57 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM103118WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 02 07:10:33 2018
Response via : Initial Calibration

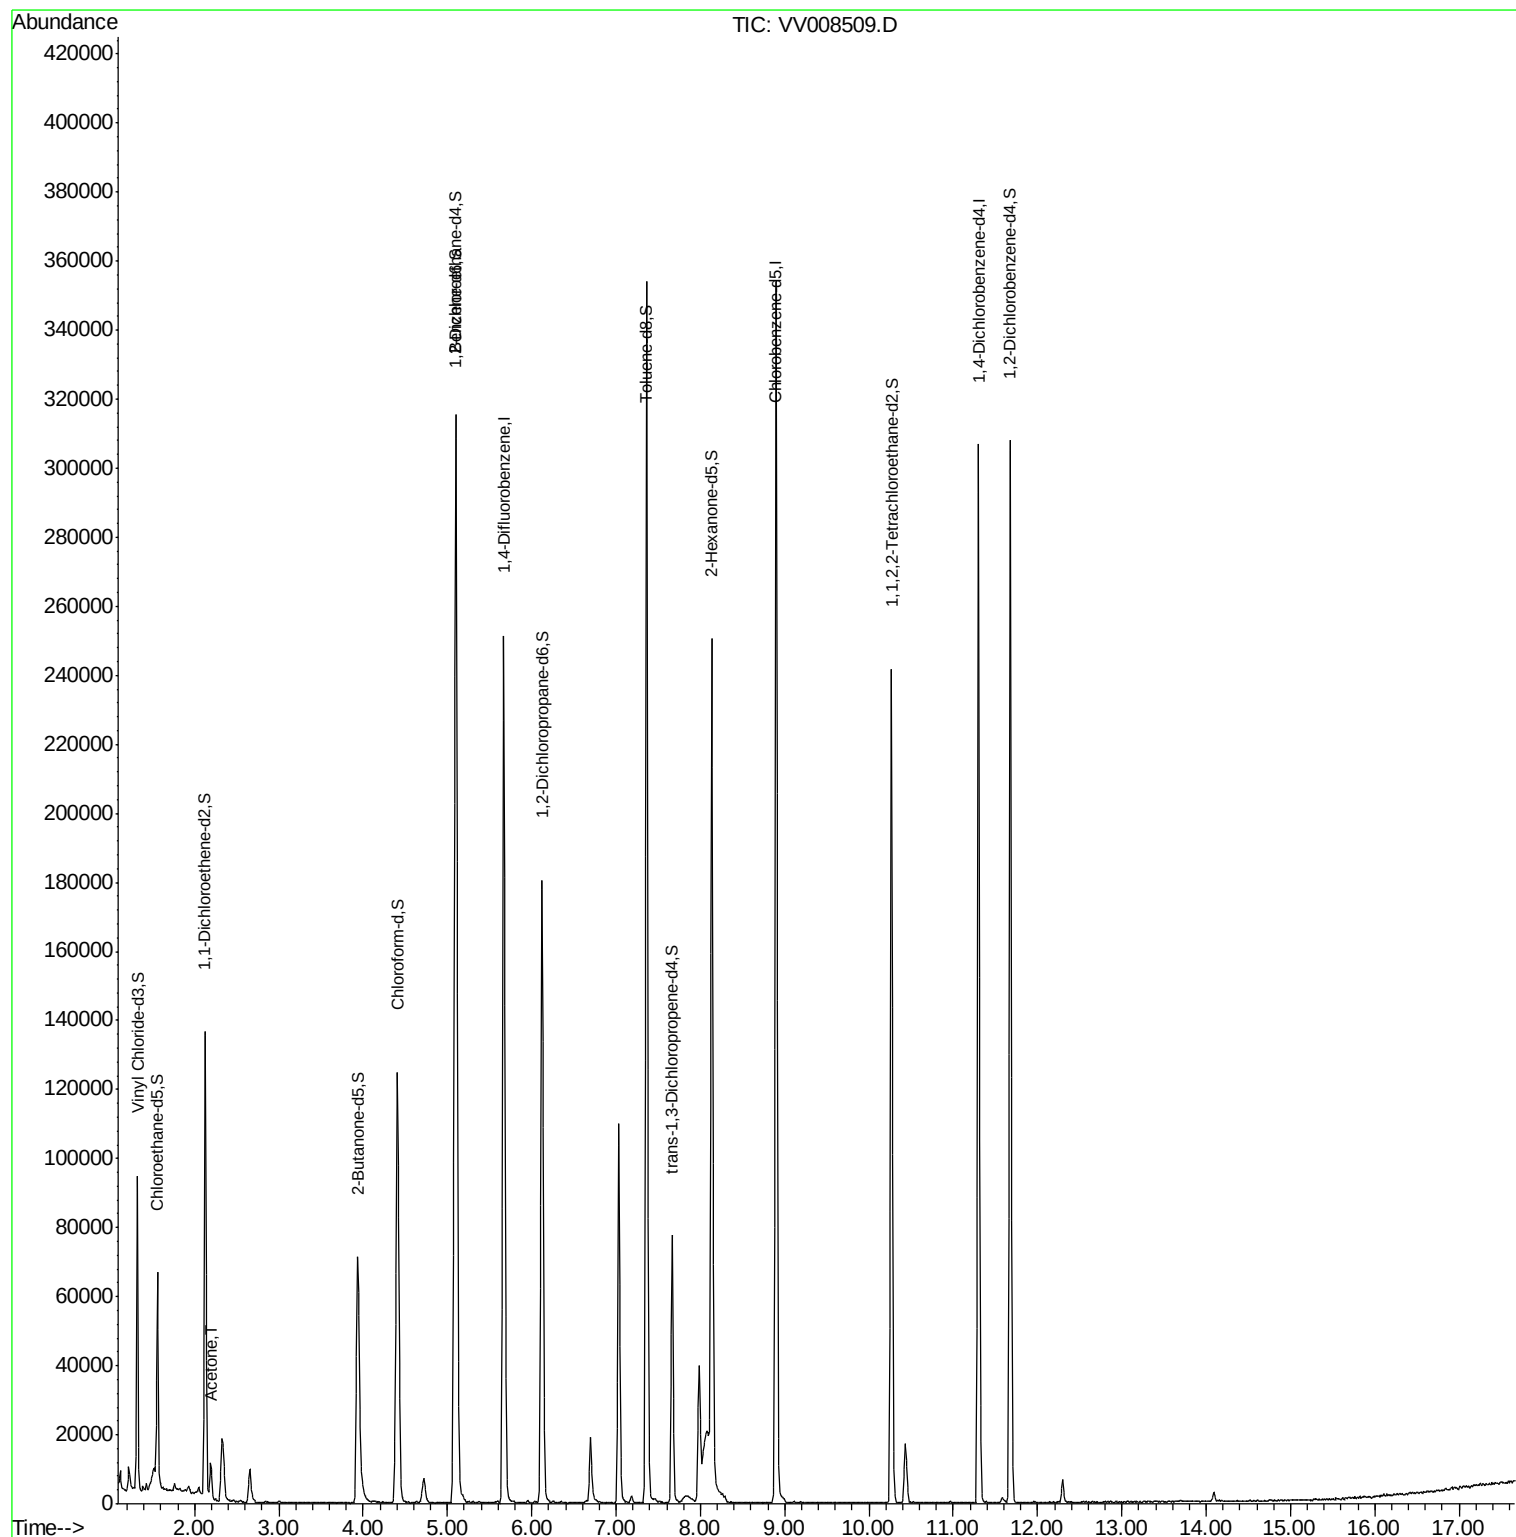

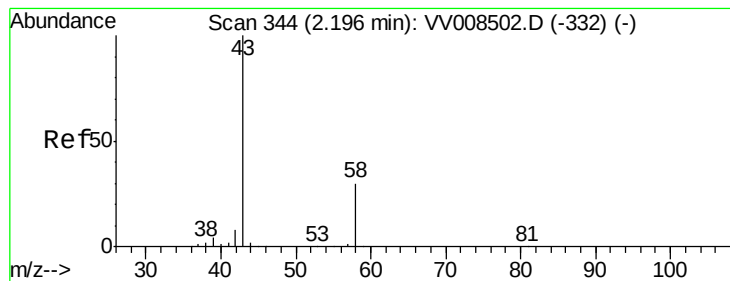

#13

Acetone

Concen: 7.840 ug/L

RT: 2.20 min Scan# 344

Delta R.T. -0.00 min

Lab File: VV008509.D

Acq: 01 Nov 2018 13:10

Instrument :

MSVOA_V

ClientSampleId :


ETBX2

Tgt Ion: 43 Resp: 8235

Ion Ratio Lower Upper

43 100

58 33.3 0.0 61.4

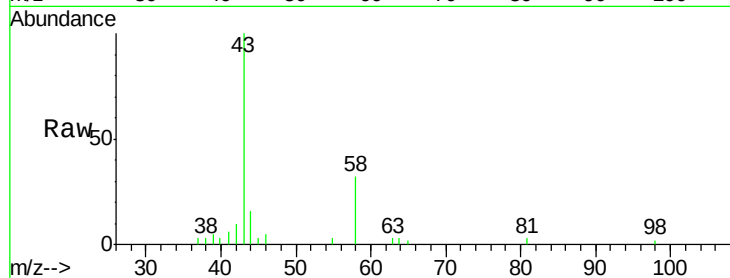

Abundance Ion 43.00 (42.70 to 43.70): VV0

Ion 58.00 (57.70 to 58.70): VV0

