

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV110118\
 Data File : VV008510.D
 Acq On : 01 Nov 2018 13:33
 Operator : SY/MD
 Sample : J5726-06
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBX3

Quant Time: Nov 02 07:39:22 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM103118WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 02 07:10:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	210754	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	192137	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	82148	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	57974	43.26	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.52%
7) Chloroethane-d5	1.56	69	42112	56.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	112.88%
11) 1,1-Dichloroethene-d2	2.13	63	75579	35.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.22%
21) 2-Butanone-d5	3.94	46	125142	96.47	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.47%
24) Chloroform-d	4.41	84	136299	46.34	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.68%
26) 1,2-Dichloroethane-d4	5.09	65	94497	48.08	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.16%
32) Benzene-d6	5.10	84	276131	47.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.92%
36) 1,2-Dichloropropane-d6	6.12	67	93139	47.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.16%
41) Toluene-d8	7.36	98	248767	46.81	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.62%
43) trans-1,3-Dichloropropene-	7.67	79	45794	46.12	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.24%
47) 2-Hexanone-d5	8.14	63	93496	94.74	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.74%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	127274	47.00	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	86677	48.13	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.26%


Target Compounds					Qvalue
13) Acetone	2.19	43	4707	4.385 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110118\
Data File : VV008510.D
Acq On : 01 Nov 2018 13:33
Operator : SY/MD
Sample : J5726-06
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBX3

Quant Time: Nov 02 07:39:22 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM103118WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 02 07:10:33 2018
Response via : Initial Calibration

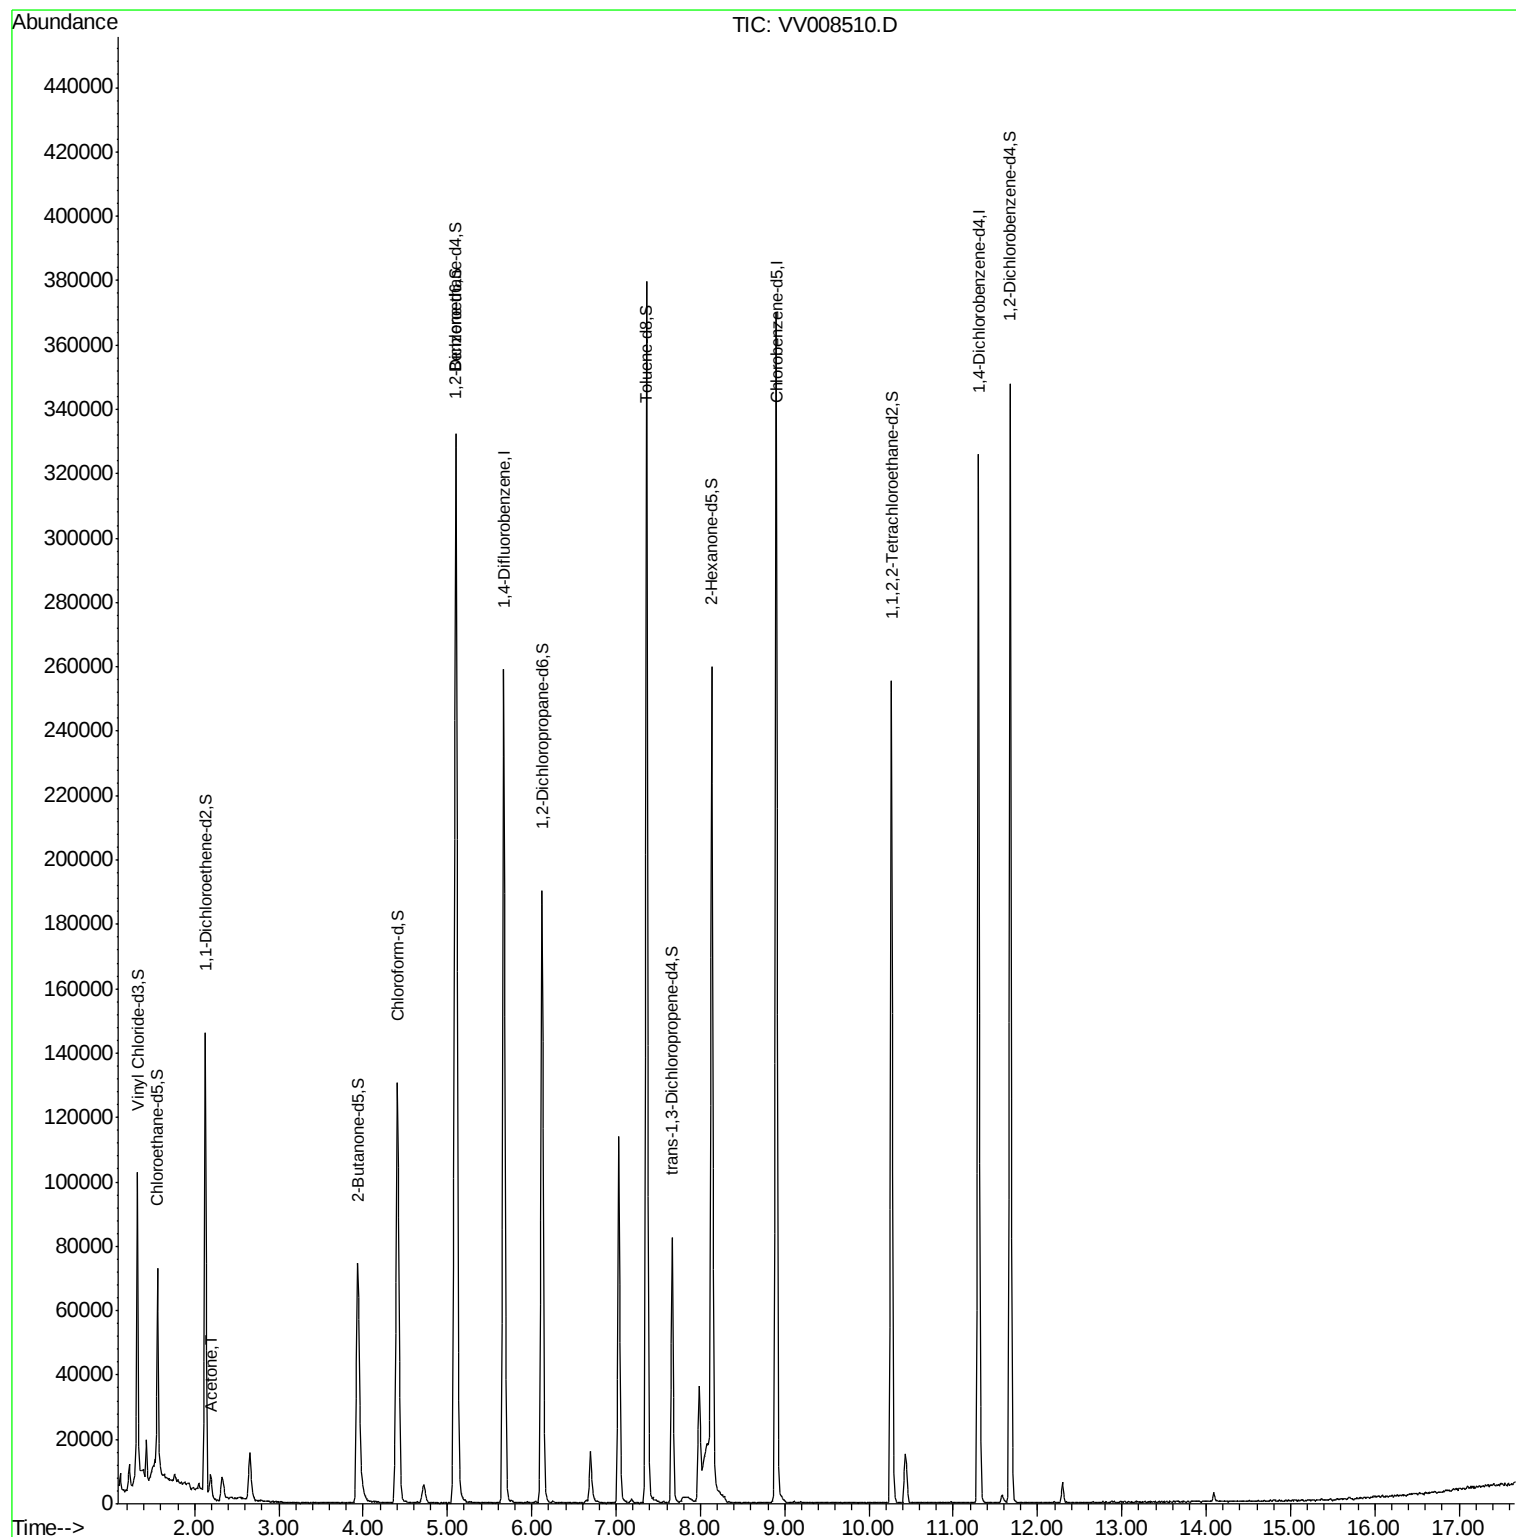

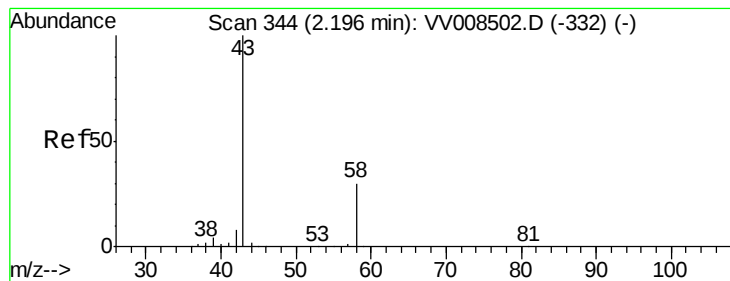

#13
 Acetone
 Concen: 4.385 ug/L
 RT: 2.19 min Scan# 343
 Delta R.T. -0.00 min
 Lab File: VV008510.D
 Acq: 01 Nov 2018 13:33

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBX3

Tgt Ion: 43 Resp: 4707
 Ion Ratio Lower Upper
 43 100
 58 33.7 0.0 61.4

