


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV110118\
Data File : VV008501.D
Acq On : 01 Nov 2018 09:26
Operator : SY/MD
Sample : BFB55
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB55

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM103118WMA.M
Title : VOC Analysis
Last Update : Fri Nov 02 18:36:43 2018

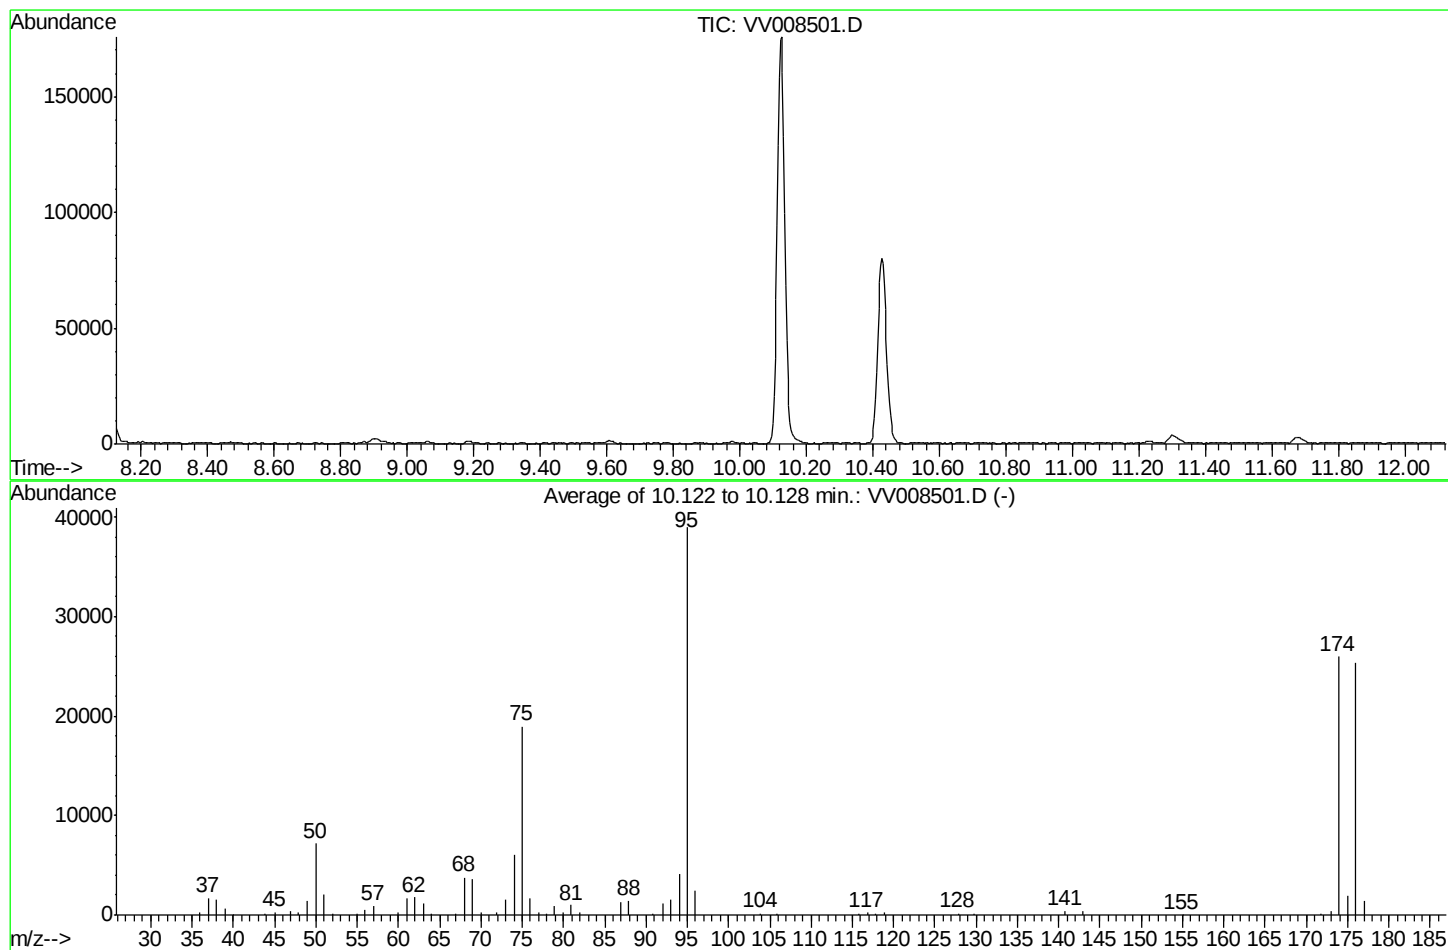

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	7184	PASS
75	95	30	80	48.7	18976	PASS
95	95	100	100	100.0	38962	PASS
96	95	5	9	6.4	2478	PASS
173	174	0.00	2	1.3	339	PASS
174	95	50	120	66.7	25978	PASS
175	174	5	9	7.3	1885	PASS
176	174	95	101	97.7	25373	PASS
177	176	5	9	5.7	1439	PASS

m/z	Abundance
35.90	307.0
37.00	1777.0
38.00	1586.0
39.00	672.0
39.90	139.0
43.90	420.0
45.00	353.0
46.90	425.0
47.90	226.0
49.00	1446.0
50.00	7545.0
51.00	2208.0
52.00	140.0
55.00	110.0
56.00	576.0
57.00	968.0
59.90	325.0
61.00	1721.0
61.90	1792.0
63.00	1308.0
64.00	187.0
67.00	123.0
68.00	3859.0
69.00	3778.0
70.00	264.0
71.90	248.0
73.00	1579.0
74.00	6315.0
75.00	19632.0
76.00	1730.0
77.00	298.0
77.90	132.0
78.90	963.0
79.90	270.0
80.90	1075.0
81.90	221.0
86.90	1363.0
87.90	1524.0
90.90	193.0
92.00	1180.0
92.90	1646.0
94.00	4215.0
95.00	40008.0
96.00	2650.0
103.80	142.0
105.80	137.0
115.70	142.0
116.80	201.0
117.80	147.0
118.80	210.0
127.90	148.0
129.80	137.0
140.80	365.0
142.90	360.0
171.80	105.0
173.00	327.0
173.90	25960.0
175.00	1956.0
175.90	25536.0
177.00	1449.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
35.90	284.0
37.00	1719.0
38.00	1534.0
39.00	683.0
40.00	157.0
43.90	461.0
45.00	328.0
47.00	392.0
47.90	213.0
49.00	1455.0
50.00	7457.0
51.00	2113.0
52.00	138.0
55.00	105.0
56.00	563.0
57.00	962.0
59.90	332.0
61.00	1803.0
61.90	1821.0
63.00	1227.0
63.90	162.0
67.00	101.0
68.00	3860.0
69.00	3636.0
70.00	293.0
71.90	208.0
73.00	1594.0
74.00	6174.0
75.00	19520.0
76.00	1695.0
77.00	241.0
78.00	145.0
78.80	928.0
79.90	288.0
80.90	1030.0
81.90	227.0
87.00	1302.0
87.90	1513.0
90.80	155.0
92.00	1237.0
92.90	1590.0
94.00	4218.0
95.00	40296.0
96.00	2585.0
103.90	152.0
105.90	135.0
115.80	124.0
116.80	225.0
117.80	146.0
118.80	229.0
127.90	160.0
129.80	141.0
140.80	437.0
142.90	365.0
155.00	103.0
171.80	118.0
173.00	346.0
173.90	26696.0
175.00	1896.0
175.90	26256.0
177.00	1476.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
35.90	242.0
37.00	1546.0
38.00	1460.0
39.00	650.0
39.90	146.0
43.90	450.0
45.00	256.0
47.00	362.0
47.80	198.0
49.00	1353.0
50.00	6550.0
51.00	1832.0
52.00	114.0
56.00	496.0
57.00	878.0
59.90	319.0
61.00	1623.0
62.00	1636.0
63.00	1070.0
63.90	125.0
66.90	101.0
68.00	3506.0
69.00	3315.0
70.00	305.0
71.90	168.0
73.00	1451.0
74.00	5554.0
75.00	17776.0
76.00	1544.0
76.90	180.0
78.00	125.0
78.80	825.0
79.90	301.0
80.90	896.0
81.90	217.0
87.00	1154.0
87.90	1309.0
90.80	128.0
92.00	1163.0
93.00	1394.0
94.00	3953.0
95.00	36584.0
96.00	2199.0
103.90	157.0
105.90	134.0
116.80	219.0
117.80	127.0
118.80	200.0
127.80	156.0
129.80	126.0
140.80	422.0
142.90	323.0
172.90	346.0
173.90	25280.0
175.00	1803.0
175.90	24328.0
176.90	1394.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
39.90	113.0
43.80	252.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55