

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110121\
 Data File : VV023109.D
 Acq On : 01 Nov 2021 12:09
 Operator : SY/MD
 Sample : M4364-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG323

Quant Time: Nov 02 01:14:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 01:11:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	132584	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	131964	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58133	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	40487	3.495	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	69.800%	
7) Chloroethane-d5	1.568	69	35754	4.989	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	99.800%	
11) 1,1-Dichloroethene-d2	2.108	63	60460	3.617	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.400%	
20) 2-Butanone-d5	3.883	46	93294	50.199	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	100.400%	
24) Chloroform-d	4.346	84	95351	5.063	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.200%	
26) 1,2-Dichloroethane-d4	5.031	65	43817	4.935	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.800%	
32) Benzene-d6	5.047	84	181982	4.723	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.400%	
36) 1,2-Dichloropropane-d6	6.069	67	55452	4.675	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	93.600%	
41) Toluene-d8	7.317	98	151958	4.391	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.800%	
43) trans-1,3-Dichloroprop...	7.622	79	13889	3.342	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	66.800%	
46) 2-Hexanone-d5	8.088	63	67896	44.131	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	88.260%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	38369	4.685	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	93.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	56247	5.423	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	108.400%	
Target Compounds						Qvalue
15) Methyl Acetate	2.446	43	1436	0.414	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110121\
Data File : VV023109.D
Acq On : 01 Nov 2021 12:09
Operator : SY/MD
Sample : M4364-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG323

Quant Time: Nov 02 01:14:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 01:11:36 2021
Response via : Initial Calibration

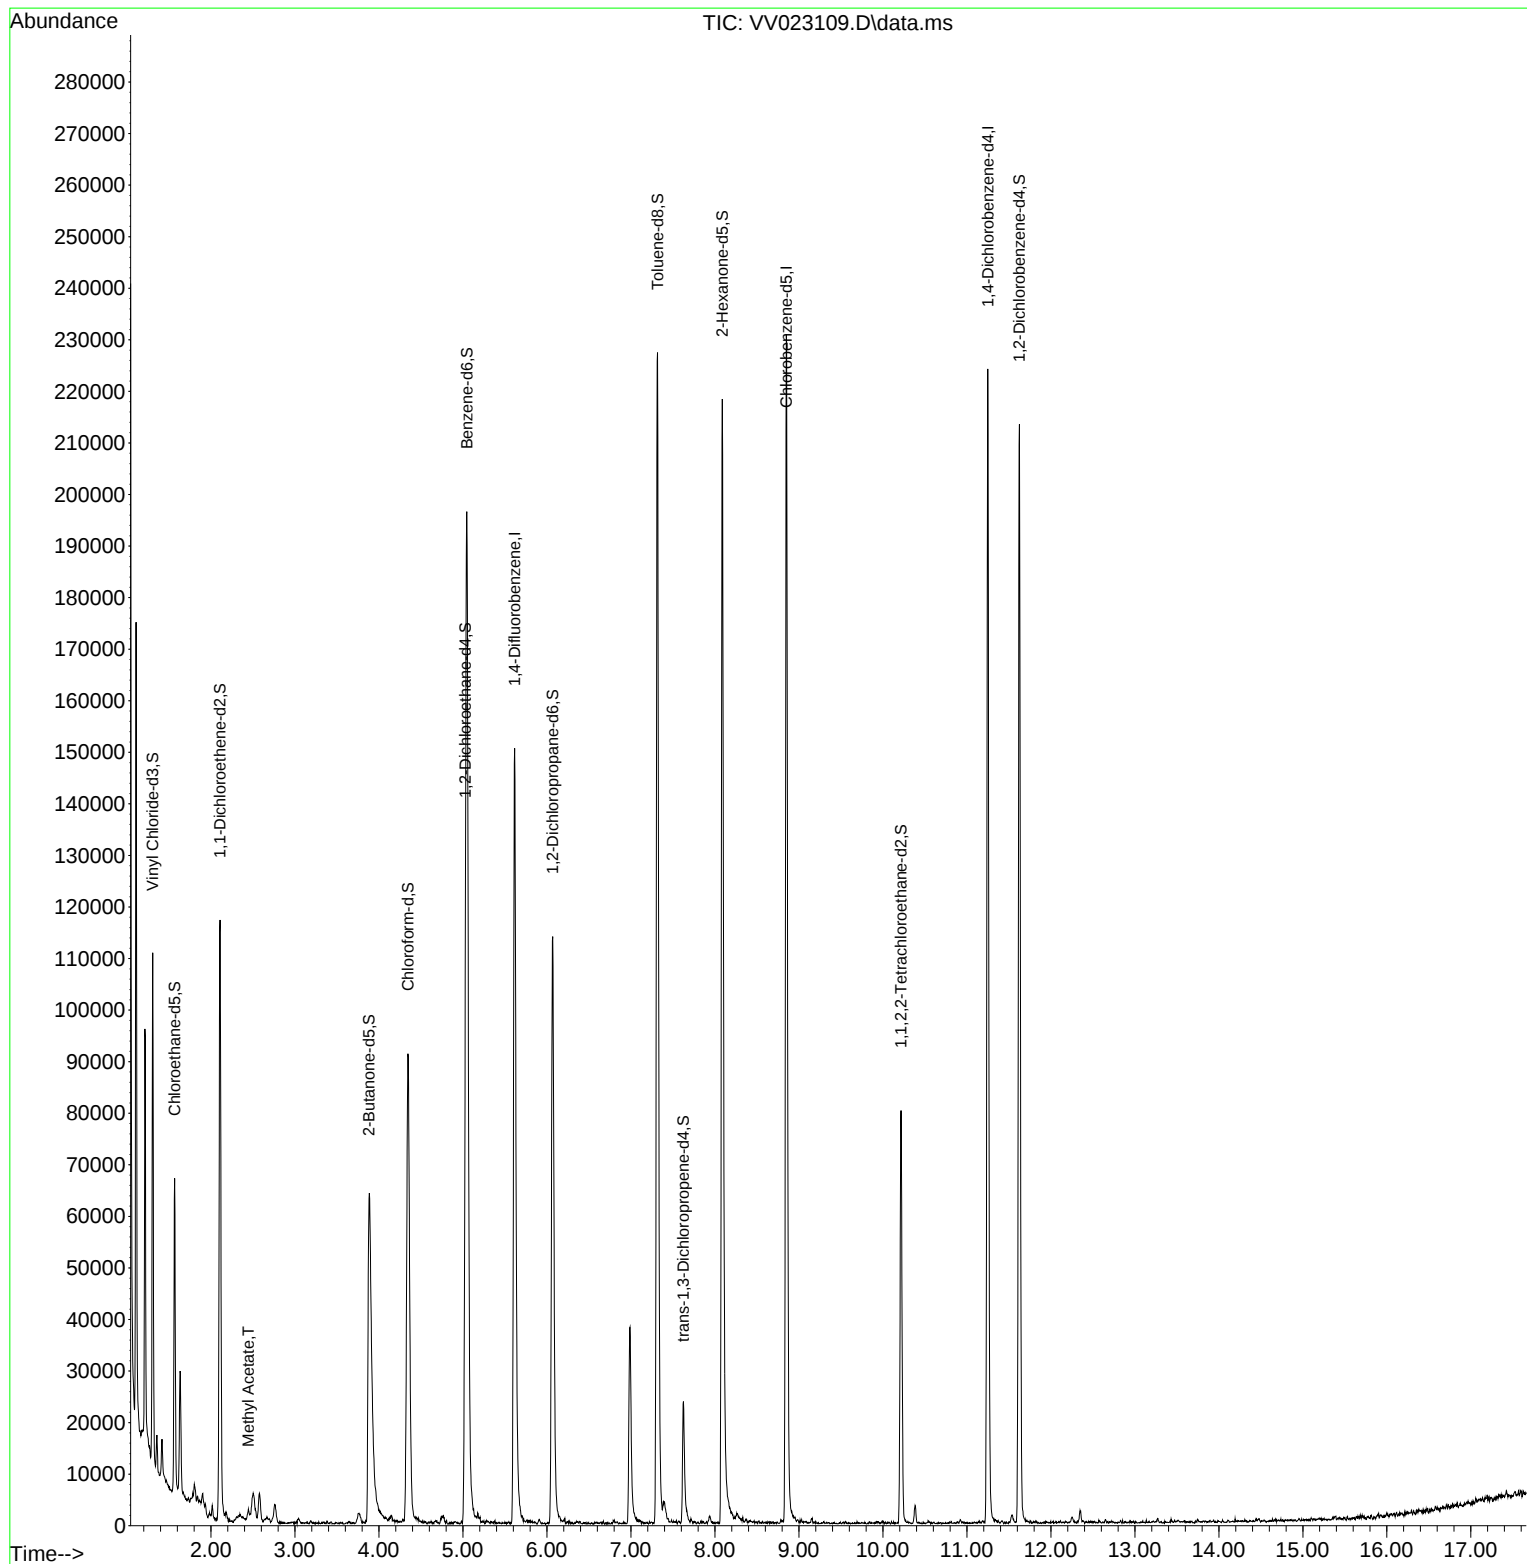

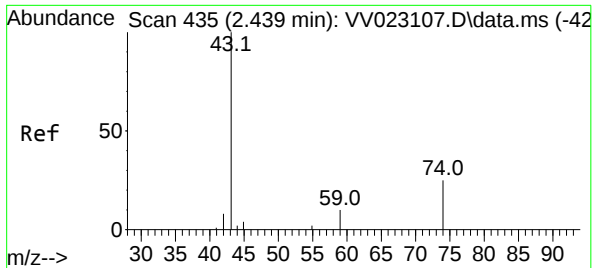

#15
Methyl Acetate
Concen: 0.414 ug/L
RT: 2.446 min Scan# 41
Delta R.T. 0.006 min
Lab File: VV023109.D
Acq: 01 Nov 2021 12:09

Instrument :
MSVOA_V
ClientSampleId :
BG323

Tgt Ion: 43 Resp: 1436
Ion Ratio Lower Upper
43 100
74 27.5 22.2 33.2

