

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110121\
 Data File : VV023113.D
 Acq On : 01 Nov 2021 13:43
 Operator : SY/MD
 Sample : M4364-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG339

Quant Time: Nov 02 01:15:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 01:11:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	122228	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	125020	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	61829	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	31879	2.985	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	59.600%
7) Chloroethane-d5	1.568	69	29949	4.533	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.600%
11) 1,1-Dichloroethene-d2	2.108	63	49661	3.223	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.400%
20) 2-Butanone-d5	3.889	46	112308	65.550	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	131.100%#
24) Chloroform-d	4.352	84	89584	5.159	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.200%
26) 1,2-Dichloroethane-d4	5.037	65	43562	5.322	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.400%
32) Benzene-d6	5.053	84	167034	4.576	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
36) 1,2-Dichloropropane-d6	6.072	67	55322	4.924	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.400%
41) Toluene-d8	7.320	98	147570	4.501	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.000%
43) trans-1,3-Dichloroprop...	7.629	79	20130	5.113	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	102.200%
46) 2-Hexanone-d5	8.088	63	92430	63.415	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	126.840%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42275	5.449	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	60388	5.474	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.400%
Target Compounds						Qvalue
13) Acetone	2.179	43	1642	1.953	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110121\
Data File : VV023113.D
Acq On : 01 Nov 2021 13:43
Operator : SY/MD
Sample : M4364-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG339

Quant Time: Nov 02 01:15:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 01:11:36 2021
Response via : Initial Calibration

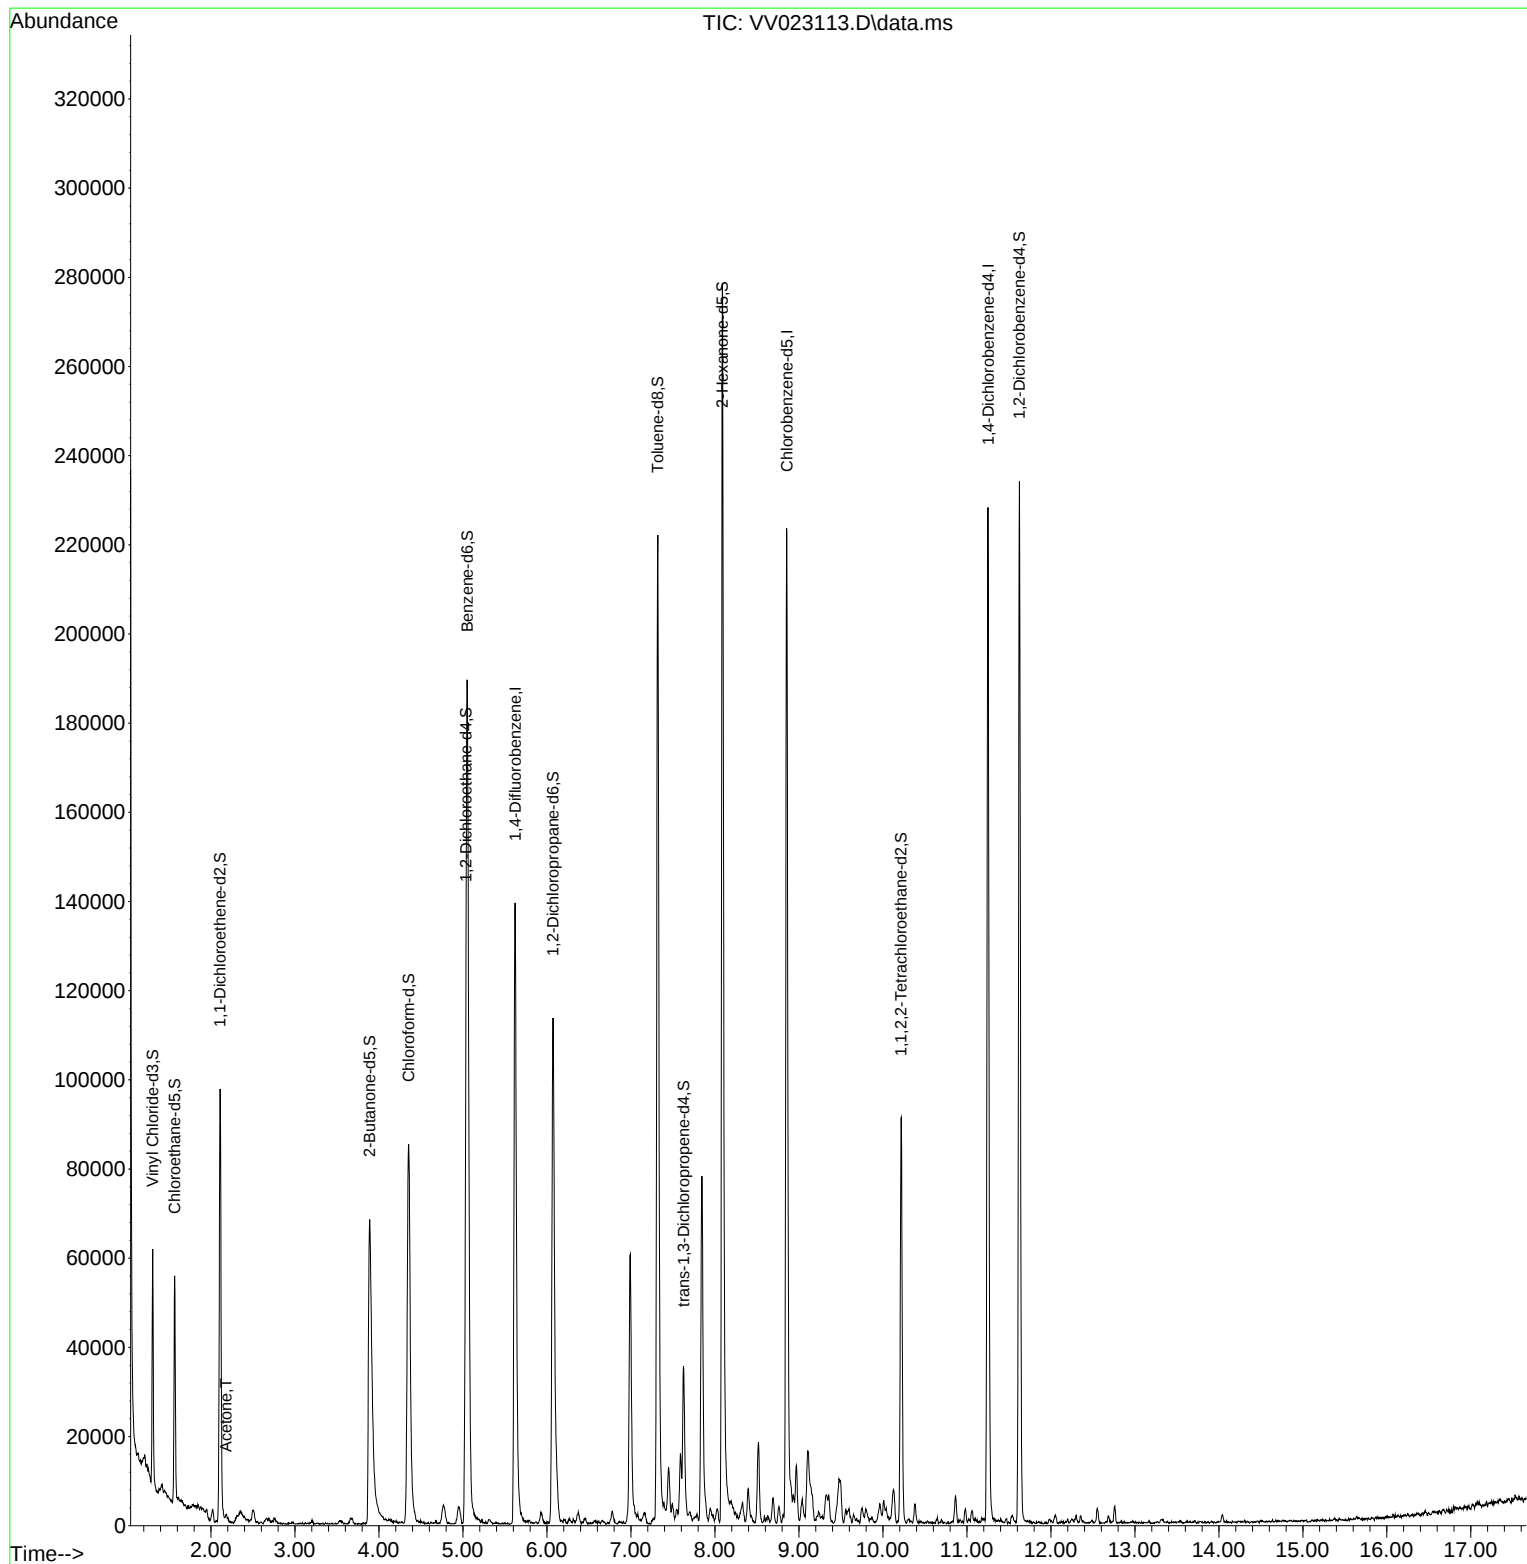

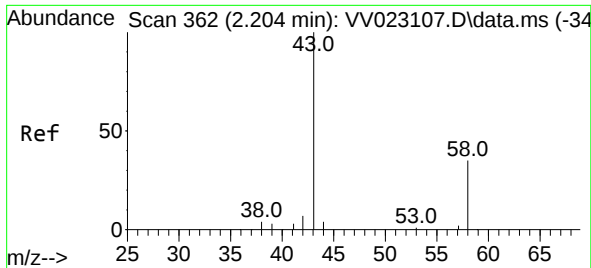

#13

Acetone

Concen: 1.953 ug/L

RT: 2.179 min Scan# 31

Delta R.T. -0.026 min

Lab File: VV023113.D

Acq: 01 Nov 2021 13:43

Instrument :

MSVOA_V

ClientSampleId :

BG339

Tgt Ion: 43 Resp: 1642

Ion Ratio Lower Upper

43 100

58 34.8 0.0 55.4

