

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110121\
 Data File : VV023127.D
 Acq On : 01 Nov 2021 19:43
 Operator : SY/MD
 Sample : M4412-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG361

Quant Time: Nov 02 01:18:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 01:11:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	125644	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	127933	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	59599	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	28758	2.619	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	52.400%
7) Chloroethane-d5	1.568	69	27806	4.094	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.800%
11) 1,1-Dichloroethene-d2	2.108	63	45490	2.872	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.400%#
20) 2-Butanone-d5	3.883	46	90775	51.542	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.080%
24) Chloroform-d	4.352	84	84622	4.741	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	5.034	65	41464	4.928	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.600%
32) Benzene-d6	5.053	84	157763	4.224	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.400%
36) 1,2-Dichloropropane-d6	6.072	67	50680	4.408	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.200%
41) Toluene-d8	7.320	98	136074	4.056	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.200%
43) trans-1,3-Dichloroprop...	7.625	79	18407	4.569	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.400%
46) 2-Hexanone-d5	8.088	63	71040	47.630	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.260%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	35761	4.504	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	53798	5.059	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.200%
Target Compounds					Qvalue	
13) Acetone	2.172	43	2262	2.618	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110121\
Data File : VV023127.D
Acq On : 01 Nov 2021 19:43
Operator : SY/MD
Sample : M4412-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG361

Quant Time: Nov 02 01:18:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 01:11:36 2021
Response via : Initial Calibration

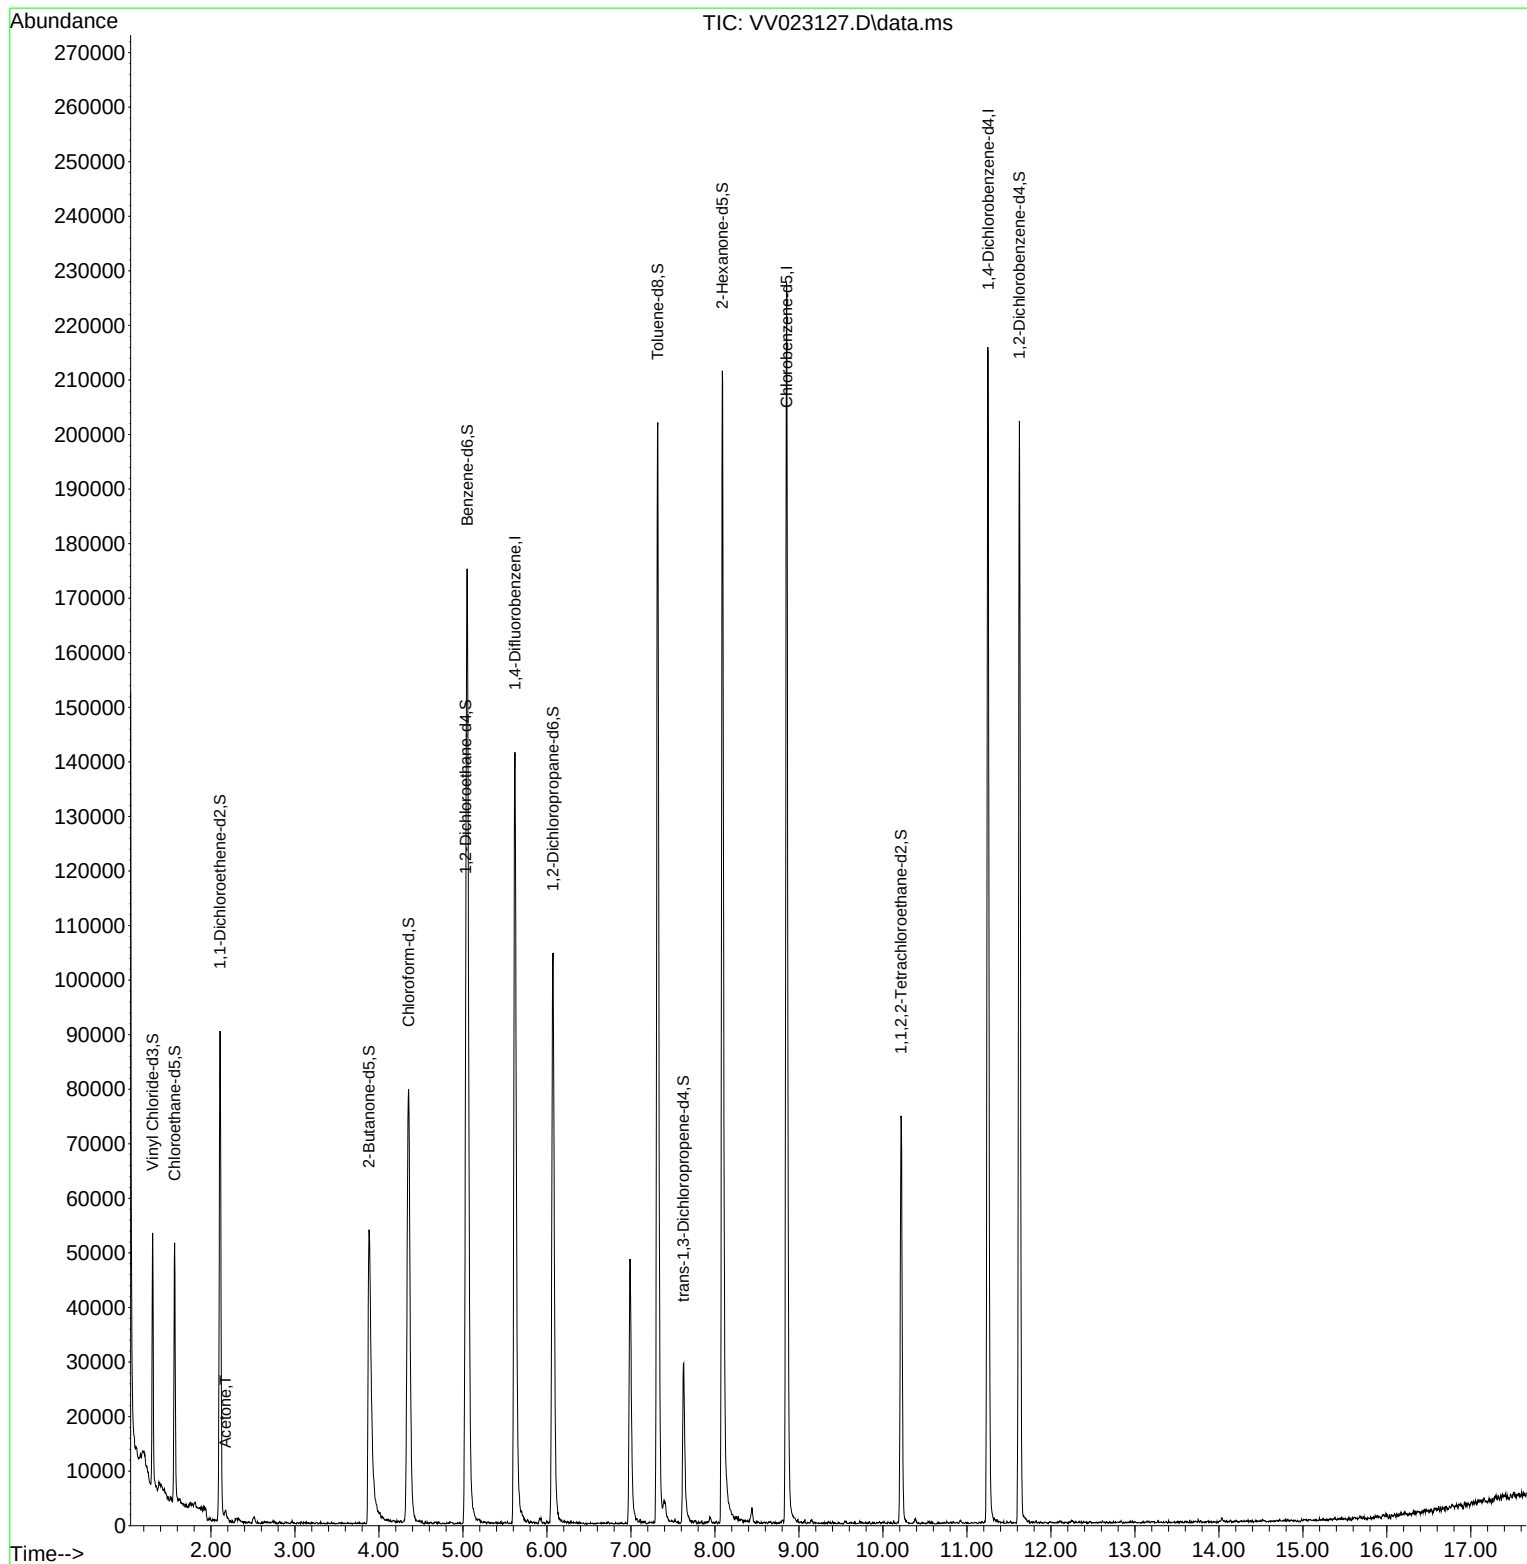

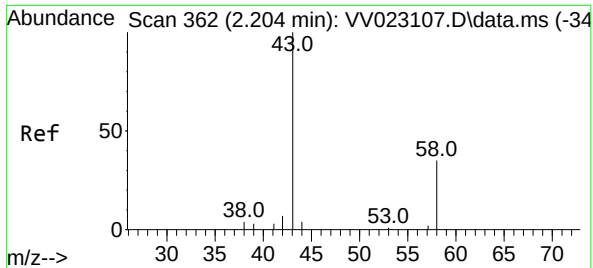

#13
 Acetone
 Concen: 2.618 ug/L
 RT: 2.172 min Scan# 31
 Delta R.T. -0.032 min
 Lab File: VV023127.D
 Acq: 01 Nov 2021 19:43

Instrument :
 MSVOA_V
 ClientSampleId :
 BG361

Tgt Ion: 43 Resp: 2262
 Ion Ratio Lower Upper
 43 100
 58 28.2 0.0 55.4

