

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110121\
 Data File : VW023128.D
 Acq On : 01 Nov 2021 20:07
 Operator : SY/MD
 Sample : M4412-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG362

Quant Time: Nov 02 01:18:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 01:11:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	120005	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	120511	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	56442	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	27731	2.645	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	52.800%
7) Chloroethane-d5	1.568	69	26917	4.150	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.000%
11) 1,1-Dichloroethene-d2	2.108	63	44845	2.964	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.200%#
20) 2-Butanone-d5	3.883	46	86850	51.630	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.260%
24) Chloroform-d	4.349	84	82467	4.837	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.800%
26) 1,2-Dichloroethane-d4	5.034	65	38437	4.783	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.600%
32) Benzene-d6	5.053	84	151816	4.315	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.400%
36) 1,2-Dichloropropane-d6	6.072	67	47843	4.417	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.400%
41) Toluene-d8	7.320	98	127333	4.029	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.600%
43) trans-1,3-Dichloroprop...	7.628	79	15558	4.100	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.000%
46) 2-Hexanone-d5	8.088	63	67624	48.132	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.260%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34221	4.576	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	51553	5.119	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.400%
Target Compounds					Qvalue	
13) Acetone	2.172	43	2961	3.588	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110121\
Data File : VV023128.D
Acq On : 01 Nov 2021 20:07
Operator : SY/MD
Sample : M4412-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG362

Quant Time: Nov 02 01:18:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 01:11:36 2021
Response via : Initial Calibration

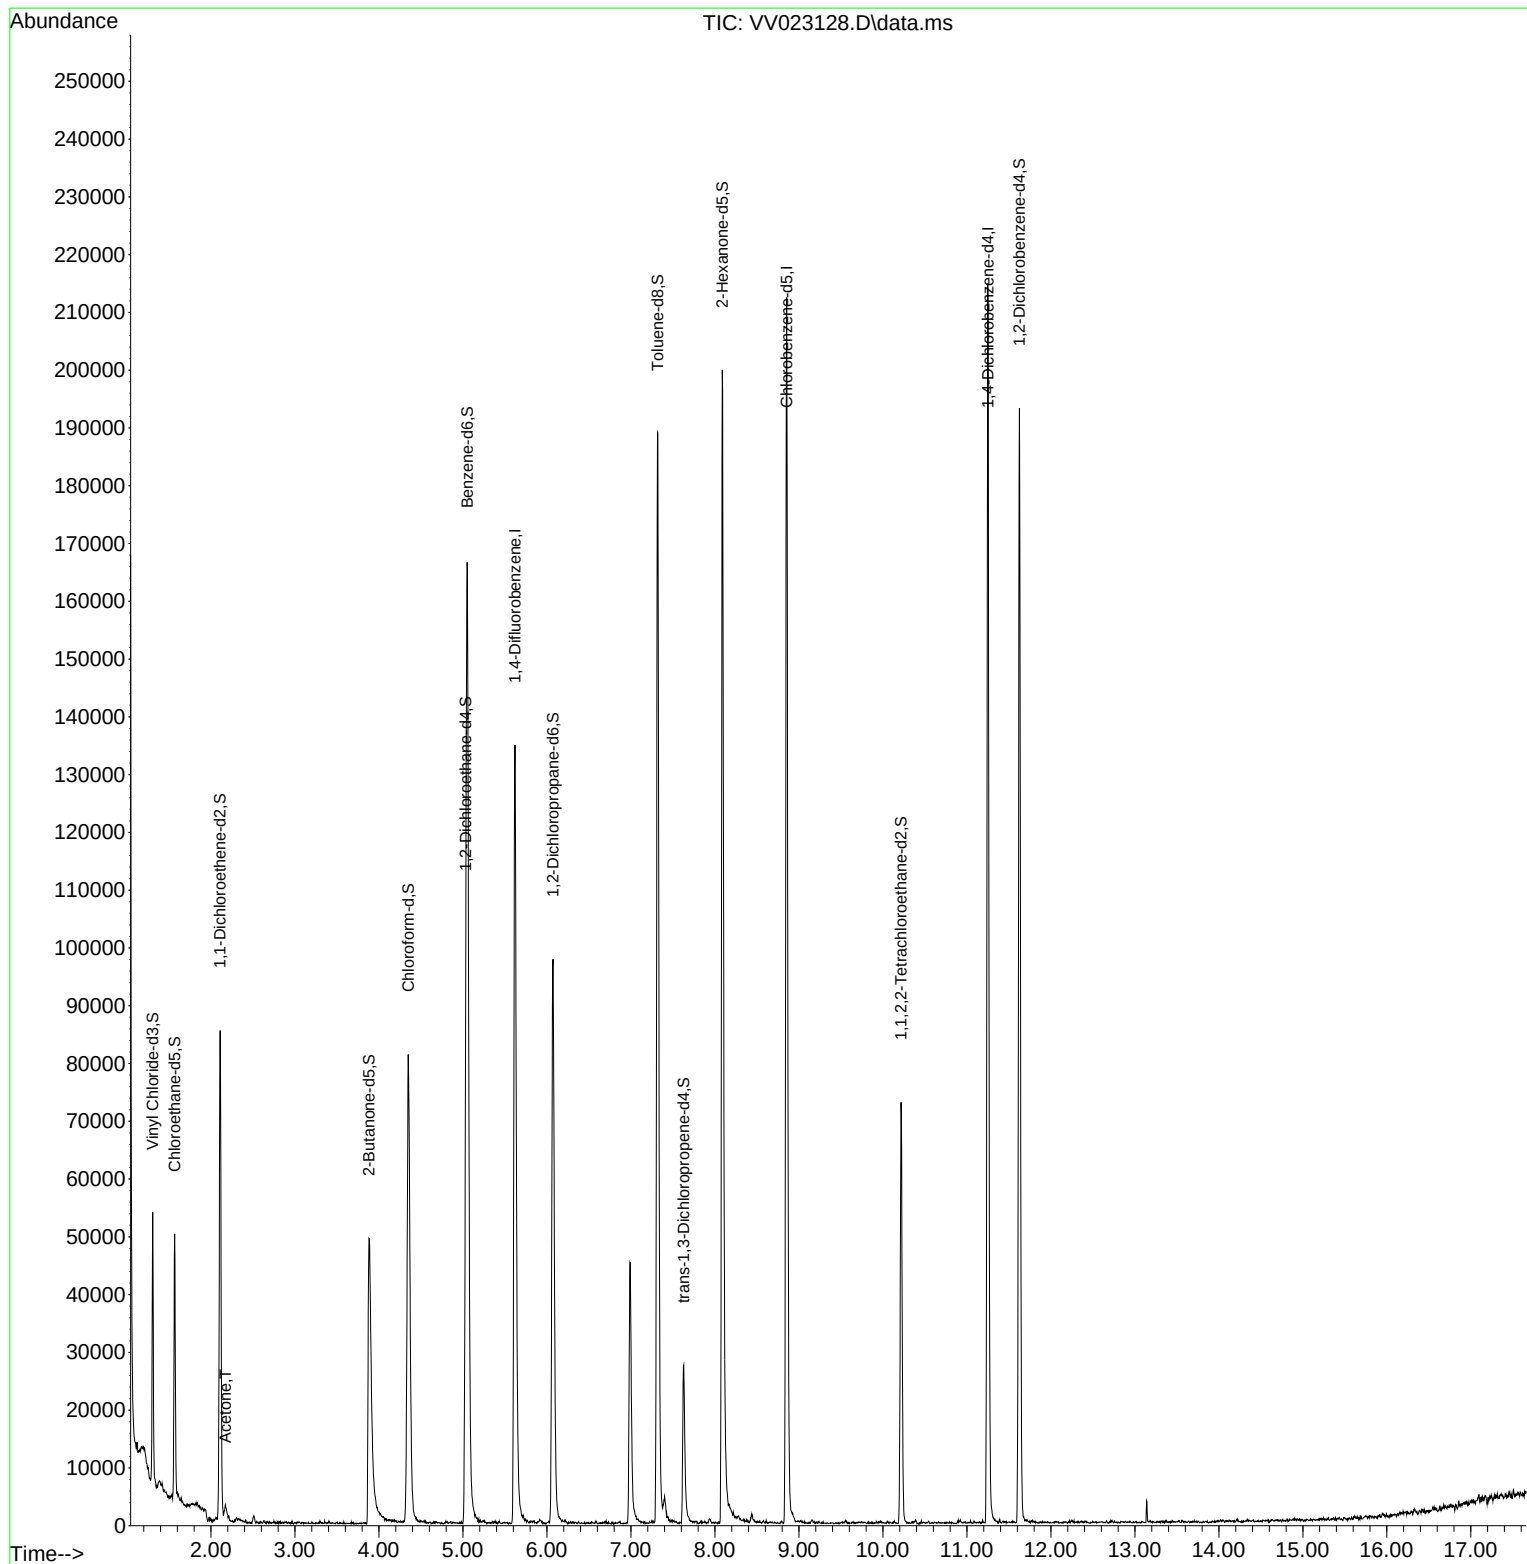

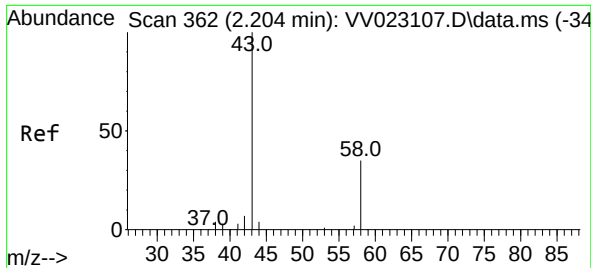

#13

Acetone

Concen: 3.588 ug/L

RT: 2.172 min Scan# 31

Delta R.T. -0.032 min

Lab File: VV023128.D


Acq: 01 Nov 2021 20:07

Instrument :

MSVOA_V

ClientSampleId :

BG362

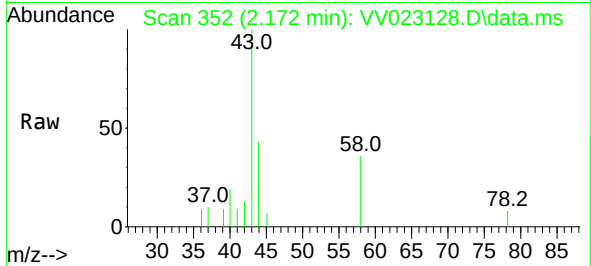

Tgt Ion: 43 Resp: 2961

Ion Ratio Lower Upper

43 100

58 30.0 0.0 55.4

