

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW110121\  
 Data File : VW023130.D  
 Acq On : 01 Nov 2021 20:55  
 Operator : SY/MD  
 Sample : M4412-08  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 26 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BG364

Quant Time: Nov 02 01:18:39 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR102221WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Tue Nov 02 01:11:36 2021  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|
| -----                         |        |       |          |          |        |          |
| Internal Standards            |        |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 5.619  | 114   | 122160   | 5.000    | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 8.854  | 117   | 126014   | 5.000    | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.249 | 152   | 58296    | 5.000    | ug/L   | 0.00     |
|                               |        |       |          |          |        |          |
| System Monitoring Compounds   |        |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.307  | 65    | 26973    | 2.527    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =      | 50.600%  |
| 7) Chloroethane-d5            | 1.568  | 69    | 25895    | 3.922    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =      | 78.400%  |
| 11) 1,1-Dichloroethene-d2     | 2.108  | 63    | 42712    | 2.774    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =      | 55.400%# |
| 20) 2-Butanone-d5             | 3.886  | 46    | 84647    | 49.433   | ug/L   | -0.02    |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =      | 98.860%  |
| 24) Chloroform-d              | 4.352  | 84    | 80644    | 4.647    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 93.000%  |
| 26) 1,2-Dichloroethane-d4     | 5.034  | 65    | 37549    | 4.590    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 91.800%  |
| 32) Benzene-d6                | 5.053  | 84    | 149871   | 4.074    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 81.400%  |
| 36) 1,2-Dichloropropane-d6    | 6.072  | 67    | 46891    | 4.140    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =      | 82.800%  |
| 41) Toluene-d8                | 7.317  | 98    | 126725   | 3.835    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 76.600%  |
| 43) trans-1,3-Dichloroprop... | 7.625  | 79    | 16583    | 4.179    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =      | 83.600%  |
| 46) 2-Hexanone-d5             | 8.088  | 63    | 67708    | 46.087   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =      | 92.180%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.217 | 84    | 33624    | 4.300    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =      | 86.000%  |
| 66) 1,2-Dichlorobenzene-d4    | 11.625 | 152   | 51539    | 4.955    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =      | 99.200%  |
|                               |        |       |          |          |        |          |
| Target Compounds              |        |       |          |          | Qvalue |          |
| 13) Acetone                   | 2.172  | 43    | 2642     | 3.145    | ug/L   | 89       |
| -----                         |        |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV110121\  
Data File : VV023130.D  
Acq On : 01 Nov 2021 20:55  
Operator : SY/MD  
Sample : M4412-08  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 26 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
BG364

Quant Time: Nov 02 01:18:39 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR102221WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Tue Nov 02 01:11:36 2021  
Response via : Initial Calibration

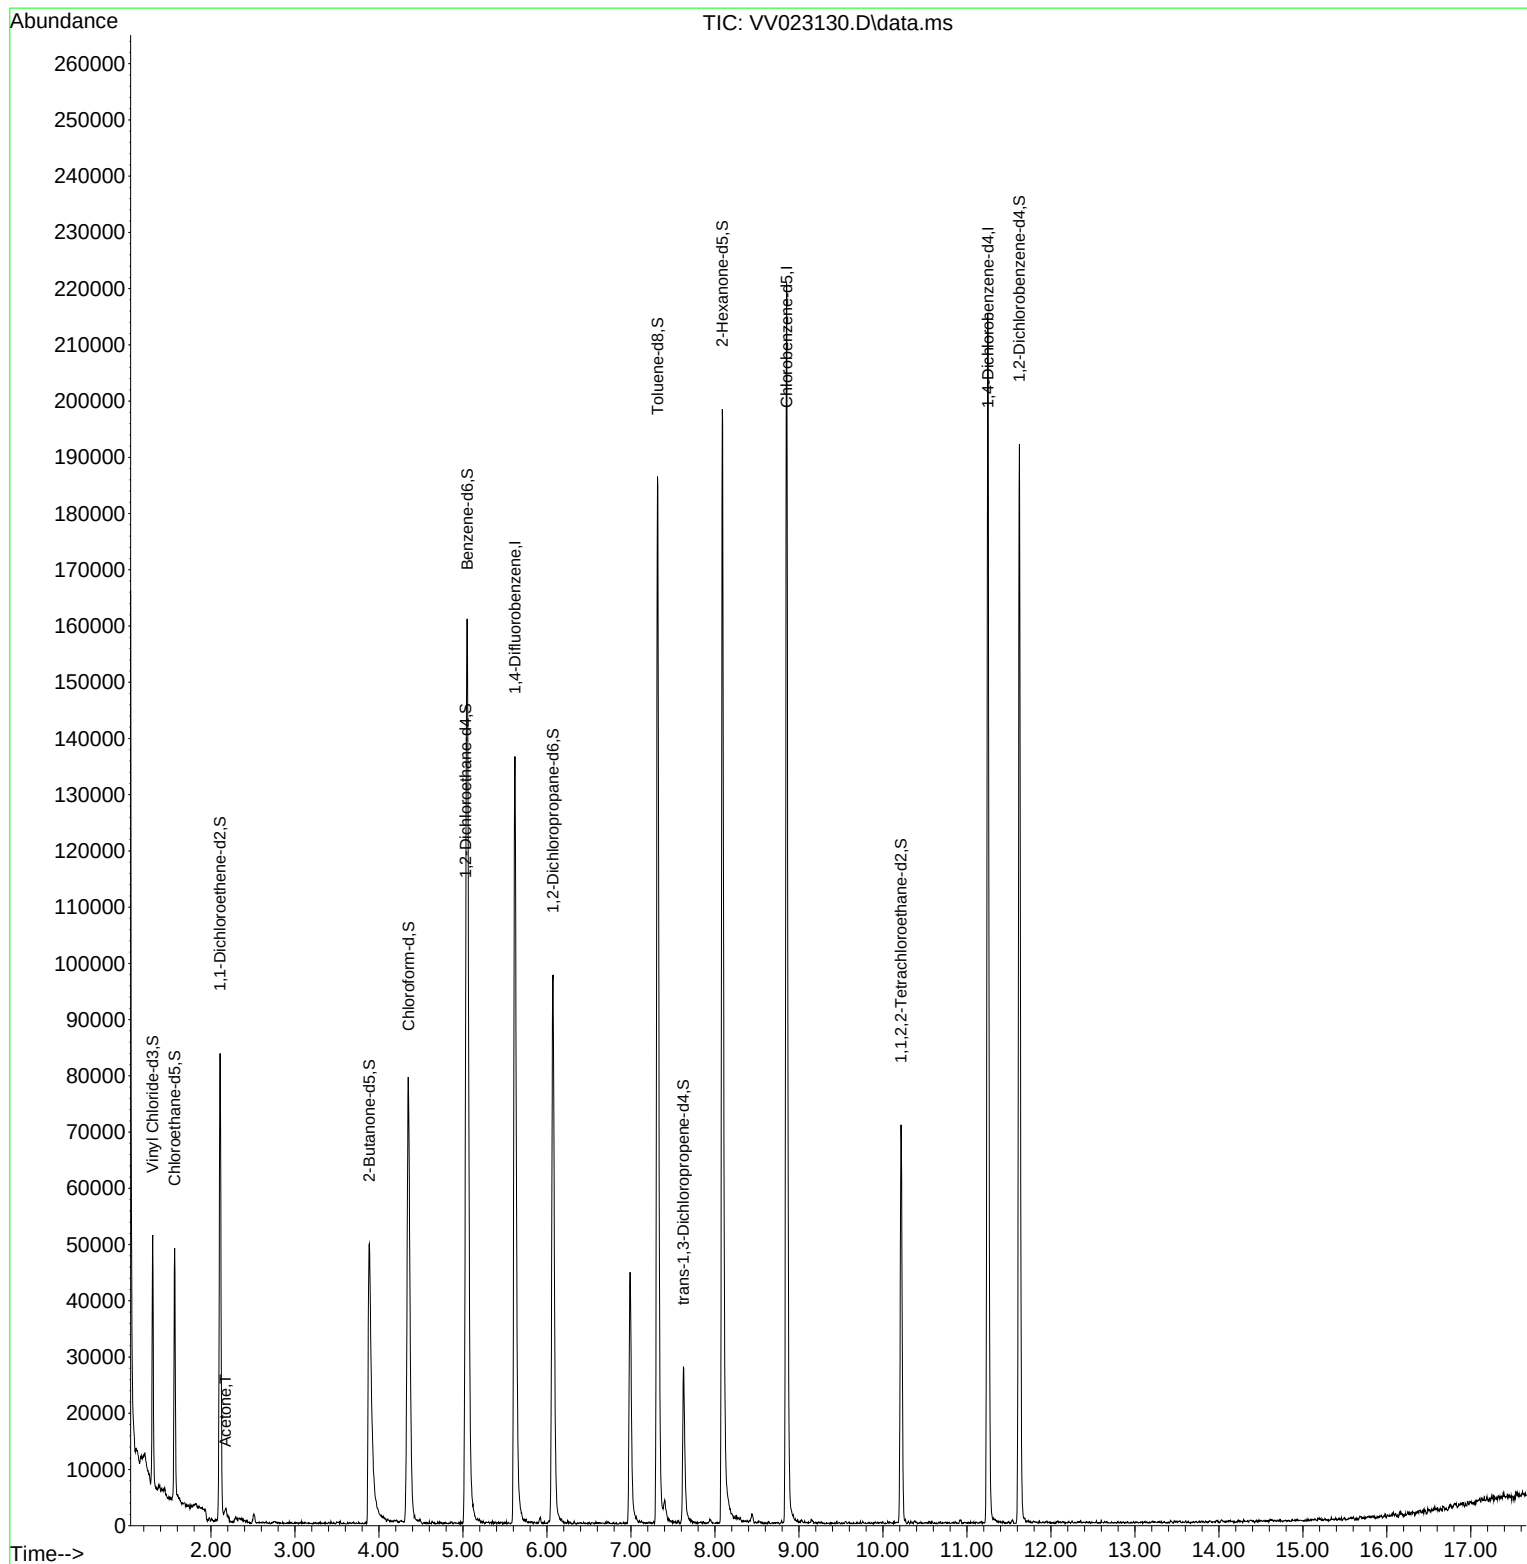

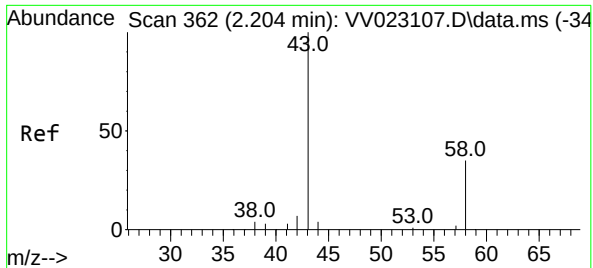

#13  
 Acetone  
 Concen: 3.145 ug/L  
 RT: 2.172 min Scan# 31  
 Delta R.T. -0.032 min  
 Lab File: VV023130.D  
 Acq: 01 Nov 2021 20:55

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 BG364

Tgt Ion: 43 Resp: 2642  
 Ion Ratio Lower Upper  
 43 100  
 58 33.6 0.0 55.4

