
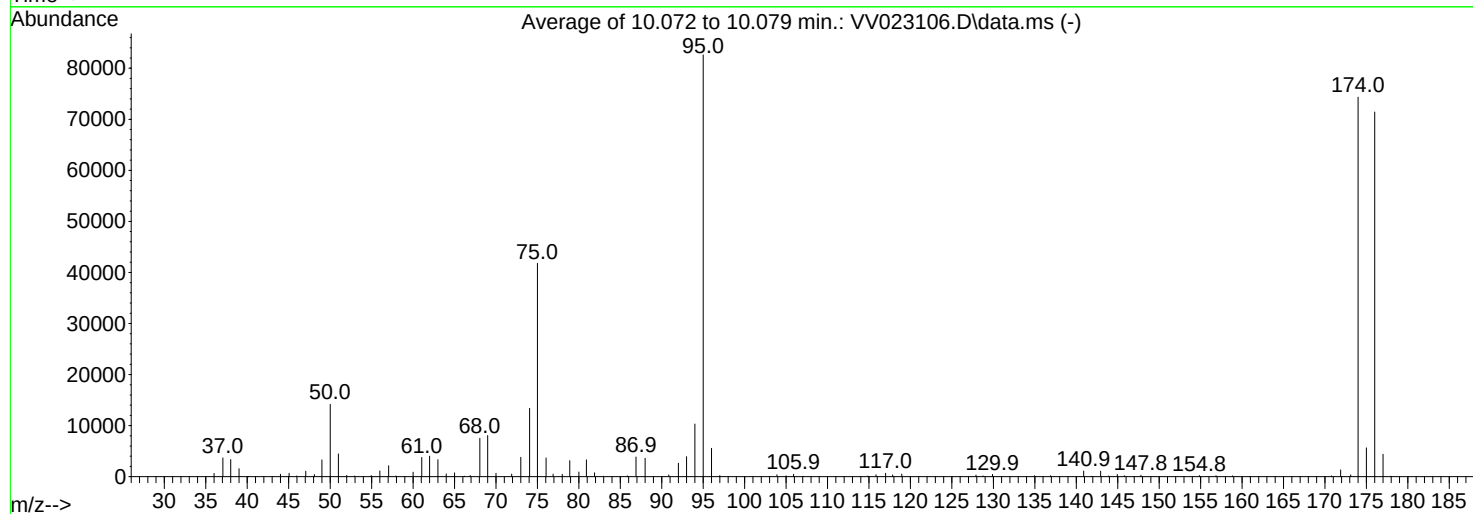


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110121\
 Data File : VV023106.D
 Acq On : 01 Nov 2021 09:58
 Operator : SY/MD
 Sample : BFB224
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB224

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Nov 02 23:31:16 2021

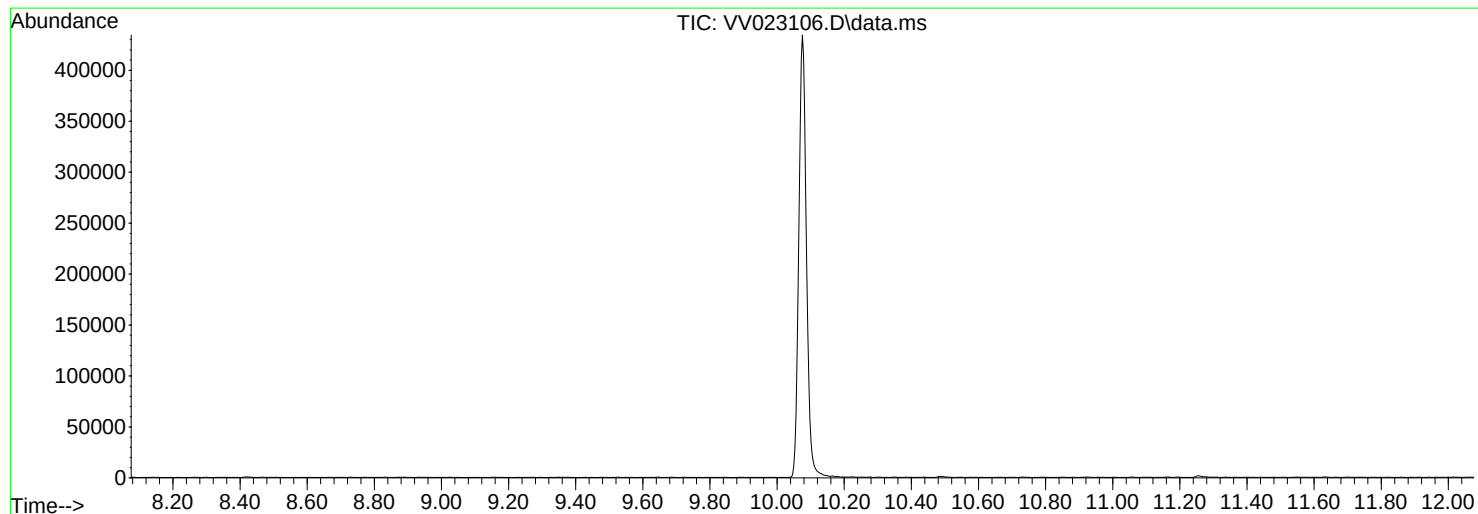

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	14171	PASS
75	95	30	80	50.6	41779	PASS
95	95	100	100	100.0	82624	PASS
96	95	5	9	6.7	5544	PASS
173	174	0.00	2	0.4	334	PASS
174	95	50	120	90.0	74336	PASS
175	174	5	9	7.6	5659	PASS
176	174	95	105	96.1	71413	PASS
177	176	5	10	6.2	4393	PASS

m/z	Abundance
40.00	200.0
44.00	243.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

m/z	Abundance
36.00	669.0
37.00	3672.0
38.00	3289.0
39.00	1532.0
40.10	200.0
44.00	745.0
45.00	664.0
45.90	143.0
47.10	1114.0
48.10	393.0
49.00	3382.0
50.00	14136.0
51.00	4543.0
52.00	266.0
53.00	140.0
55.00	229.0
56.00	1045.0
57.10	2181.0
58.00	132.0
60.00	871.0
61.00	3754.0
62.00	3997.0
63.00	3444.0
64.00	482.0
65.00	767.0
66.20	125.0
66.90	224.0
68.10	7322.0
69.00	8059.0
70.00	646.0
71.90	477.0
73.00	3853.0
74.00	13432.0
75.00	41376.0
76.00	3601.0
76.90	536.0
78.00	464.0
78.90	3136.0
80.00	885.0
80.90	3140.0
81.90	698.0
83.00	124.0
85.80	198.0
86.90	3744.0
88.00	3508.0
90.90	325.0
92.00	2714.0
93.00	3850.0
94.00	9857.0
95.00	81312.0
96.00	5485.0
97.00	211.0
103.90	356.0
105.00	139.0
105.90	414.0
107.00	105.0
114.80	117.0
115.80	409.0
117.00	679.0
117.90	329.0
118.90	515.0
124.00	103.0
127.90	304.0
128.70	165.0
129.90	448.0
134.90	215.0
136.90	169.0
140.90	1095.0
141.80	112.0
143.00	1004.0
143.90	150.0
144.90	396.0
145.80	220.0
147.80	241.0
154.90	191.0
156.90	162.0
158.80	119.0
170.80	168.0
171.90	1212.0
174.00	71040.0
175.00	5644.0
176.00	68520.0
177.00	4168.0
178.00	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

m/z	Abundance
36.00	641.0
37.10	3789.0
38.00	3466.0
39.00	1616.0
40.10	206.0
44.00	717.0
45.10	678.0
46.00	143.0
47.10	1058.0
48.10	431.0
49.00	3380.0
50.00	14670.0
51.00	4573.0
52.00	248.0
53.00	117.0
54.90	249.0
56.00	1166.0
57.00	2203.0
57.90	130.0
60.00	916.0
61.10	3931.0
62.00	4161.0
63.00	3463.0
64.00	548.0
65.00	797.0
66.20	114.0
66.90	232.0
68.00	7702.0
69.00	8335.0
70.00	646.0
71.90	515.0
73.00	3982.0
74.10	13902.0
75.00	43328.0
76.10	3810.0
76.90	530.0
78.00	507.0
78.90	3214.0
80.00	946.0
80.90	3403.0
81.90	783.0
83.00	107.0
85.90	158.0
86.90	4039.0
88.00	3795.0
90.80	358.0
92.00	2740.0
93.00	4095.0
94.00	10698.0
95.00	85584.0
96.00	5745.0
97.00	216.0
103.90	393.0
105.00	149.0
105.90	476.0
107.10	108.0
114.90	139.0
115.90	405.0
117.00	681.0
117.80	350.0
119.00	551.0
127.90	335.0
128.80	167.0
129.90	441.0
134.90	210.0
136.90	194.0
140.90	1160.0
141.80	124.0
143.00	1103.0
143.90	142.0
145.00	436.0
145.80	195.0
147.80	272.0
154.90	221.0
156.90	180.0
158.90	177.0
170.80	174.0
171.90	1401.0
174.00	77024.0
175.00	5828.0
176.00	74136.0
177.00	4543.0
178.00	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

m/z	Abundance
36.00	594.0
37.10	3512.0
38.00	3269.0
39.00	1535.0
40.20	200.0
44.00	647.0
45.10	626.0
46.00	133.0
47.00	990.0
48.10	419.0
49.00	3123.0
50.00	13708.0
51.00	4232.0
52.00	216.0
52.90	119.0
54.90	221.0
56.00	1151.0
57.00	2037.0
58.00	122.0
60.00	895.0
61.00	3574.0
62.00	3893.0
63.00	3065.0
64.00	601.0
65.00	741.0
66.90	230.0
68.00	7505.0
69.00	7813.0
70.00	643.0
71.90	504.0
73.00	3597.0
74.10	12862.0
75.00	40632.0
76.10	3625.0
76.90	456.0
78.00	486.0
78.90	3018.0
80.00	928.0
80.90	3336.0
81.90	781.0
82.90	103.0
85.90	139.0
86.90	3788.0
88.00	3480.0
90.80	353.0
92.00	2464.0
93.00	3832.0
94.00	10361.0
95.00	80976.0
96.00	5401.0
97.00	218.0
103.90	435.0
105.00	164.0
105.90	484.0
114.90	153.0
115.90	361.0
117.00	653.0
117.80	361.0
119.00	491.0
127.90	308.0
128.80	167.0
129.90	413.0
135.00	183.0
136.90	191.0
140.90	1055.0
142.90	1096.0
143.90	112.0
145.00	453.0
145.80	164.0
147.00	111.0
147.80	291.0
154.80	263.0
156.80	187.0
158.90	192.0
160.90	101.0
170.80	155.0
171.90	1350.0
173.10	1003.0
174.00	74944.0
175.00	5504.0
176.00	71584.0
177.00	4468.0
177.90	100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224