

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
 Data File : VV032822.D
 Acq On : 01 Nov 2023 12:05
 Operator : SY/MD
 Sample : 05132-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 02 01:10:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 02 01:08:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	328559	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	363297	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	160935	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	131603	42.113	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	84.220%		
7) Chloroethane-d5	1.532	69	117339	44.895	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	89.800%		
11) 1,1-Dichloroethene-d2	2.060	65	56520	43.788	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.580%		
21) 2-Butanone-d5	3.786	46	121111	89.349	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	89.350%		
24) Chloroform-d	4.252	84	224085	44.924	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.840%		
26) 1,2-Dichloroethane-d4	4.944	65	144625	46.651	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.300%		
32) Benzene-d6	4.963	84	441740	47.291	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.580%		
36) 1,2-Dichloropropane-d6	5.989	67	136170	47.984	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.960%		
41) Toluene-d8	7.246	98	415839	45.212	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.420%		
43) trans-1,3-Dichloroprop...	7.555	79	67027	45.351	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.700%		
47) 2-Hexanone-d5	8.027	63	92443	89.230	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	89.230%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	198864	46.179	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.360%		
66) 1,2-Dichlorobenzene-d4	11.564	152	158908	51.239	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.480%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.555	75	3199	0.812	ug/L	# 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
Data File : VV032822.D
Acq On : 01 Nov 2023 12:05
Operator : SY/MD
Sample : 05132-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Nov 02 01:10:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 02 01:08:52 2023
Response via : Initial Calibration

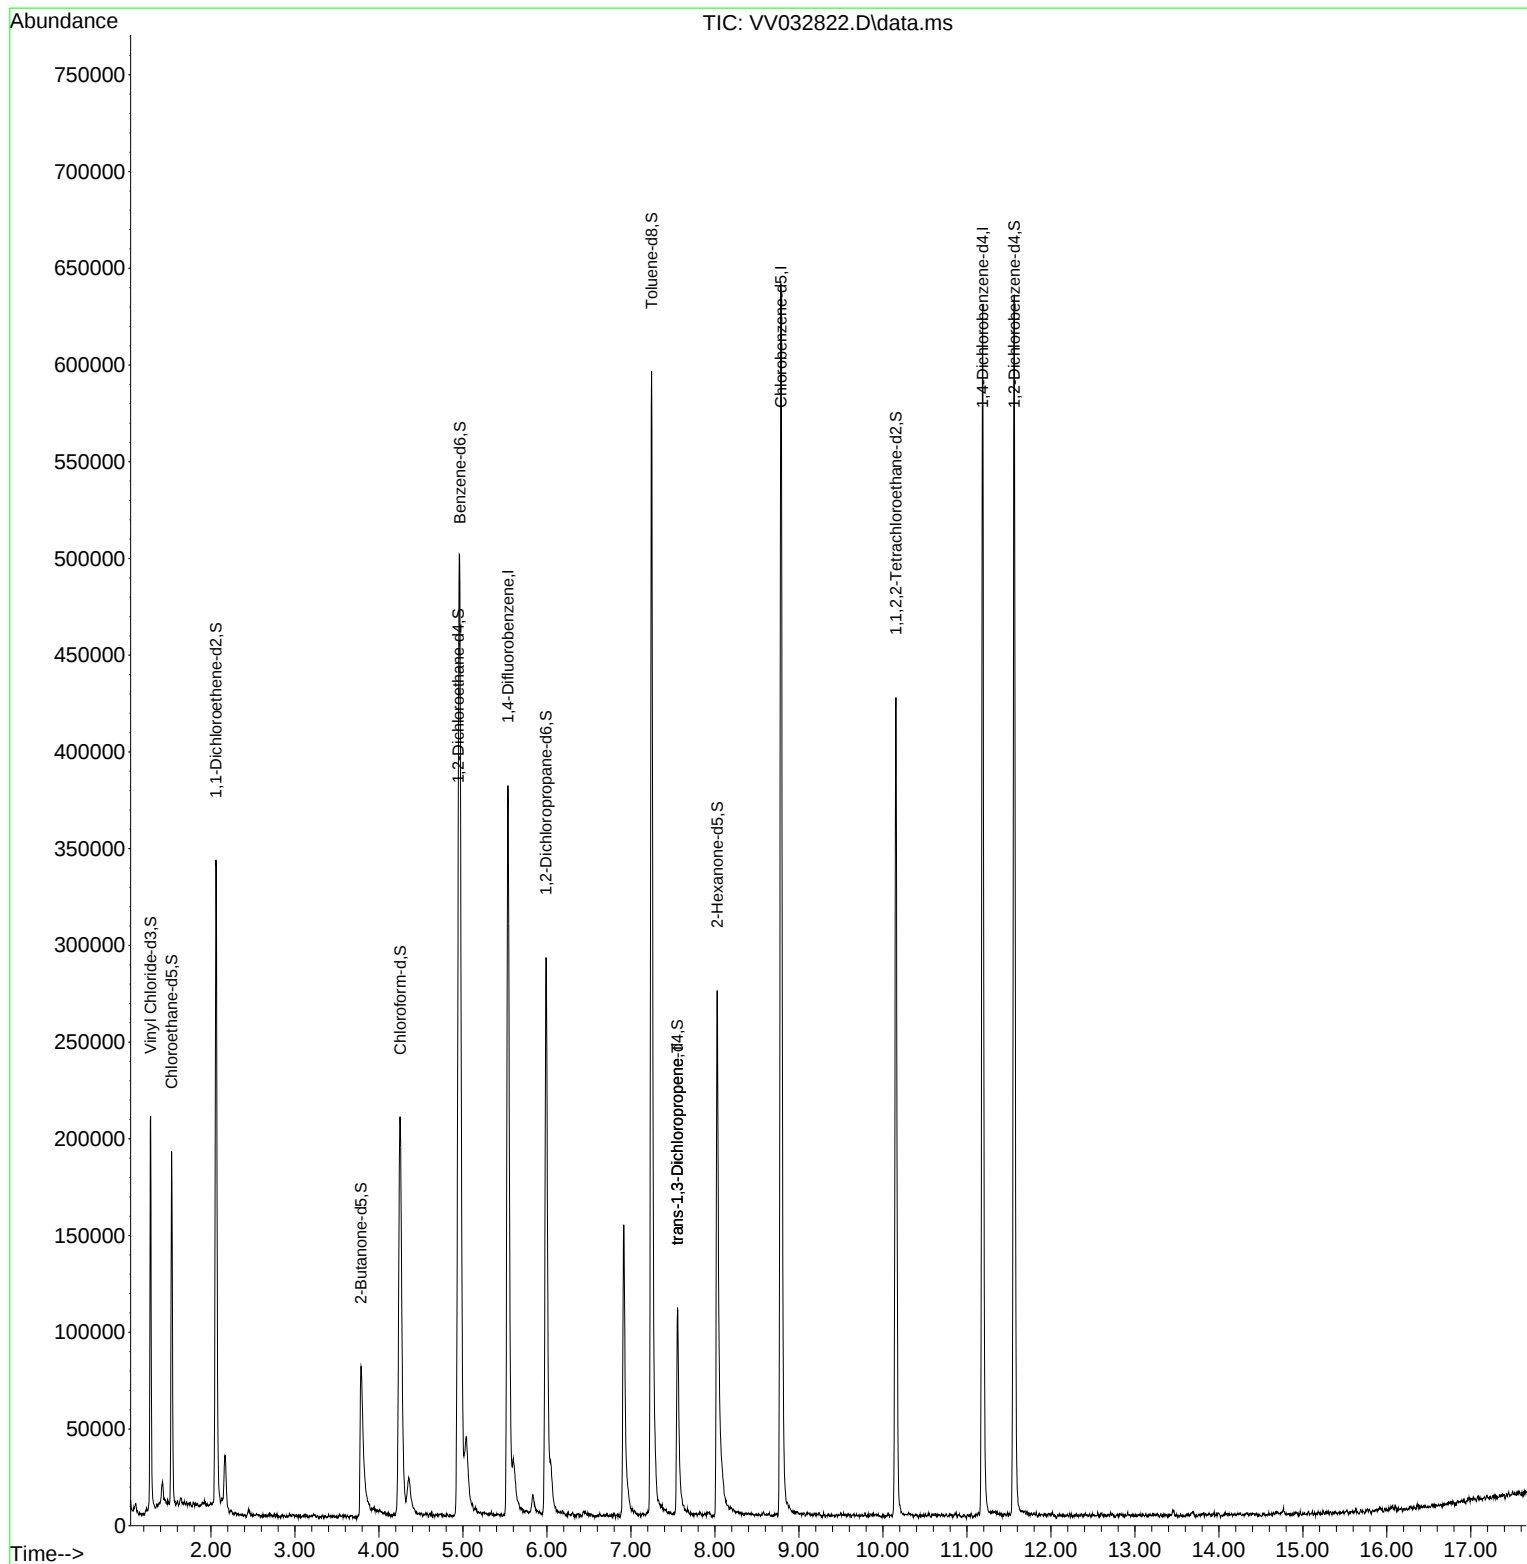

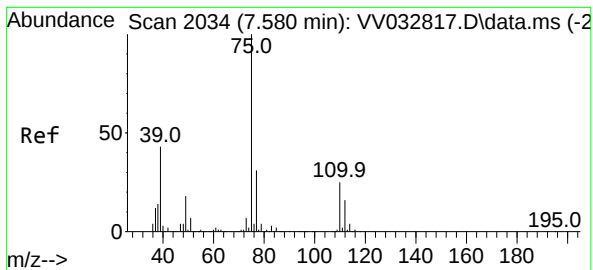

#44
 trans-1,3-Dichloropropene
 Concen: 0.812 ug/L
 RT: 7.555 min Scan# 2034
 Delta R.T. -0.026 min
 Lab File: VV032822.D
 Acq: 01 Nov 2023 12:05

Instrument :
 MSVOA_V
 ClientSampleId :

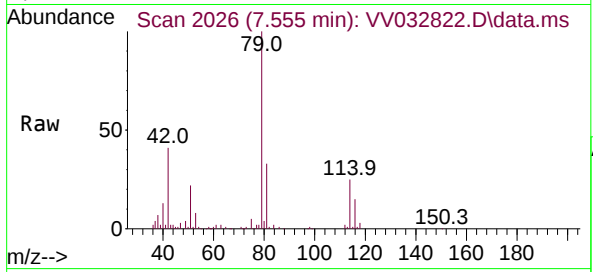

Tgt Ion: 75 Resp: 3199
 Ion Ratio Lower Upper
 75 100
 77 42.2 22.0 40.8#

