

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
 Data File : VV032818.D
 Acq On : 01 Nov 2023 10:32
 Operator : SY/MD
 Sample : VV1101WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK209

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032818.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	86	rBV	218354	237605	17.27%	2.197%
2	1.532	147	153	168	rVB	193529	228448	16.60%	2.112%
3	2.060	309	317	335	rVB	355618	516134	37.50%	4.772%
4	2.423	424	430	433	rBV7	2279	2775	0.20%	0.026%
5	2.506	453	456	461	rBV7	2070	1947	0.14%	0.018%
6	2.532	462	464	467	rVB3	2146	832	0.06%	0.008%
7	2.561	467	473	475	rBV6	2383	2085	0.15%	0.019%
8	2.596	480	484	485	rBV4	1086	612	0.04%	0.006%
9	2.632	491	495	497	rBV5	2028	1693	0.12%	0.016%
10	2.770	534	538	540	rBV5	1659	1211	0.09%	0.011%
11	2.867	564	568	571	rBV5	1994	1748	0.13%	0.016%
12	3.040	618	622	624	rBV5	1369	1010	0.07%	0.009%
13	3.056	625	627	630	rVB4	2233	938	0.07%	0.009%
14	3.079	630	634	635	rBV4	875	543	0.04%	0.005%
15	3.169	658	662	664	rBV5	1885	1381	0.10%	0.013%
16	3.204	670	673	675	rBV5	1419	778	0.06%	0.007%
17	3.378	724	727	728	rBV2	1193	574	0.04%	0.005%
18	3.404	733	735	741	rBV6	1328	1192	0.09%	0.011%
19	3.455	747	751	752	rVB3	1202	652	0.05%	0.006%
20	3.484	757	760	763	rBV3	1295	1000	0.07%	0.009%
21	3.522	770	772	775	rVB4	1749	900	0.07%	0.008%
22	3.561	781	784	786	rBV4	1876	867	0.06%	0.008%
23	3.571	786	787	792	rVV4	1182	780	0.06%	0.007%
24	3.609	796	799	803	rBV6	1305	1105	0.08%	0.010%
25	3.664	814	816	819	rBV4	1523	779	0.06%	0.007%
26	3.725	832	835	837	rBV4	1079	538	0.04%	0.005%
27	3.789	846	855	877	rBV2	78871	206208	14.98%	1.907%
28	4.140	961	964	966	rBV4	1994	839	0.06%	0.008%
29	4.252	984	999	1018	rBV	222114	573191	41.65%	5.300%
30	4.551	1091	1092	1094	rBV	1263	631	0.05%	0.006%
31	4.712	1139	1142	1145	rBV4	1301	932	0.07%	0.009%
32	4.731	1145	1148	1150	rBV4	1894	1245	0.09%	0.012%
33	4.821	1173	1176	1178	rBV4	1838	1363	0.10%	0.013%
34	4.960	1202	1219	1236	rBV2	515367	1376200	100.00%	12.724%
35	5.403	1355	1357	1359	rBV3	1710	712	0.05%	0.007%
36	5.535	1387	1398	1413	rBV	381018	779090	56.61%	7.203%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
 Data File : VV032818.D
 Acq On : 01 Nov 2023 10:32
 Operator : SY/MD
 Sample : VV1101WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK209

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	5.989	1528	1539	1573	rBV	298533	669202	48.63%	6.187%
38	6.329	1643	1645	1647	rBV3	1558	669	0.05%	0.006%
39	6.558	1714	1716	1719	rBV4	1334	1040	0.08%	0.010%
40	6.616	1732	1734	1739	rBV6	1744	1494	0.11%	0.014%
41	6.719	1763	1766	1771	rBV7	2771	2602	0.19%	0.024%
42	6.741	1771	1773	1774	rBV2	1273	602	0.04%	0.006%
43	6.780	1783	1785	1787	rBV3	1153	658	0.05%	0.006%
44	6.850	1804	1807	1812	rBV6	2325	2700	0.20%	0.025%
45	6.876	1812	1815	1816	rVV3	1241	585	0.04%	0.005%
46	6.915	1816	1827	1857	rVV	154186	327110	23.77%	3.024%
47	7.246	1919	1930	1964	rBV	623120	1161883	84.43%	10.743%
48	7.554	2017	2026	2044	rBV	112532	212107	15.41%	1.961%
49	8.027	2164	2173	2204	rBV	273798	565141	41.07%	5.225%
50	8.532	2326	2330	2334	rBV6	1886	1833	0.13%	0.017%
51	8.657	2366	2369	2372	rBV5	1198	620	0.05%	0.006%
52	8.786	2398	2409	2434	rBV	651463	1110318	80.68%	10.266%
53	9.043	2487	2489	2491	rBV3	2180	969	0.07%	0.009%
54	9.143	2516	2520	2522	rBV4	2503	1598	0.12%	0.015%
55	9.336	2578	2580	2582	rBV3	1004	543	0.04%	0.005%
56	9.413	2600	2604	2606	rBV5	2225	1925	0.14%	0.018%
57	9.632	2669	2672	2679	rVB7	2821	2715	0.20%	0.025%
58	9.661	2679	2681	2683	rBV3	1315	577	0.04%	0.005%
59	9.706	2693	2695	2698	rBV3	1473	755	0.05%	0.007%
60	9.866	2742	2745	2746	rBV3	1768	1227	0.09%	0.011%
61	9.911	2756	2759	2762	rBV5	1526	1241	0.09%	0.011%
62	9.927	2762	2764	2766	rVV4	1587	691	0.05%	0.006%
63	10.017	2788	2792	2793	rBV4	2118	1265	0.09%	0.012%
64	10.152	2824	2834	2855	rBV	441463	701498	50.97%	6.486%
65	10.471	2929	2933	2934	rBV4	1626	1122	0.08%	0.010%
66	10.689	2999	3001	3002	rBV2	1411	741	0.05%	0.007%
67	10.918	3068	3072	3074	rBV4	1377	940	0.07%	0.009%
68	10.931	3074	3076	3079	rVV4	1353	544	0.04%	0.005%
69	11.114	3131	3133	3135	rBV2	1609	834	0.06%	0.008%
70	11.188	3145	3156	3172	rBV	620977	976466	70.95%	9.028%
71	11.500	3251	3253	3257	rVV4	1768	1013	0.07%	0.009%
72	11.561	3261	3272	3295	rVV	668614	1059222	76.97%	9.794%
73	12.021	3412	3415	3417	rBV3	1282	624	0.05%	0.006%
74	12.037	3417	3420	3422	rVV4	1408	906	0.07%	0.008%
75	12.059	3424	3427	3432	rBV6	1665	1194	0.09%	0.011%
76	12.107	3439	3442	3445	rBV5	2040	1699	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
 Data File : VV032818.D
 Acq On : 01 Nov 2023 10:32
 Operator : SY/MD
 Sample : VV1101WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK209

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M

Title : VOC Analysis

77	12.162	3457	3459	3462	rVB4	1288	562	0.04%	0.005%
78	12.281	3494	3496	3499	rVB4	1829	1069	0.08%	0.010%
79	12.313	3503	3506	3508	rBV4	1812	1271	0.09%	0.012%
80	12.564	3582	3584	3586	rBV3	1505	739	0.05%	0.007%
81	12.676	3616	3619	3621	rBV3	1278	970	0.07%	0.009%
82	12.757	3642	3644	3648	rVB4	2020	1243	0.09%	0.011%
83	12.869	3677	3679	3683	rBV4	913	553	0.04%	0.005%
84	12.898	3686	3688	3693	rVB5	1797	1057	0.08%	0.010%
85	12.975	3710	3712	3714	rBV2	1490	666	0.05%	0.006%
86	13.069	3738	3741	3743	rVB3	1448	694	0.05%	0.006%
87	13.088	3743	3747	3749	rBV4	2017	1358	0.10%	0.013%
88	13.178	3772	3775	3778	rBV4	2016	1607	0.12%	0.015%
89	13.300	3810	3813	3814	rBV3	1625	1021	0.07%	0.009%
90	13.355	3828	3830	3835	rVB6	2047	1219	0.09%	0.011%
91	13.448	3848	3859	3868	rBV2	13016	24917	1.81%	0.230%
92	13.561	3892	3894	3899	rBV6	1460	1305	0.09%	0.012%
93	13.924	4005	4007	4009	rVB3	1661	547	0.04%	0.005%
94	14.049	4042	4046	4047	rBV3	1998	1522	0.11%	0.014%
95	14.094	4057	4060	4061	rBV2	1215	651	0.05%	0.006%
96	14.152	4076	4078	4080	rVB2	1707	694	0.05%	0.006%
97	14.390	4149	4152	4155	rBV5	1827	1177	0.09%	0.011%
98	14.918	4313	4316	4320	rBV6	1723	1358	0.10%	0.013%
99	15.165	4391	4393	4394	rBV2	1800	871	0.06%	0.008%
100	15.390	4461	4463	4466	rBV4	2019	1050	0.08%	0.010%




Sum of corrected areas: 10815532

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
Data File : VV032818.D
Acq On : 01 Nov 2023 10:32
Operator : SY/MD
Sample : VV1101WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK209

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

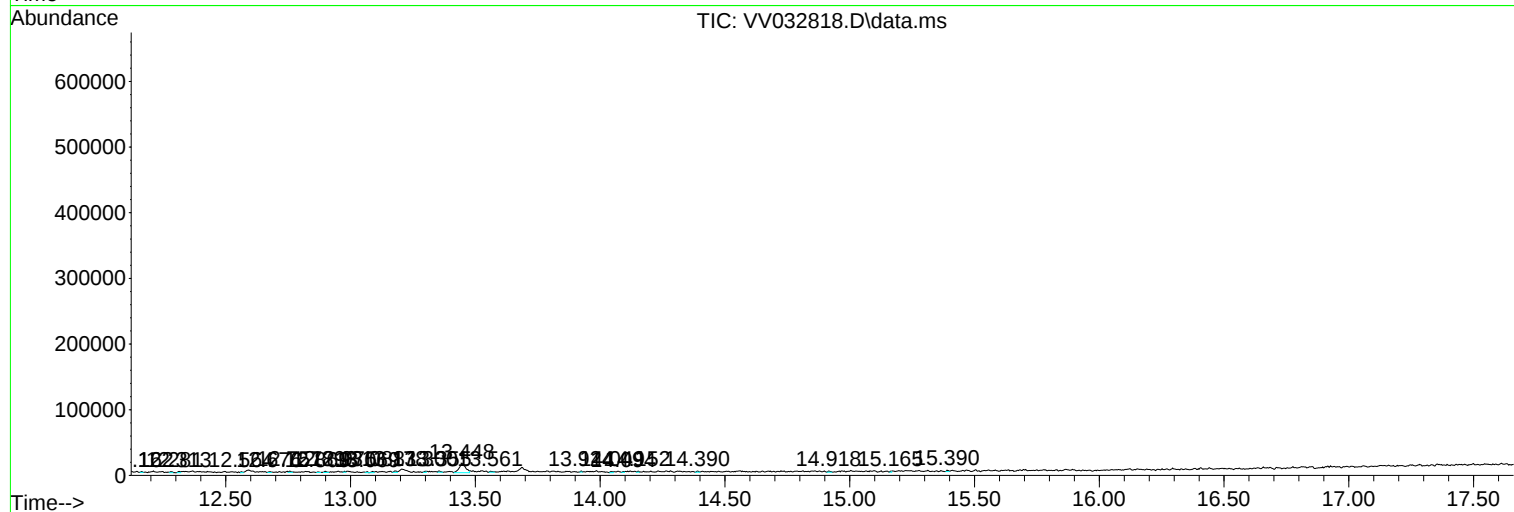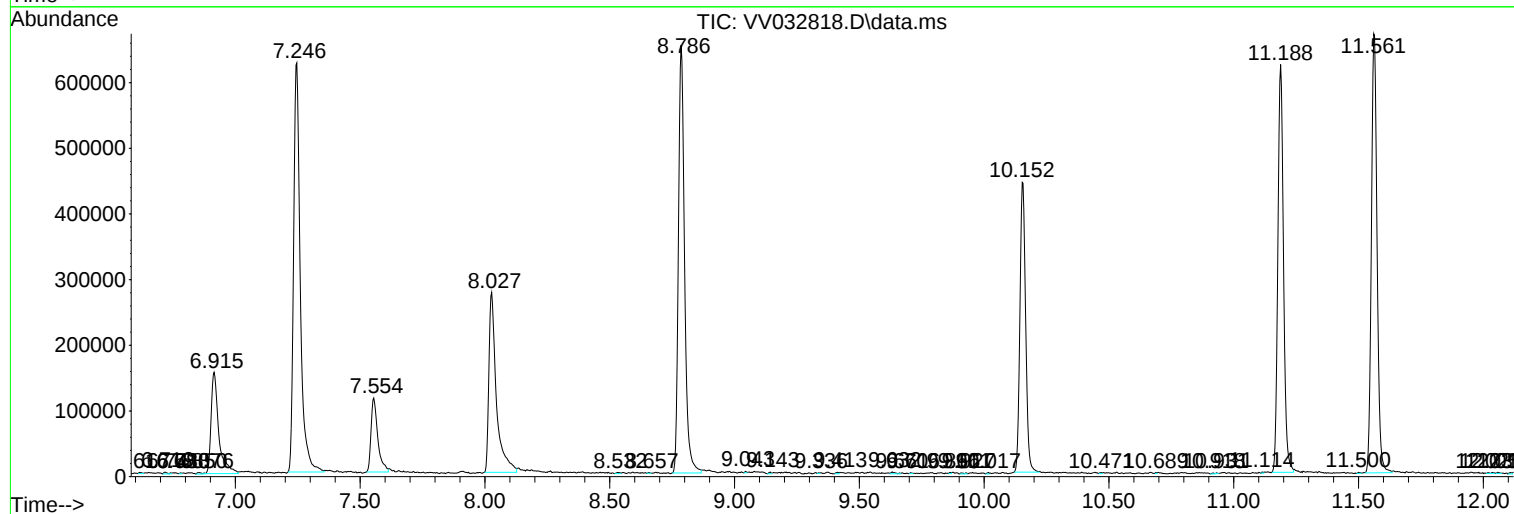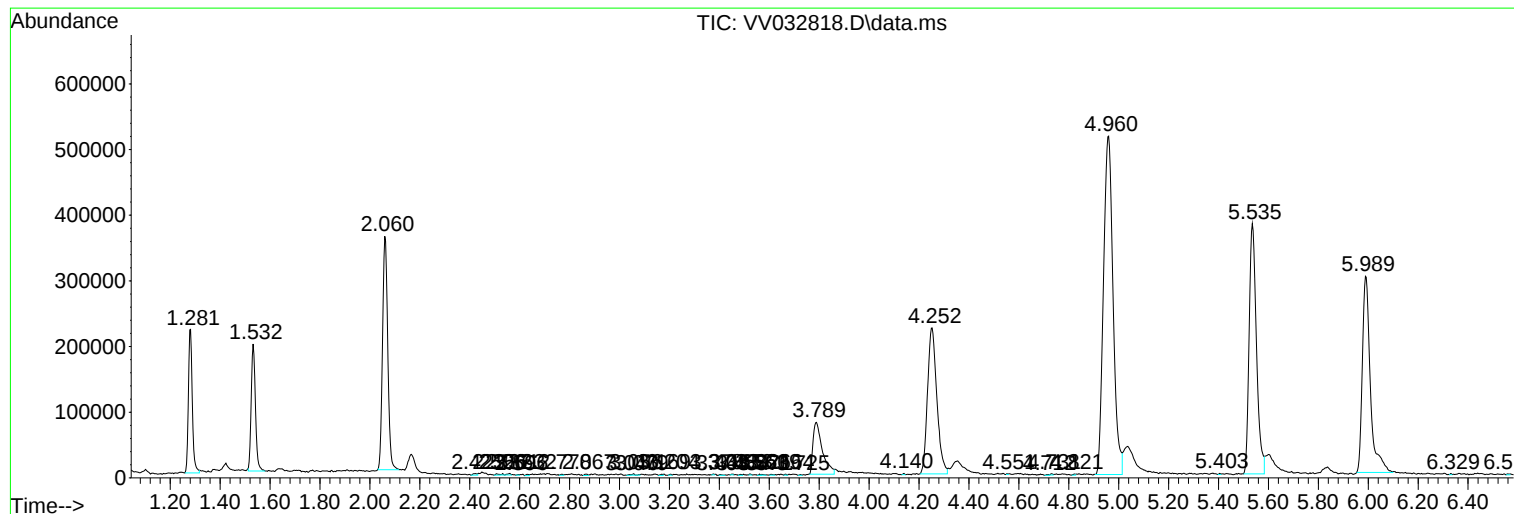

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
Data File : VV032818.D
Acq On : 01 Nov 2023 10:32
Operator : SY/MD
Sample : VV1101WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK209

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
Data File : VV032818.D
Acq On : 01 Nov 2023 10:32
Operator : SY/MD
Sample : VV1101WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK209

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc