

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
 Data File : VV032819.D
 Acq On : 01 Nov 2023 10:55
 Operator : SY/MD
 Sample : 05132-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5Q9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032819.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rBV	210098	222853	17.02%	2.141%
2	1.532	147	153	166	rVB	181638	208767	15.95%	2.006%
3	2.060	309	317	334	rVB	338169	484880	37.04%	4.659%
4	2.426	429	431	434	rBV4	1474	1008	0.08%	0.010%
5	2.497	450	453	456	rBV3	1999	1513	0.12%	0.015%
6	2.622	490	492	498	rVB7	2100	1505	0.11%	0.014%
7	2.667	502	506	507	rBV4	1158	636	0.05%	0.006%
8	2.770	534	538	541	rBV5	1679	1341	0.10%	0.013%
9	2.831	554	557	559	rBV4	1276	899	0.07%	0.009%
10	2.864	565	567	568	rBV2	1409	587	0.04%	0.006%
11	2.960	593	597	599	rBV4	1457	948	0.07%	0.009%
12	3.098	638	640	643	rVB4	1331	561	0.04%	0.005%
13	3.143	650	654	657	rBV7	1905	1347	0.10%	0.013%
14	3.166	659	661	664	rBV3	1696	1108	0.08%	0.011%
15	3.230	679	681	684	rVB4	1494	657	0.05%	0.006%
16	3.249	685	687	690	rBV4	720	373	0.03%	0.004%
17	3.320	706	709	713	rBV6	1079	827	0.06%	0.008%
18	3.339	713	715	716	rBV2	973	473	0.04%	0.005%
19	3.381	724	728	730	rVV5	1161	662	0.05%	0.006%
20	3.436	740	745	747	rBV5	2162	2212	0.17%	0.021%
21	3.458	751	752	756	rVB4	1833	985	0.08%	0.009%
22	3.484	756	760	762	rBV5	1856	1511	0.12%	0.015%
23	3.513	767	769	770	rVV2	1315	397	0.03%	0.004%
24	3.548	778	780	783	rVB4	1530	609	0.05%	0.006%
25	3.564	783	785	787	rBV2	1108	695	0.05%	0.007%
26	3.577	787	789	792	rBV4	759	458	0.03%	0.004%
27	3.626	803	804	806	rBV2	1025	457	0.03%	0.004%
28	3.658	812	814	815	rBV2	1146	505	0.04%	0.005%
29	3.725	832	835	839	rBV6	1159	889	0.07%	0.009%
30	3.790	846	855	879	rBV2	71397	197505	15.09%	1.898%
31	4.188	977	979	982	rBV3	1698	795	0.06%	0.008%
32	4.253	982	999	1020	rBV	213848	571178	43.63%	5.488%
33	4.767	1158	1159	1164	rVB5	938	399	0.03%	0.004%
34	4.796	1164	1168	1170	rBV4	1200	886	0.07%	0.009%
35	4.957	1203	1218	1235	rBV2	497817	1309129	100.00%	12.578%
36	5.420	1360	1362	1367	rVB5	1899	1214	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
 Data File : VV032819.D
 Acq On : 01 Nov 2023 10:55
 Operator : SY/MD
 Sample : 05132-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5Q9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	5.535	1387	1398	1413	rBV	373738	761800	58.19%	7.319%
38	5.989	1528	1539	1568	rBV	285649	635540	48.55%	6.106%
39	6.600	1728	1729	1731	rBV2	733	372	0.03%	0.004%
40	6.844	1802	1805	1807	rVB4	2028	961	0.07%	0.009%
41	6.863	1807	1811	1812	rBV4	1602	1122	0.09%	0.011%
42	6.915	1817	1827	1855	rVV	137660	288101	22.01%	2.768%
43	7.246	1919	1930	1961	rBV	588377	1111674	84.92%	10.681%
44	7.555	2017	2026	2050	rBV	104106	202981	15.51%	1.950%
45	7.783	2095	2097	2101	rVB4	2038	1203	0.09%	0.012%
46	7.873	2116	2125	2126	rBV8	3453	4304	0.33%	0.041%
47	8.027	2164	2173	2208	rBV	255350	547738	41.84%	5.263%
48	8.526	2325	2328	2333	rBV6	2579	2608	0.20%	0.025%
49	8.786	2398	2409	2434	rBV	646170	1099204	83.96%	10.561%
50	9.365	2587	2589	2593	rVB4	1346	666	0.05%	0.006%
51	9.593	2658	2660	2664	rBV4	1841	1208	0.09%	0.012%
52	9.725	2699	2701	2703	rBV3	905	442	0.03%	0.004%
53	9.751	2708	2709	2712	rBV3	958	440	0.03%	0.004%
54	9.786	2717	2720	2721	rBV3	1100	612	0.05%	0.006%
55	9.940	2766	2768	2770	rBV3	1101	501	0.04%	0.005%
56	9.995	2780	2785	2790	rBV8	2514	2995	0.23%	0.029%
57	10.156	2822	2835	2849	rBV	424437	679120	51.88%	6.525%
58	10.387	2904	2907	2908	rBV3	1185	725	0.06%	0.007%
59	10.432	2917	2921	2923	rBV4	1209	848	0.06%	0.008%
60	10.471	2929	2933	2936	rBV5	2516	1907	0.15%	0.018%
61	10.516	2946	2947	2949	rBV2	836	386	0.03%	0.004%
62	10.555	2957	2959	2960	rBV	1573	522	0.04%	0.005%
63	10.619	2977	2979	2982	rBV3	1163	840	0.06%	0.008%
64	10.924	3073	3074	3076	rBV2	1624	560	0.04%	0.005%
65	11.188	3145	3156	3175	rBV	618872	967321	73.89%	9.294%
66	11.423	3227	3229	3232	rBV4	2113	1610	0.12%	0.015%
67	11.458	3238	3240	3242	rBV3	1269	575	0.04%	0.006%
68	11.561	3261	3272	3295	rBV	651279	1032178	78.84%	9.917%
69	11.735	3325	3326	3330	rBV4	980	749	0.06%	0.007%
70	11.911	3379	3381	3387	rVB7	2793	1856	0.14%	0.018%
71	11.992	3405	3406	3408	rBV	968	396	0.03%	0.004%
72	12.005	3408	3410	3411	rBV3	1622	497	0.04%	0.005%
73	12.252	3483	3487	3488	rBV4	1872	1193	0.09%	0.011%
74	12.291	3497	3499	3500	rBV2	3905	1810	0.14%	0.017%
75	12.407	3531	3535	3538	rBV5	1880	1425	0.11%	0.014%
76	12.760	3643	3645	3646	rBV2	1198	659	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
 Data File : VV032819.D
 Acq On : 01 Nov 2023 10:55
 Operator : SY/MD
 Sample : 05132-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5Q9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.783	3650	3652	3654	rBV3	1199	573	0.04%	0.006%
78	12.815	3661	3662	3667	rVB5	1685	1345	0.10%	0.013%
79	12.850	3667	3673	3676	rBV7	1822	1849	0.14%	0.018%
80	12.895	3684	3687	3692	rVB6	1536	1444	0.11%	0.014%
81	12.924	3692	3696	3700	rBV6	1336	1092	0.08%	0.010%
82	12.979	3711	3713	3714	rBV2	1389	501	0.04%	0.005%
83	13.124	3755	3758	3762	rVB5	2467	1578	0.12%	0.015%
84	13.146	3762	3765	3766	rBV3	1893	847	0.06%	0.008%
85	13.297	3810	3812	3814	rBV3	1491	806	0.06%	0.008%
86	13.345	3822	3827	3828	rBV4	1560	1335	0.10%	0.013%
87	13.384	3837	3839	3841	rBV3	948	370	0.03%	0.004%
88	13.410	3845	3847	3852	rBV5	2760	2245	0.17%	0.022%
89	13.722	3942	3944	3946	rBV3	1212	696	0.05%	0.007%
90	13.783	3960	3963	3965	rBV4	1240	670	0.05%	0.006%
91	13.860	3985	3987	3989	rBV3	1622	882	0.07%	0.008%
92	14.008	4031	4033	4035	rVB3	1789	645	0.05%	0.006%
93	14.030	4035	4040	4043	rBV7	2318	1860	0.14%	0.018%
94	14.062	4047	4050	4051	rBV3	1341	848	0.06%	0.008%
95	14.114	4065	4066	4069	rBV3	1149	659	0.05%	0.006%
96	14.194	4087	4091	4096	rBV8	2622	3080	0.24%	0.030%
97	14.313	4125	4128	4129	rBV3	1620	1002	0.08%	0.010%
98	14.606	4217	4219	4221	rBV2	2464	1357	0.10%	0.013%
99	15.098	4370	4372	4375	rBV4	1474	998	0.08%	0.010%
100	15.384	4459	4461	4465	rBV5	2035	1128	0.09%	0.011%




Sum of corrected areas: 10408228

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
Data File : VV032819.D
Acq On : 01 Nov 2023 10:55
Operator : SY/MD
Sample : 05132-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5Q9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

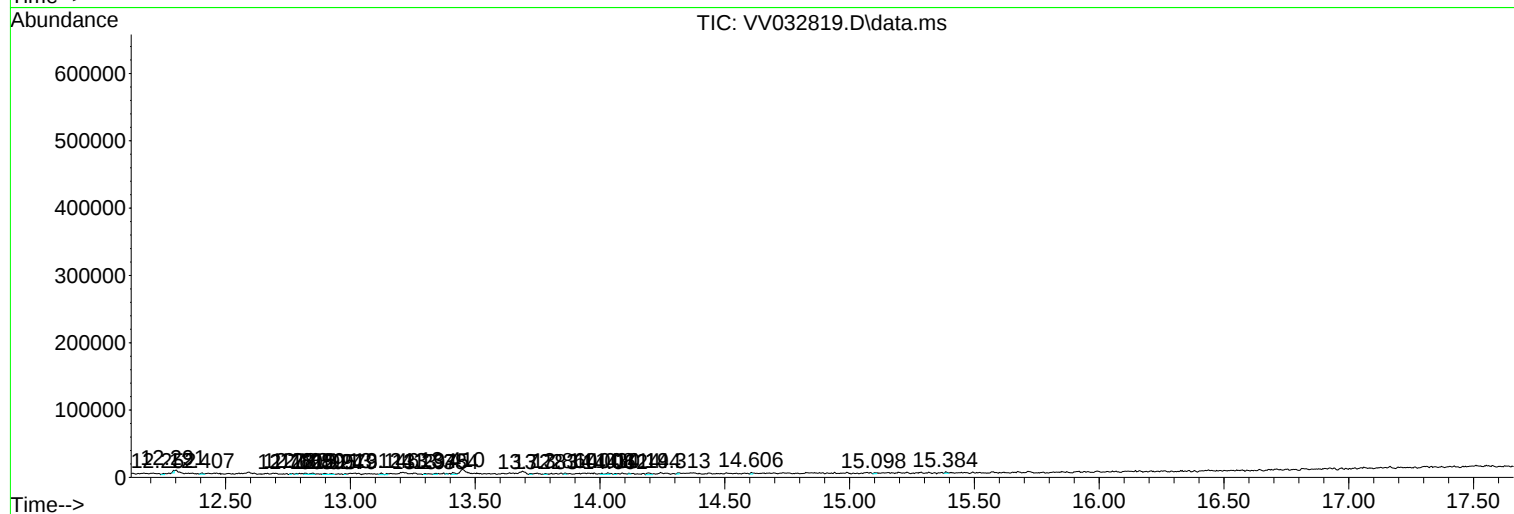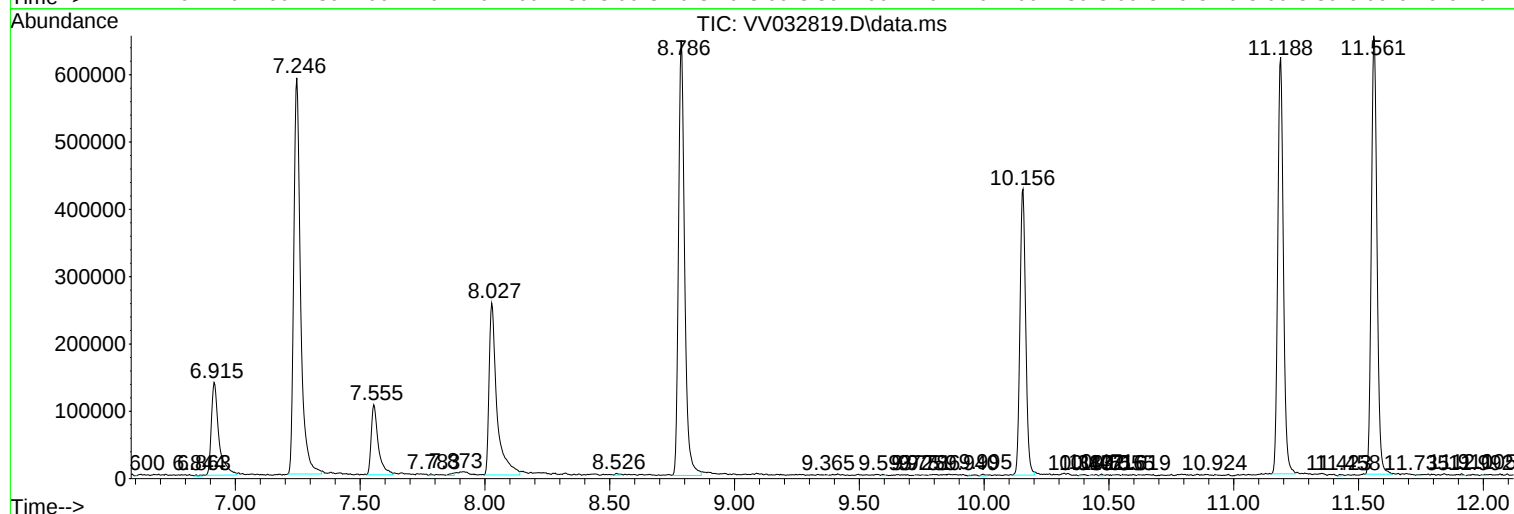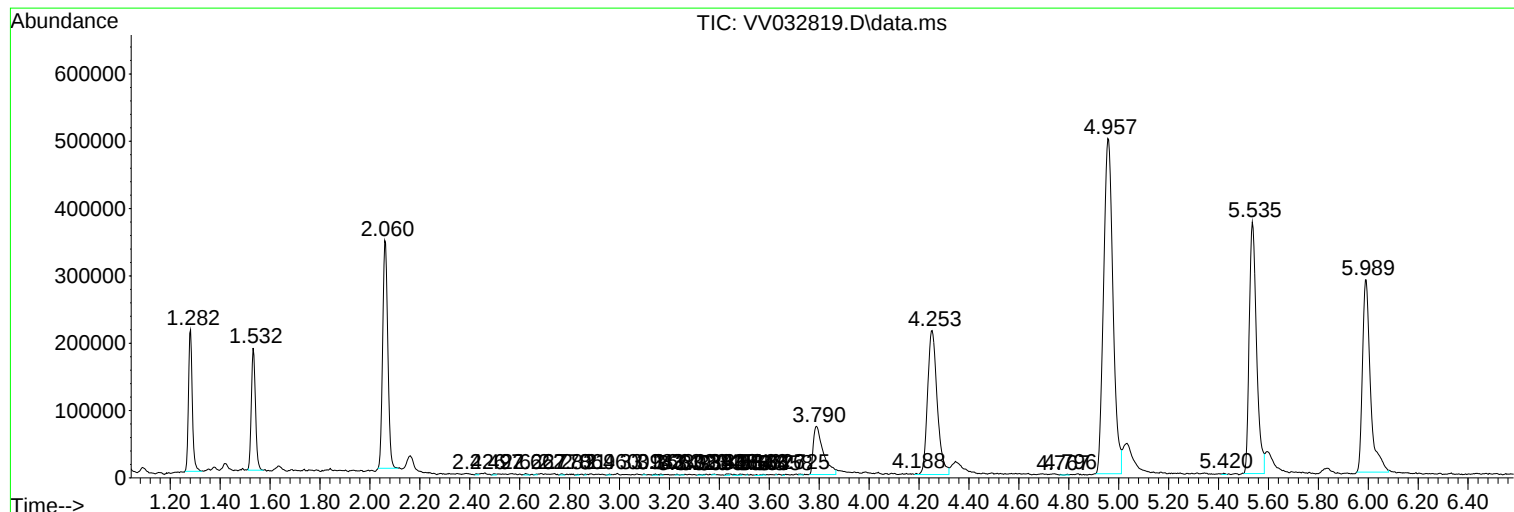

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
Data File : VV032819.D
Acq On : 01 Nov 2023 10:55
Operator : SY/MD
Sample : 05132-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5Q9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
Data File : VV032819.D
Acq On : 01 Nov 2023 10:55
Operator : SY/MD
Sample : 05132-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5Q9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------