


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110123\
Data File : VV032816.D
Acq On : 01 Nov 2023 08:54
Operator : SY/MD
Sample : BFB226
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB226

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Title : VOC Analysis
Last Update : Thu Nov 02 01:08:52 2023

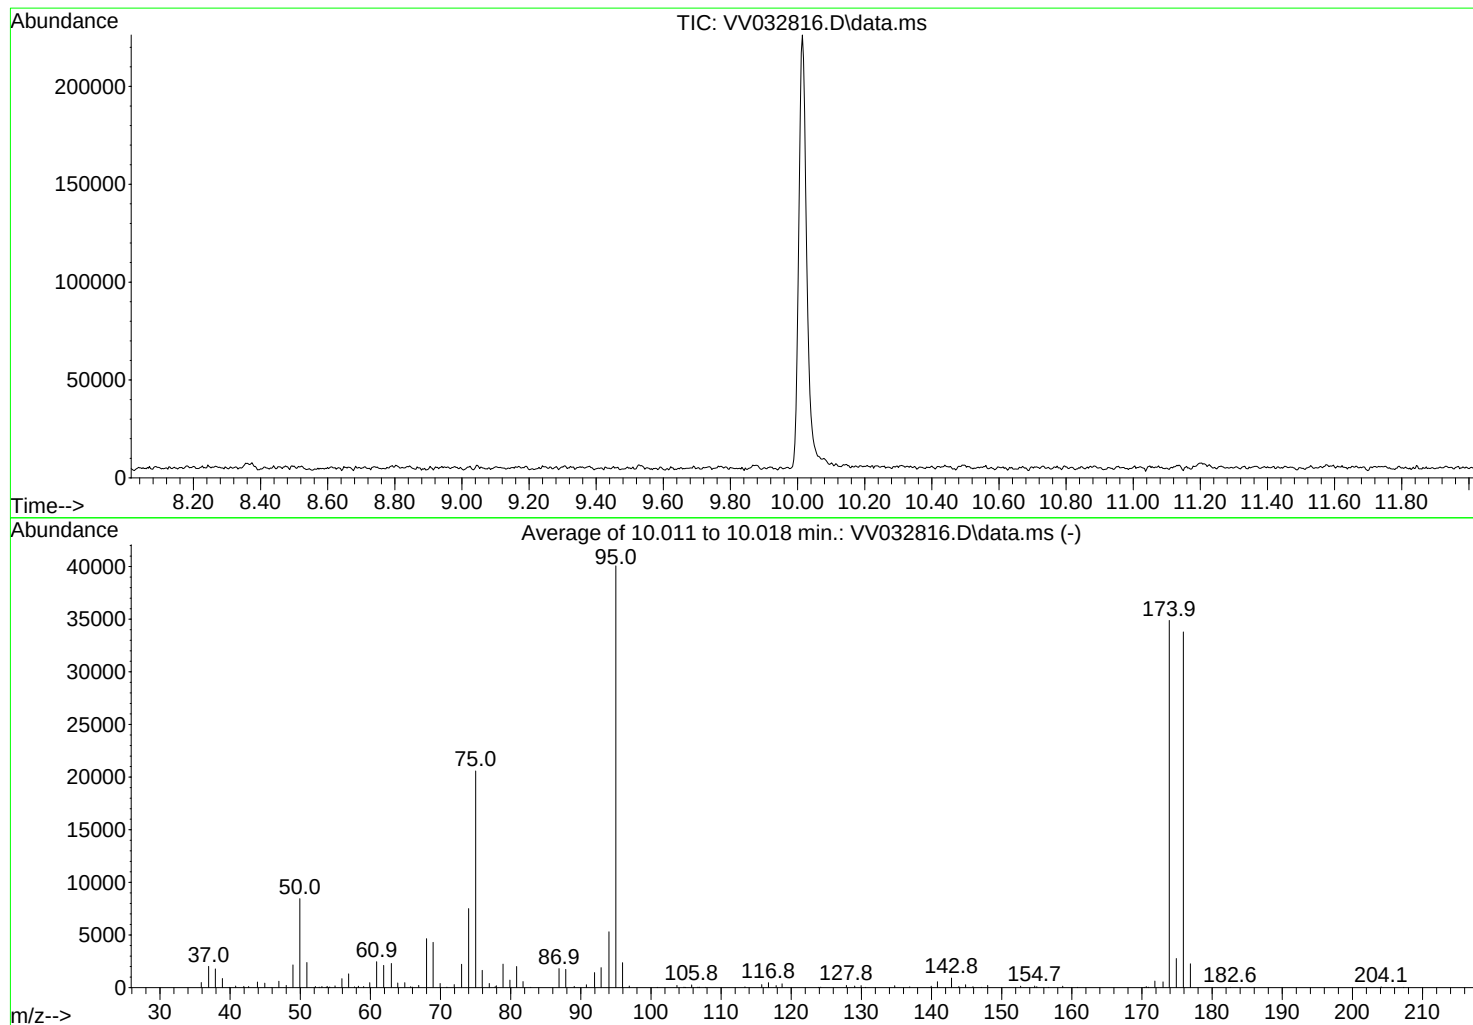

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	8446	PASS
75	95	30	80	51.4	20579	PASS
95	95	100	100	100.0	40069	PASS
96	95	5	9	5.9	2371	PASS
173	174	0.00	2	1.6	547	PASS
174	95	50	120	87.0	34880	PASS
175	174	5	9	7.9	2772	PASS
176	174	95	105	96.9	33787	PASS
177	176	5	10	6.7	2259	PASS

m/z	Abundance
35.30	163.0
36.20	197.0
37.10	125.0
37.90	162.0
39.00	211.0
39.90	343.0
41.40	159.0
42.10	112.0
42.90	130.0
43.90	352.0
44.60	168.0
45.20	107.0
46.00	143.0
46.60	113.0
47.90	143.0
48.70	140.0
49.80	100.0
50.80	115.0
51.70	102.0
52.10	100.0
53.40	172.0
55.20	137.0
60.00	108.0
61.80	159.0
64.80	112.0
67.50	107.0
71.10	121.0
76.10	106.0
82.80	113.0
96.00	120.0
101.40	125.0
109.70	110.0
148.40	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
35.90	531.0
37.00	2291.0
37.90	2028.0
38.90	1035.0
39.90	384.0
40.80	151.0
41.90	211.0
42.60	150.0
44.00	980.0
44.90	389.0
45.80	171.0
46.90	637.0
48.10	357.0
49.00	2146.0
50.00	8480.0
51.00	2645.0
51.80	152.0
52.20	207.0
53.10	180.0
53.70	120.0
54.20	184.0
55.00	167.0
56.00	978.0
56.90	1253.0
58.20	155.0
59.90	607.0
60.90	2437.0
62.00	2294.0
63.00	2342.0
63.90	519.0
64.90	520.0
65.70	121.0
66.90	232.0
68.00	4630.0
69.00	4321.0
70.00	452.0
72.00	303.0
73.00	2070.0
74.00	7685.0
75.00	20552.0
75.90	1641.0
76.90	353.0
77.80	279.0
78.90	2239.0
79.90	668.0
80.90	1888.0
81.80	618.0
82.90	128.0
86.90	1811.0
87.90	1702.0
89.00	117.0
90.80	237.0
92.00	1437.0
92.90	2001.0
94.00	5386.0
95.00	39632.0
96.00	2742.0
96.90	145.0
100.90	106.0
103.70	202.0
104.70	123.0
105.80	255.0
107.80	105.0
115.80	387.0
116.80	448.0
117.80	208.0
118.70	414.0
123.90	105.0
127.80	237.0
129.00	143.0
130.00	224.0
130.60	108.0
134.80	173.0
140.00	127.0
140.80	590.0
142.90	898.0
143.90	106.0
144.80	249.0
147.10	108.0
148.00	201.0
152.70	154.0
154.70	171.0
158.70	101.0
170.60	184.0
171.80	584.0
173.00	834.0
173.90	33968.0
174.90	2795.0
175.90	32504.0
176.90	2168.0
182.60	104.0
204.10	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
35.90	484.0
36.90	2226.0
37.90	2043.0
38.90	1117.0
40.00	377.0
40.80	160.0
41.90	269.0
42.70	158.0
44.00	901.0
44.90	443.0
45.80	153.0
46.90	617.0
48.10	379.0
49.00	2288.0
50.00	8910.0
51.00	2598.0
52.20	223.0
53.10	163.0
53.90	162.0
54.90	162.0
56.00	885.0
56.90	1349.0
57.80	120.0
58.30	150.0
59.10	120.0
59.90	600.0
60.90	2568.0
61.90	2317.0
63.00	2367.0
63.90	461.0
65.00	608.0
65.80	140.0
66.90	222.0
68.00	4838.0
69.00	4430.0
70.00	391.0
71.20	145.0
71.90	290.0
73.00	2290.0
74.00	7850.0
75.00	21184.0
76.00	1737.0
76.90	383.0
78.00	283.0
78.90	2333.0
79.90	749.0
80.80	2093.0
81.80	578.0
82.90	144.0
86.90	1826.0
87.90	1810.0
89.10	130.0
90.80	274.0
92.00	1482.0
92.90	1966.0
94.00	5399.0
95.00	41352.0
95.90	2488.0
96.90	146.0
103.70	231.0
105.80	275.0
106.70	126.0
113.40	111.0
115.80	276.0
116.70	496.0
117.90	201.0
118.70	383.0
127.80	215.0
129.10	168.0
129.90	190.0
134.70	170.0
136.90	100.0
140.00	143.0
140.80	612.0
142.90	954.0
143.90	114.0
144.90	280.0
146.00	120.0
148.00	213.0
152.70	160.0
154.70	171.0
155.00	153.0
158.70	151.0
170.60	145.0
171.80	635.0
173.00	806.0
173.90	35952.0
174.90	2846.0
175.90	35064.0
176.90	2357.0
204.10	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
35.90	456.0
36.90	1910.0
38.00	1773.0
38.90	1077.0
40.00	353.0
40.80	154.0
41.90	220.0
42.90	172.0
43.90	777.0
45.00	464.0
45.80	160.0
47.00	582.0
47.90	347.0
48.90	2060.0
50.00	8249.0
51.00	2275.0
52.20	202.0
52.70	154.0
53.80	208.0
54.90	173.0
55.90	698.0
56.90	1336.0
57.70	126.0
58.40	128.0
59.00	181.0
59.90	524.0
60.90	2391.0
61.90	2188.0
63.00	2157.0
63.90	363.0
65.00	626.0
66.00	132.0
66.90	173.0
68.00	4503.0
68.90	4160.0
69.90	367.0
70.90	136.0
71.90	276.0
73.00	2315.0
74.00	7009.0
75.00	20000.0
75.90	1864.0
77.00	448.0
77.90	276.0
78.90	2120.0
79.90	736.0
80.80	2051.0
81.70	525.0
83.00	141.0
86.90	1775.0
87.80	1672.0
89.10	135.0
90.80	295.0
91.90	1387.0
92.90	1753.0
94.00	5109.0
95.00	39224.0
95.90	2243.0
96.90	157.0
103.70	219.0
104.90	107.0
105.80	270.0
106.90	137.0
113.40	116.0
115.80	207.0
116.70	472.0
117.90	199.0
118.70	287.0
124.20	130.0
127.90	195.0
129.10	145.0
129.90	164.0
134.70	207.0
136.90	149.0
139.80	123.0
140.90	486.0
142.80	885.0
143.90	112.0
144.80	313.0
145.80	145.0
148.00	211.0
152.70	122.0
154.70	116.0
155.00	110.0
156.70	104.0
158.70	156.0
160.80	106.0
170.30	111.0
170.90	131.0
171.90	657.0
173.90	34720.0
174.90	2676.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

175.90	33792.0
176.90	2251.0
207.30	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226