

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110220\
 Data File : VV019198.D
 Acq On : 02 Nov 2020 11:30
 Operator : SY/MD
 Sample : VV1102MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK69

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	90	rVB	116096	119154	13.45%	1.709%
2	1.579	145	152	165	rVB	101738	111334	12.56%	1.597%
3	2.122	311	321	344	rBV	200725	299378	33.78%	4.294%
4	2.364	393	396	398	rBV	253	175	0.02%	0.003%
5	2.418	408	413	415	rBV2	217	217	0.02%	0.003%
6	2.447	420	422	425	rVV2	243	149	0.02%	0.002%
7	2.473	428	430	433	rVB	260	119	0.01%	0.002%
8	2.634	478	480	481	rBV	249	117	0.01%	0.002%
9	2.843	543	545	548	rBV	202	158	0.02%	0.002%
10	2.881	554	557	560	rVB	248	195	0.02%	0.003%
11	2.913	563	567	569	rBV	265	158	0.02%	0.002%
12	2.952	577	579	582	rBV	207	132	0.01%	0.002%
13	3.142	636	638	641	rBV2	199	129	0.01%	0.002%
14	3.277	676	680	681	rBV2	212	148	0.02%	0.002%
15	3.376	706	711	714	rBV2	234	228	0.03%	0.003%
16	3.402	717	719	722	rVB	211	103	0.01%	0.001%
17	3.576	771	773	778	rVB2	196	173	0.02%	0.002%
18	3.679	803	805	807	rVV	299	129	0.01%	0.002%
19	3.720	807	818	826	rVB2	326	692	0.08%	0.010%
20	3.904	866	875	910	rBV	54635	148085	16.71%	2.124%
21	4.376	1006	1022	1053	rBV2	146395	357819	40.38%	5.132%
22	4.605	1091	1093	1095	rBV2	230	125	0.01%	0.002%
23	4.621	1095	1098	1099	rBV	333	161	0.02%	0.002%
24	4.727	1129	1131	1133	rBV	194	106	0.01%	0.002%
25	4.765	1139	1143	1146	rBV2	269	215	0.02%	0.003%
26	4.804	1151	1155	1157	rBV2	261	224	0.03%	0.003%
27	4.846	1164	1168	1170	rBV2	272	236	0.03%	0.003%
28	4.907	1183	1187	1190	rBV2	212	228	0.03%	0.003%
29	4.987	1209	1212	1216	rVB2	390	256	0.03%	0.004%
30	5.006	1216	1218	1220	rBV	167	119	0.01%	0.002%
31	5.071	1221	1238	1272	rBV2	341848	886203	100.00%	12.710%
32	5.408	1340	1343	1345	rBV	317	167	0.02%	0.002%
33	5.640	1400	1415	1442	rBV	307510	604198	68.18%	8.665%
34	5.932	1496	1506	1524	rVB3	6979	14153	1.60%	0.203%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110220\
 Data File : VV019198.D
 Acq On : 02 Nov 2020 11:30
 Operator : SY/MD
 Sample : VV1102MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK69

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	6.006	1524	1529	1533	rBV2	211	293	0.03%	0.004%
36	6.093	1542	1556	1579	rBV	198254	399590	45.09%	5.731%
37	6.270	1609	1611	1613	rVB	378	131	0.01%	0.002%
38	6.437	1659	1663	1667	rBV	284	238	0.03%	0.003%
39	6.534	1690	1693	1696	rVB	228	130	0.01%	0.002%
40	6.556	1697	1700	1701	rBV	215	119	0.01%	0.002%
41	6.601	1711	1714	1716	rBV	358	185	0.02%	0.003%
42	6.617	1716	1719	1722	rVV	182	147	0.02%	0.002%
43	6.678	1733	1738	1740	rBV2	315	285	0.03%	0.004%
44	6.704	1744	1746	1749	rBV2	170	126	0.01%	0.002%
45	6.842	1785	1789	1791	rBV2	283	175	0.02%	0.003%
46	7.006	1829	1840	1870	rBV	116397	213858	24.13%	3.067%
47	7.338	1931	1943	1961	rBV	419210	717067	80.91%	10.284%
48	7.579	2015	2018	2022	rVB3	308	210	0.02%	0.003%
49	7.604	2022	2026	2028	rBV	317	243	0.03%	0.003%
50	7.643	2028	2038	2062	rBV	82466	146332	16.51%	2.099%
51	7.891	2109	2115	2119	rBV2	380	413	0.05%	0.006%
52	7.910	2119	2121	2124	rVV	211	144	0.02%	0.002%
53	8.058	2164	2167	2170	rBV2	214	149	0.02%	0.002%
54	8.106	2171	2182	2213	rBV	197349	352473	39.77%	5.055%
55	8.424	2277	2281	2283	rBV2	420	340	0.04%	0.005%
56	8.469	2292	2295	2297	rBV2	257	202	0.02%	0.003%
57	8.543	2315	2318	2319	rBV	252	136	0.02%	0.002%
58	8.627	2340	2344	2346	rBV	288	222	0.03%	0.003%
59	8.765	2384	2387	2391	rBV2	239	241	0.03%	0.003%
60	8.791	2391	2395	2397	rVV	178	132	0.01%	0.002%
61	8.871	2408	2420	2444	rBV	466672	748037	84.41%	10.728%
62	9.035	2468	2471	2476	rBV2	522	582	0.07%	0.008%
63	9.116	2494	2496	2502	rBV2	306	310	0.03%	0.004%
64	9.305	2549	2555	2556	rBV2	240	191	0.02%	0.003%
65	9.344	2564	2567	2570	rBV	208	133	0.02%	0.002%
66	9.360	2570	2572	2578	rVB2	356	283	0.03%	0.004%
67	9.389	2578	2581	2585	rBV	255	180	0.02%	0.003%
68	9.418	2585	2590	2593	rBV	316	299	0.03%	0.004%
69	9.563	2632	2635	2637	rBV	329	230	0.03%	0.003%
70	9.669	2664	2668	2671	rBV2	280	264	0.03%	0.004%
71	9.733	2685	2688	2693	rVB2	197	149	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110220\
 Data File : VV019198.D
 Acq On : 02 Nov 2020 11:30
 Operator : SY/MD
 Sample : VV1102MBL01
 Misc : 5.0µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK69

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	9.759	2693	2696	2699	rBV	283	240	0.03%	0.003%
73	9.862	2724	2728	2733	rVB	379	389	0.04%	0.006%
74	9.945	2751	2754	2756	rBV	196	143	0.02%	0.002%
75	10.000	2767	2771	2773	rBV2	333	296	0.03%	0.004%
76	10.145	2808	2816	2823	rBV4	1416	2357	0.27%	0.034%
77	10.235	2833	2844	2860	rBV	245946	384368	43.37%	5.512%
78	10.476	2913	2919	2922	rBV	339	361	0.04%	0.005%
79	10.511	2926	2930	2933	rBV	336	337	0.04%	0.005%
80	10.566	2943	2947	2953	rBV3	462	610	0.07%	0.009%
81	10.591	2953	2955	2961	rVV2	377	384	0.04%	0.006%
82	10.662	2974	2977	2979	rBV	179	107	0.01%	0.002%
83	10.804	3018	3021	3026	rBV2	276	293	0.03%	0.004%
84	10.903	3045	3052	3055	rBV2	278	301	0.03%	0.004%
85	10.923	3055	3058	3059	rVV2	374	199	0.02%	0.003%
86	10.935	3059	3062	3070	rVB5	1243	1613	0.18%	0.023%
87	11.135	3120	3124	3125	rBV2	223	136	0.02%	0.002%
88	11.270	3155	3166	3193	rBV	492819	750592	84.70%	10.765%
89	11.646	3271	3283	3304	rBV	449987	697225	78.68%	9.999%
90	12.051	3406	3409	3410	rBV	187	111	0.01%	0.002%
91	12.328	3492	3495	3497	rBV2	268	194	0.02%	0.003%
92	12.582	3568	3574	3575	rBV2	271	279	0.03%	0.004%
93	12.678	3599	3604	3612	rBV3	568	761	0.09%	0.011%
94	12.784	3635	3637	3643	rVB2	273	251	0.03%	0.004%
95	13.009	3704	3707	3711	rVB	260	219	0.02%	0.003%
96	13.151	3748	3751	3753	rBV2	281	224	0.03%	0.003%
97	13.225	3772	3774	3778	rBV	321	254	0.03%	0.004%
98	13.279	3788	3791	3792	rBV	238	113	0.01%	0.002%
99	13.546	3868	3874	3877	rBV4	396	587	0.07%	0.008%
100	14.141	4056	4059	4064	rBV	389	358	0.04%	0.005%


Sum of corrected areas: 6972724

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110220\
Data File : VV019198.D
Acq On : 02 Nov 2020 11:30
Operator : SY/MD
Sample : VV1102MBL01
Misc : 5.0µ/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK69

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

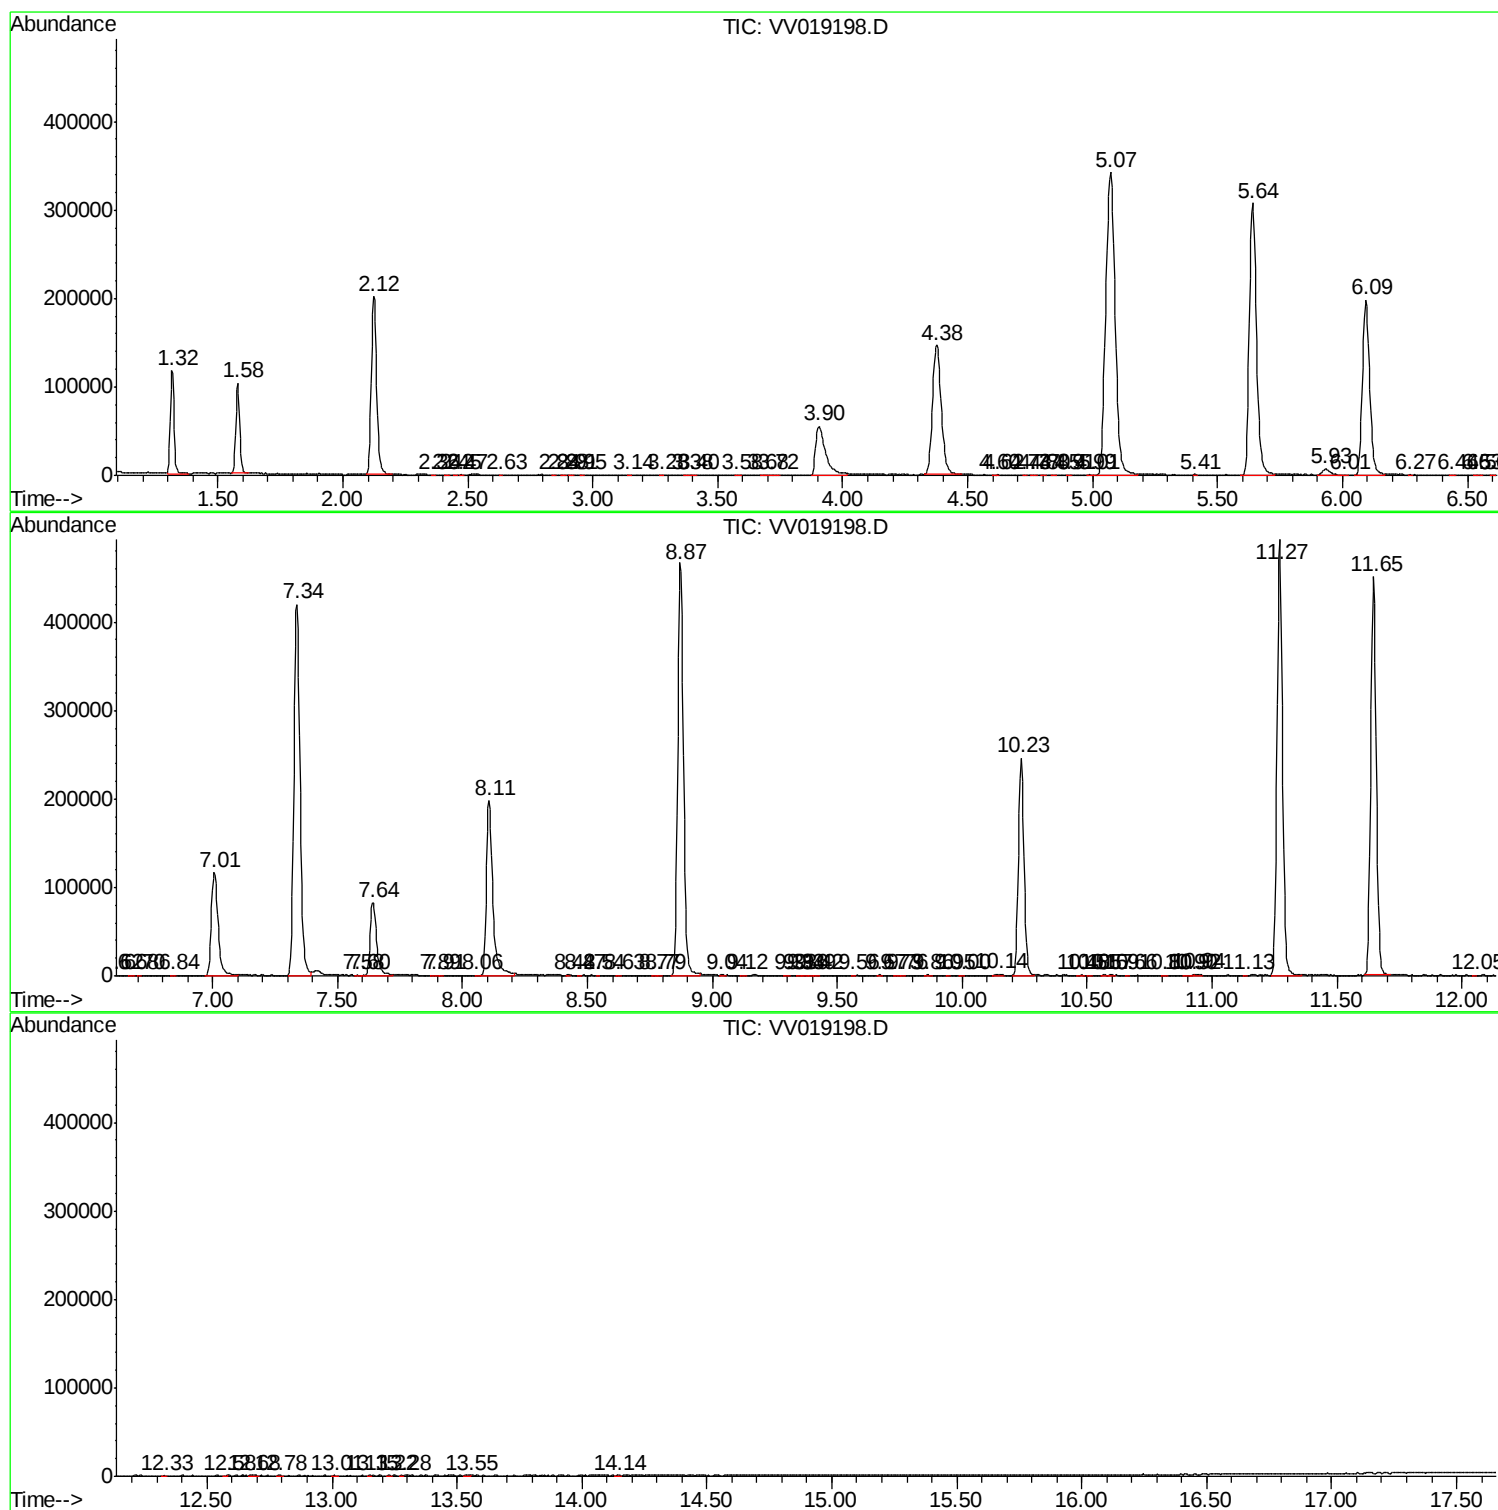

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV110220\
Data File : VV019198.D
Acq On : 02 Nov 2020 11:30
Operator : SY/MD
Sample : VV1102MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK69

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV110220\
Data File : VV019198.D
Acq On : 02 Nov 2020 11:30
Operator : SY/MD
Sample : VV1102MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK69

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc