

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110220\
 Data File : VV019200.D
 Acq On : 02 Nov 2020 13:26
 Operator : SY/MD
 Sample : L4502-22ME
 Misc : 5.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG445ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB	130437	155133	12.51%	1.653%
2	1.579	144	152	166	rBV	91541	152605	12.31%	1.626%
3	2.103	303	315	329	rBV	280239	412657	33.28%	4.396%
4	2.444	418	421	422	rBV	270	146	0.01%	0.002%
5	2.563	455	458	460	rVB	233	117	0.01%	0.001%
6	2.579	461	463	466	rVV2	195	123	0.01%	0.001%
7	2.637	470	481	489	rVB3	747	1554	0.13%	0.017%
8	2.736	510	512	517	rVB	236	115	0.01%	0.001%
9	2.839	539	544	546	rBV2	399	429	0.03%	0.005%
10	2.888	556	559	562	rBV	170	118	0.01%	0.001%
11	3.052	607	610	613	rVB2	387	273	0.02%	0.003%
12	3.074	613	617	623	rVB	291	256	0.02%	0.003%
13	3.103	623	626	628	rBV	268	163	0.01%	0.002%
14	3.171	645	647	649	rBV	219	136	0.01%	0.001%
15	3.232	662	666	671	rBV2	327	332	0.03%	0.004%
16	3.328	694	696	700	rBV	178	121	0.01%	0.001%
17	3.363	703	707	711	rVB	199	176	0.01%	0.002%
18	3.389	711	715	717	rBV2	178	152	0.01%	0.002%
19	3.463	735	738	741	rBV	288	167	0.01%	0.002%
20	3.524	753	757	762	rVB2	178	224	0.02%	0.002%
21	3.550	762	765	766	rBV	218	118	0.01%	0.001%
22	3.769	830	833	838	rBV2	228	243	0.02%	0.003%
23	3.839	847	855	859	rBV	468	506	0.04%	0.005%
24	3.920	868	880	905	rBV2	46164	162391	13.10%	1.730%
25	4.370	1005	1020	1044	rBV	191206	484248	39.06%	5.159%
26	4.614	1093	1096	1103	rVB2	390	414	0.03%	0.004%
27	4.662	1107	1111	1113	rBV2	380	334	0.03%	0.004%
28	4.714	1125	1127	1131	rVB2	295	188	0.02%	0.002%
29	4.740	1131	1135	1138	rBV2	255	256	0.02%	0.003%
30	4.810	1153	1157	1158	rBV	277	137	0.01%	0.001%
31	4.859	1168	1172	1175	rBV	175	144	0.01%	0.002%
32	4.968	1201	1206	1209	rBV	291	215	0.02%	0.002%
33	5.064	1219	1236	1264	rBV2	496052	1239900	100.00%	13.208%
34	5.309	1309	1312	1314	rBV2	262	139	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110220\
 Data File : VV019200.D
 Acq On : 02 Nov 2020 13:26
 Operator : SY/MD
 Sample : L4502-22ME
 Misc : 5.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG445ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	5.363	1321	1329	1337	rBV5	1571	3015	0.24%	0.032%
36	5.559	1387	1390	1394	rBV2	286	294	0.02%	0.003%
37	5.633	1401	1413	1445	rBV	291950	606712	48.93%	6.463%
38	5.881	1488	1490	1493	rBV2	240	180	0.01%	0.002%
39	5.923	1494	1503	1518	rVV6	10052	22594	1.82%	0.241%
40	6.090	1541	1555	1590	rBV	263111	553717	44.66%	5.899%
41	6.334	1626	1631	1634	rBV	222	190	0.02%	0.002%
42	6.350	1634	1636	1638	rVV	226	127	0.01%	0.001%
43	6.363	1638	1640	1646	rVB	293	229	0.02%	0.002%
44	6.486	1675	1678	1683	rBV2	187	136	0.01%	0.001%
45	6.569	1699	1704	1706	rBV2	228	157	0.01%	0.002%
46	6.653	1718	1730	1732	rBV3	505	835	0.07%	0.009%
47	6.836	1782	1787	1788	rBV2	242	180	0.01%	0.002%
48	6.884	1798	1802	1805	rBV2	201	186	0.02%	0.002%
49	7.006	1828	1840	1875	rBV	154217	306514	24.72%	3.265%
50	7.334	1929	1942	1961	rBV	579250	1033058	83.32%	11.005%
51	7.601	2022	2025	2027	rBV2	203	136	0.01%	0.001%
52	7.640	2027	2037	2070	rVV	104099	217745	17.56%	2.320%
53	7.813	2087	2091	2092	rBV2	374	235	0.02%	0.003%
54	7.871	2105	2109	2112	rBV2	227	195	0.02%	0.002%
55	7.993	2135	2147	2170	rBV	237456	397778	32.08%	4.237%
56	8.141	2175	2193	2217	rBV2	153509	507311	40.92%	5.404%
57	8.386	2266	2269	2273	rBV	453	379	0.03%	0.004%
58	8.408	2273	2276	2281	rVB3	427	357	0.03%	0.004%
59	8.460	2289	2292	2296	rBV3	509	442	0.04%	0.005%
60	8.556	2318	2322	2327	rBV2	298	285	0.02%	0.003%
61	8.707	2365	2369	2371	rBV	247	184	0.01%	0.002%
62	8.874	2409	2421	2455	rBV	405754	773340	62.37%	8.238%
63	9.045	2470	2474	2478	rBV2	478	447	0.04%	0.005%
64	9.167	2509	2512	2513	rBV	377	207	0.02%	0.002%
65	9.302	2551	2554	2557	rBV	345	270	0.02%	0.003%
66	9.357	2569	2571	2578	rVB2	178	152	0.01%	0.002%
67	9.389	2578	2581	2587	rVB2	280	230	0.02%	0.002%
68	9.428	2587	2593	2595	rBV2	248	260	0.02%	0.003%
69	9.530	2618	2625	2629	rBV2	339	403	0.03%	0.004%
70	9.572	2634	2638	2641	rBV	236	167	0.01%	0.002%
71	9.591	2642	2644	2646	rBV	242	115	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV110220\
 Data File : VV019200.D
 Acq On : 02 Nov 2020 13:26
 Operator : SY/MD
 Sample : L4502-22ME
 Misc : 5.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG445ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	9.681	2668	2672	2675	rBV2	357	368	0.03%	0.004%
73	9.984	2763	2766	2768	rBV	196	139	0.01%	0.001%
74	10.042	2780	2784	2787	rBV	369	324	0.03%	0.003%
75	10.109	2801	2805	2808	rBV2	220	164	0.01%	0.002%
76	10.148	2809	2817	2825	rVV4	2400	4020	0.32%	0.043%
77	10.247	2834	2848	2865	rBV	306968	534256	43.09%	5.691%
78	10.469	2910	2917	2918	rBV	427	425	0.03%	0.005%
79	10.501	2924	2927	2928	rBV	270	177	0.01%	0.002%
80	10.772	3005	3011	3015	rBV	293	398	0.03%	0.004%
81	10.794	3015	3018	3020	rBV	246	217	0.02%	0.002%
82	10.852	3031	3036	3038	rBV2	344	325	0.03%	0.003%
83	10.884	3043	3046	3049	rBV2	188	198	0.02%	0.002%
84	11.019	3085	3088	3094	rBV2	259	272	0.02%	0.003%
85	11.054	3094	3099	3106	rBV3	601	808	0.07%	0.009%
86	11.167	3129	3134	3140	rVB5	1462	1889	0.15%	0.020%
87	11.273	3155	3167	3186	rBV	500868	783700	63.21%	8.349%
88	11.534	3244	3248	3251	rBV	404	380	0.03%	0.004%
89	11.598	3266	3268	3269	rBV	274	135	0.01%	0.001%
90	11.649	3272	3284	3305	rVV	642532	1013524	81.74%	10.797%
91	11.868	3349	3352	3356	rBV	421	264	0.02%	0.003%
92	11.929	3367	3371	3374	rBV	288	235	0.02%	0.003%
93	12.016	3396	3398	3403	rBV2	223	193	0.02%	0.002%
94	12.087	3416	3420	3424	rBV2	301	317	0.03%	0.003%
95	12.215	3457	3460	3463	rVB	215	116	0.01%	0.001%
96	12.501	3545	3549	3550	rBV	200	143	0.01%	0.002%
97	12.852	3654	3658	3661	rBV	306	260	0.02%	0.003%
98	13.591	3884	3888	3892	rBV2	306	327	0.03%	0.003%
99	13.771	3942	3944	3947	rVB2	324	159	0.01%	0.002%
100	14.546	4179	4185	4186	rBV2	521	501	0.04%	0.005%


Sum of corrected areas: 9387226

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV110220\
Data File : VV019200.D
Acq On : 02 Nov 2020 13:26
Operator : SY/MD
Sample : L4502-22ME
Misc : 5.27g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG445ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

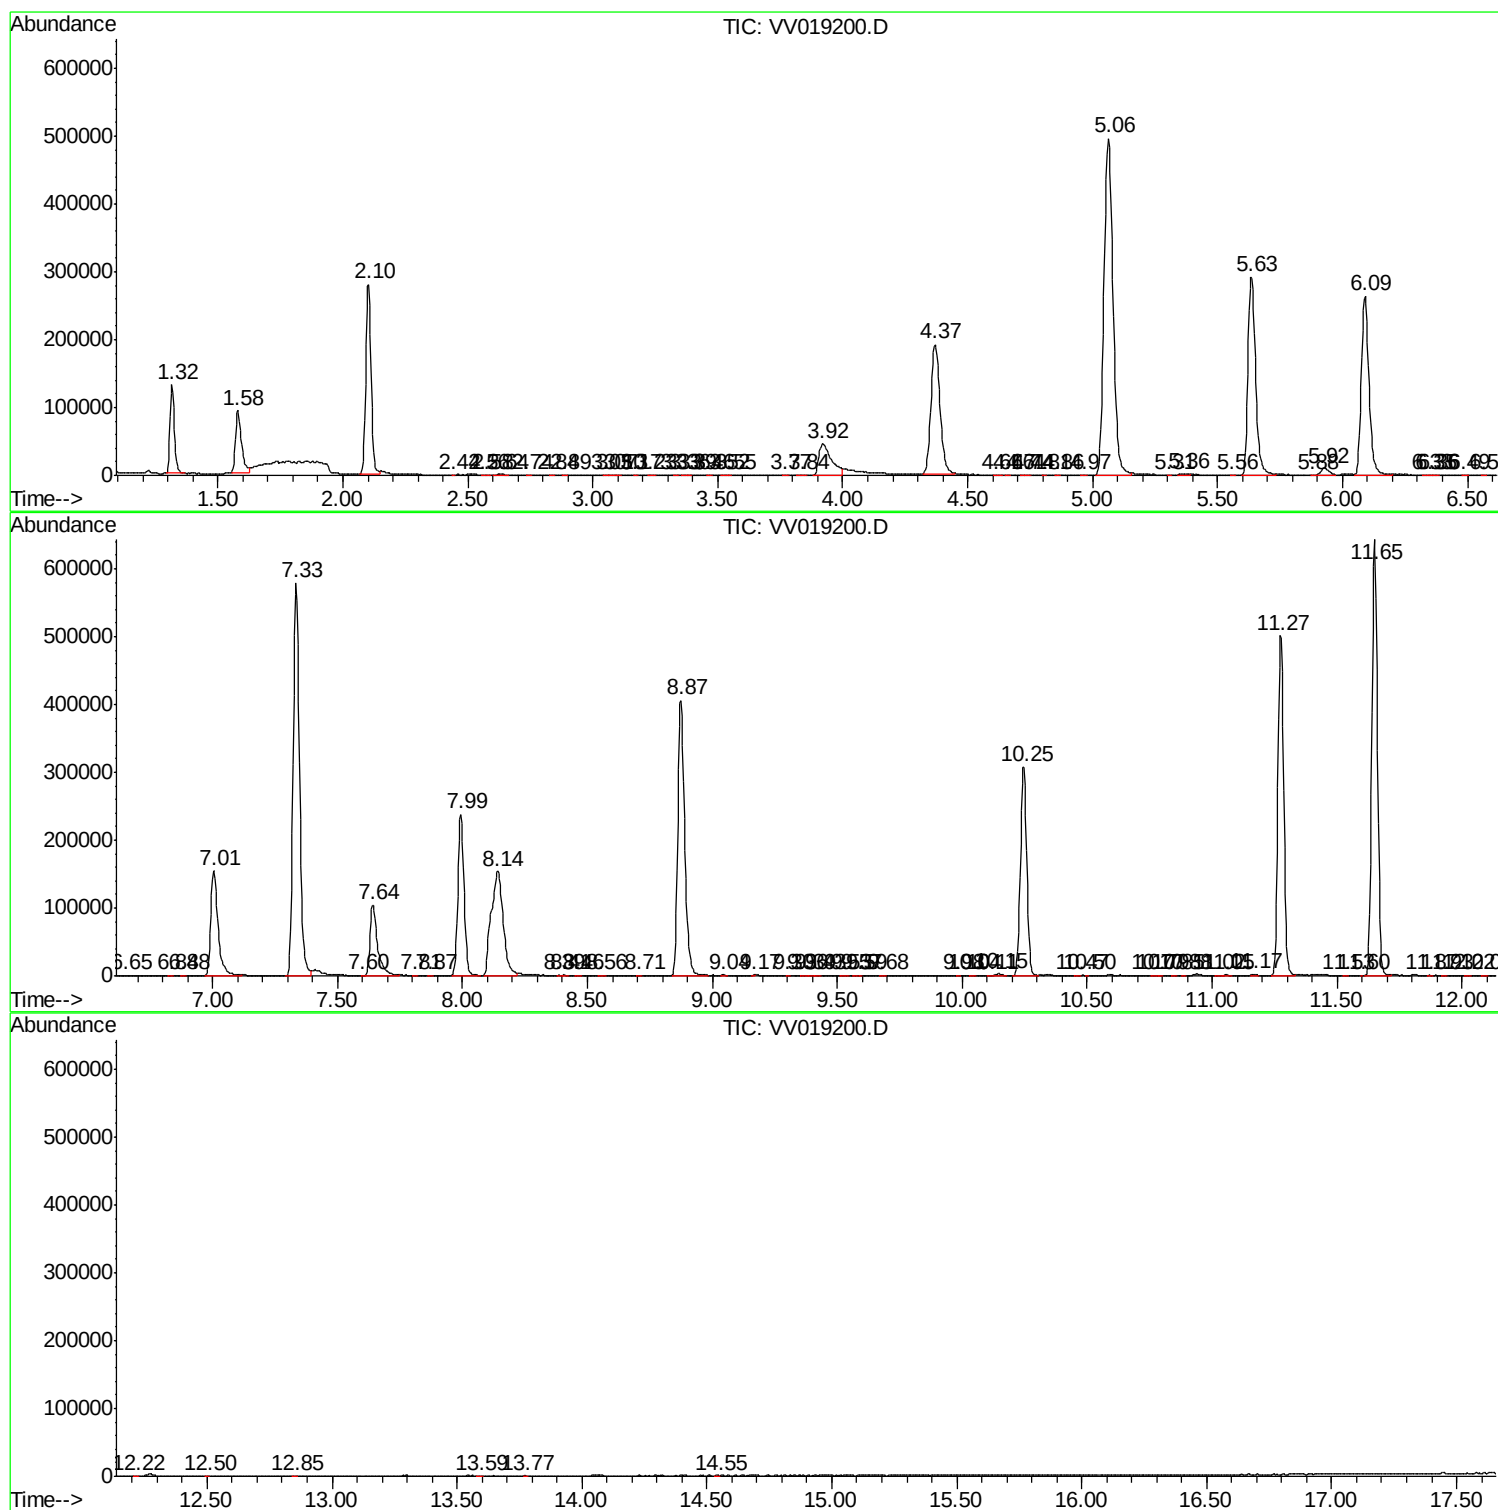

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV110220\
Data File : VV019200.D
Acq On : 02 Nov 2020 13:26
Operator : SY/MD
Sample : L4502-22ME
Misc : 5.27g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG445ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV110220\
Data File : VV019200.D
Acq On : 02 Nov 2020 13:26
Operator : SY/MD
Sample : L4502-22ME
Misc : 5.27g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG445ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc