


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV110220\
 Data File : VV019195.D
 Acq On : 02 Nov 2020 07:58
 Operator : SY/MD
 Sample : BFB87
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB87

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis
 Last Update : Tue Nov 03 03:19:34 2020

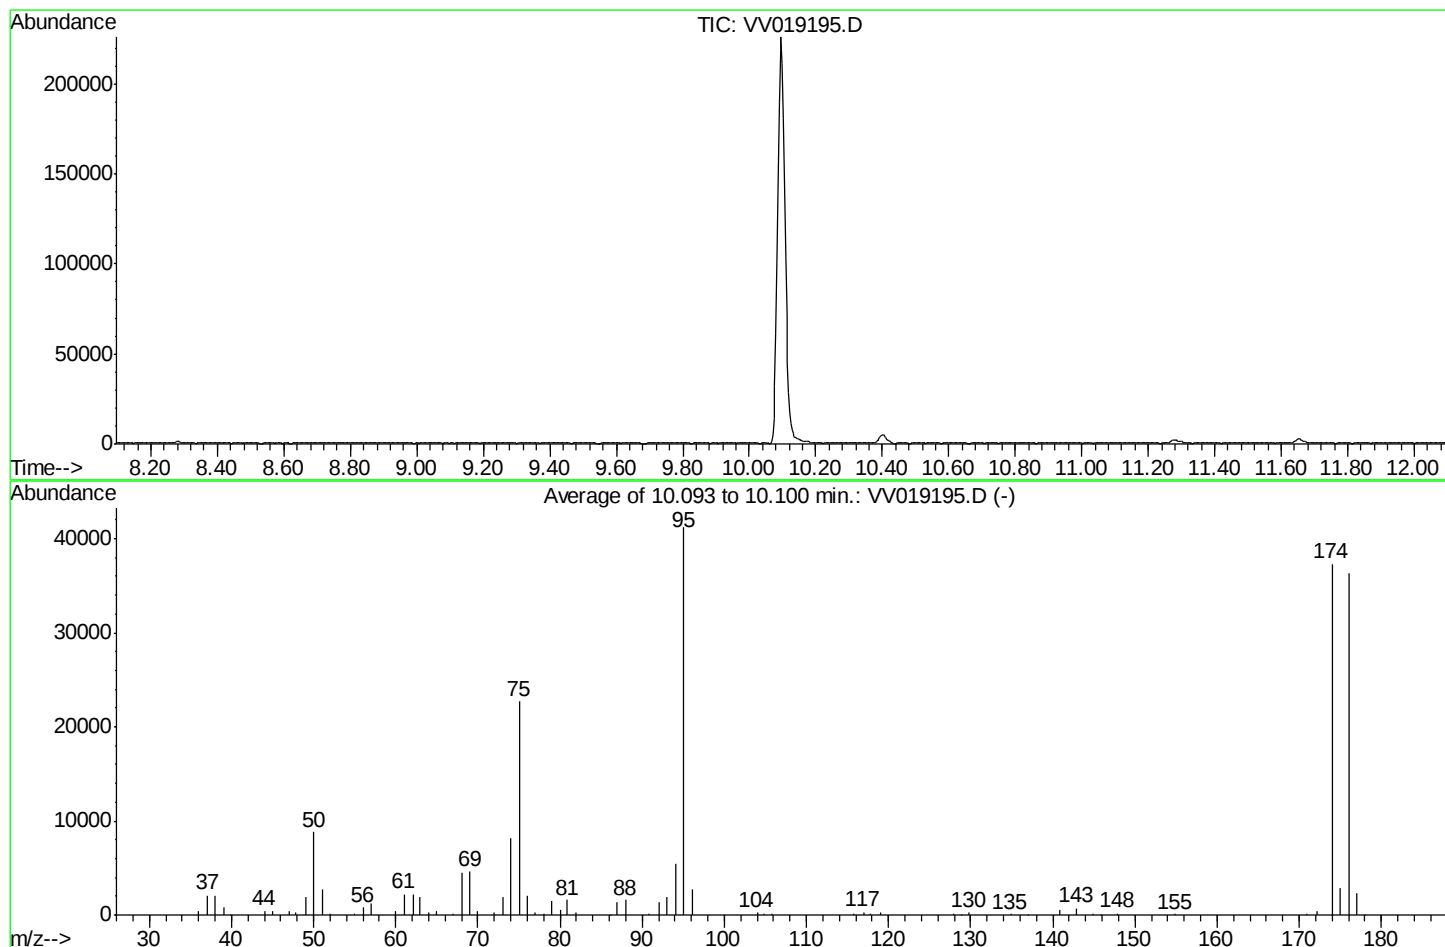

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	8812	PASS
75	95	30	80	55.0	22661	PASS
95	95	100	100	100.0	41202	PASS
96	95	5	9	6.6	2727	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.6	37330	PASS
175	174	5	9	7.8	2927	PASS
176	174	95	101	97.5	36384	PASS
177	176	5	9	6.5	2380	PASS

m/z	Abundance
36.00	461.0
37.10	2180.0
38.10	2154.0
39.10	781.0
44.00	810.0
45.00	344.0
47.00	445.0
47.90	286.0
49.10	1955.0
50.00	8911.0
51.10	2616.0
52.10	113.0
55.00	139.0
56.00	790.0
57.00	1309.0
60.00	473.0
61.00	2237.0
62.10	2126.0
63.00	1923.0
64.00	266.0
65.00	447.0
67.00	151.0
68.00	4461.0
69.00	4741.0
70.00	386.0
71.90	222.0
73.10	2059.0
74.00	8148.0
75.10	23144.0
76.00	2065.0
77.00	213.0
78.00	174.0
78.90	1526.0
80.00	480.0
80.90	1651.0
81.90	302.0
86.20	107.0
86.90	1425.0
88.00	1662.0
90.90	179.0
92.00	1311.0
93.00	1883.0
94.10	5630.0
95.10	40816.0
96.00	2782.0
104.00	184.0
104.90	139.0
105.80	221.0
115.70	205.0
116.90	313.0
117.80	167.0
118.90	320.0
127.90	160.0
128.80	107.0
129.80	166.0
136.90	105.0
140.90	491.0
142.90	749.0
144.90	218.0
145.90	105.0
147.90	142.0
154.90	115.0
170.90	129.0
172.20	417.0
174.00	36848.0
175.00	2957.0
176.00	36000.0
177.00	2449.0
177.90	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
36.00	423.0
37.10	2170.0
38.00	2077.0
39.00	837.0
44.00	831.0
45.00	373.0
47.10	472.0
47.80	299.0
49.00	1956.0
50.00	9181.0
51.10	2843.0
52.00	111.0
55.00	120.0
56.00	800.0
57.00	1266.0
60.00	461.0
61.00	2294.0
62.10	2183.0
63.00	1943.0
64.00	299.0
65.00	405.0
67.00	153.0
68.00	4562.0
69.00	4720.0
70.00	441.0
71.90	263.0
73.10	2033.0
74.00	8548.0
75.10	23344.0
76.00	2183.0
76.90	218.0
78.00	172.0
79.00	1645.0
80.00	520.0
80.90	1632.0
81.90	339.0
86.90	1472.0
88.00	1679.0
90.90	191.0
92.10	1442.0
93.00	1893.0
94.10	5556.0
95.10	42616.0
96.10	2828.0
104.00	234.0
104.90	111.0
105.80	193.0
115.80	203.0
116.90	339.0
117.80	155.0
119.00	318.0
127.90	188.0
128.80	110.0
129.80	234.0
134.90	140.0
140.90	520.0
142.90	777.0
144.90	205.0
147.90	154.0
154.90	118.0
171.00	106.0
172.10	455.0
174.00	38560.0
175.00	3033.0
176.00	37600.0
177.00	2475.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
36.00	383.0
37.10	1969.0
38.00	1778.0
39.00	854.0
39.90	101.0
44.00	757.0
45.00	362.0
47.10	427.0
47.90	271.0
49.00	1722.0
50.00	8345.0
51.10	2712.0
51.90	120.0
55.00	137.0
56.00	731.0
57.00	1083.0
60.00	415.0
61.00	2137.0
62.10	2084.0
63.00	1870.0
64.00	315.0
65.00	336.0
67.00	136.0
68.00	4275.0
69.10	4261.0
70.00	407.0
71.90	258.0
73.00	1818.0
74.00	7983.0
75.00	21496.0
76.00	2067.0
76.90	207.0
78.00	140.0
79.00	1509.0
80.00	499.0
80.90	1440.0
81.90	377.0
86.90	1399.0
88.00	1477.0
90.80	180.0
92.10	1396.0
93.00	1798.0
94.00	5147.0
95.10	40176.0
96.00	2571.0
104.00	282.0
105.90	164.0
115.80	181.0
117.00	329.0
117.90	145.0
118.90	279.0
127.90	194.0
129.80	248.0
134.90	131.0
140.90	482.0
142.90	725.0
144.90	155.0
147.90	163.0
172.10	430.0
174.00	36584.0
175.00	2791.0
176.00	35552.0
177.00	2216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
44.00	376.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87