

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
 Data File : VV023136.D
 Acq On : 02 Nov 2021 10:31
 Operator : SY/MD
 Sample : M4412-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG357

Quant Time: Nov 02 22:40:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 22:38:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	134799	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	135532	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	63377	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	50329	4.273	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.400%
7) Chloroethane-d5	1.568	69	40560	5.567	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.400%
11) 1,1-Dichloroethene-d2	2.108	63	68974	4.059	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.200%
20) 2-Butanone-d5	3.886	46	78930	41.772	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	83.540%
24) Chloroform-d	4.349	84	93682	4.892	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	5.030	65	42871	4.749	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.000%
32) Benzene-d6	5.050	84	181198	4.579	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
36) 1,2-Dichloropropane-d6	6.069	67	54324	4.460	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.200%
41) Toluene-d8	7.317	98	159936	4.500	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.000%
43) trans-1,3-Dichloroprop...	7.622	79	19048	4.463	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.200%
46) 2-Hexanone-d5	8.088	63	66628	42.167	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.340%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	34609	4.115	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	57518	5.087	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.800%
Target Compounds					Qvalue	
13) Acetone	2.175	43	2549	2.750	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
Data File : VV023136.D
Acq On : 02 Nov 2021 10:31
Operator : SY/MD
Sample : M4412-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG357

Quant Time: Nov 02 22:40:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 22:38:58 2021
Response via : Initial Calibration

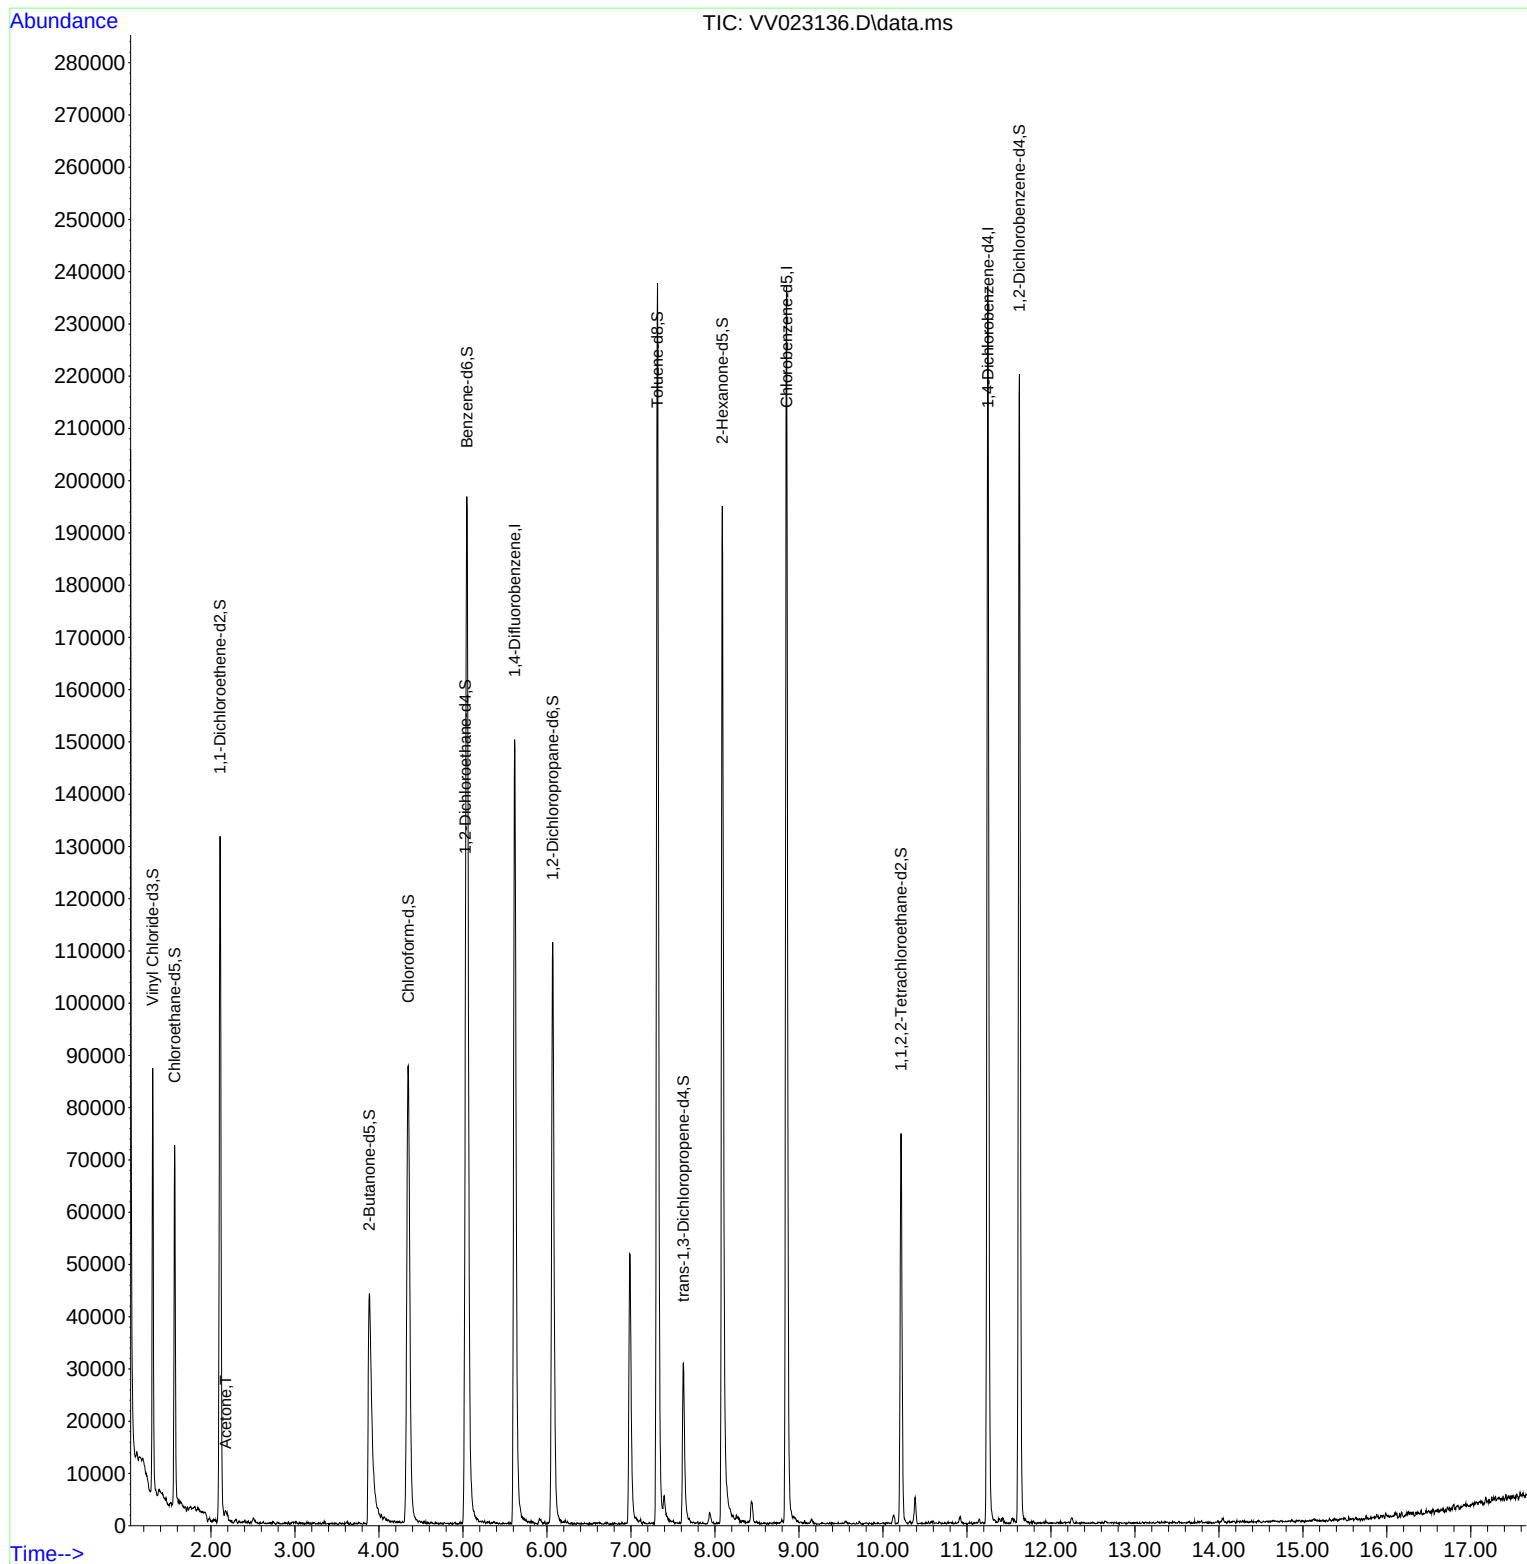

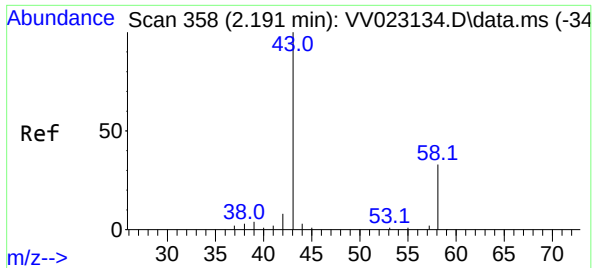

#13
 Acetone
 Concen: 2.750 ug/L
 RT: 2.175 min Scan# 31
 Delta R.T. -0.016 min
 Lab File: VV023136.D
 Acq: 02 Nov 2021 10:31

Instrument :
 MSVOA_V
 ClientSampleId :
 BG357

Tgt Ion: 43 Resp: 2549
 Ion Ratio Lower Upper
 43 100
 58 17.7 0.0 55.4

