

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
 Data File : VV023138.D
 Acq On : 02 Nov 2021 11:16
 Operator : SY/MD
 Sample : M4412-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG365

Quant Time: Nov 02 22:40:48 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 22:38:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	119575	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	122324	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	57781	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	47532	4.549	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	91.000%	
7) Chloroethane-d5	1.568	69	37652	5.826	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	116.600%	
11) 1,1-Dichloroethene-d2	2.111	63	64321	4.267	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	85.400%	
20) 2-Butanone-d5	3.889	46	77446	46.205	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	92.420%	
24) Chloroform-d	4.352	84	88500	5.210	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.200%	
26) 1,2-Dichloroethane-d4	5.037	65	41042	5.126	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.600%	
32) Benzene-d6	5.053	84	173371	4.855	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.000%	
36) 1,2-Dichloropropane-d6	6.072	67	51991	4.729	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	94.600%	
41) Toluene-d8	7.320	98	151415	4.720	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.400%	
43) trans-1,3-Dichloroprop...	7.625	79	18642	4.840	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	96.800%	
46) 2-Hexanone-d5	8.088	63	64082	44.935	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	89.860%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	33306	4.387	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	87.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	54488	5.285	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	105.800%	
Target Compounds						
13) Acetone	2.172	43	1843	2.241	ug/L	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
Data File : VV023138.D
Acq On : 02 Nov 2021 11:16
Operator : SY/MD
Sample : M4412-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG365

Quant Time: Nov 02 22:40:48 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 22:38:58 2021
Response via : Initial Calibration

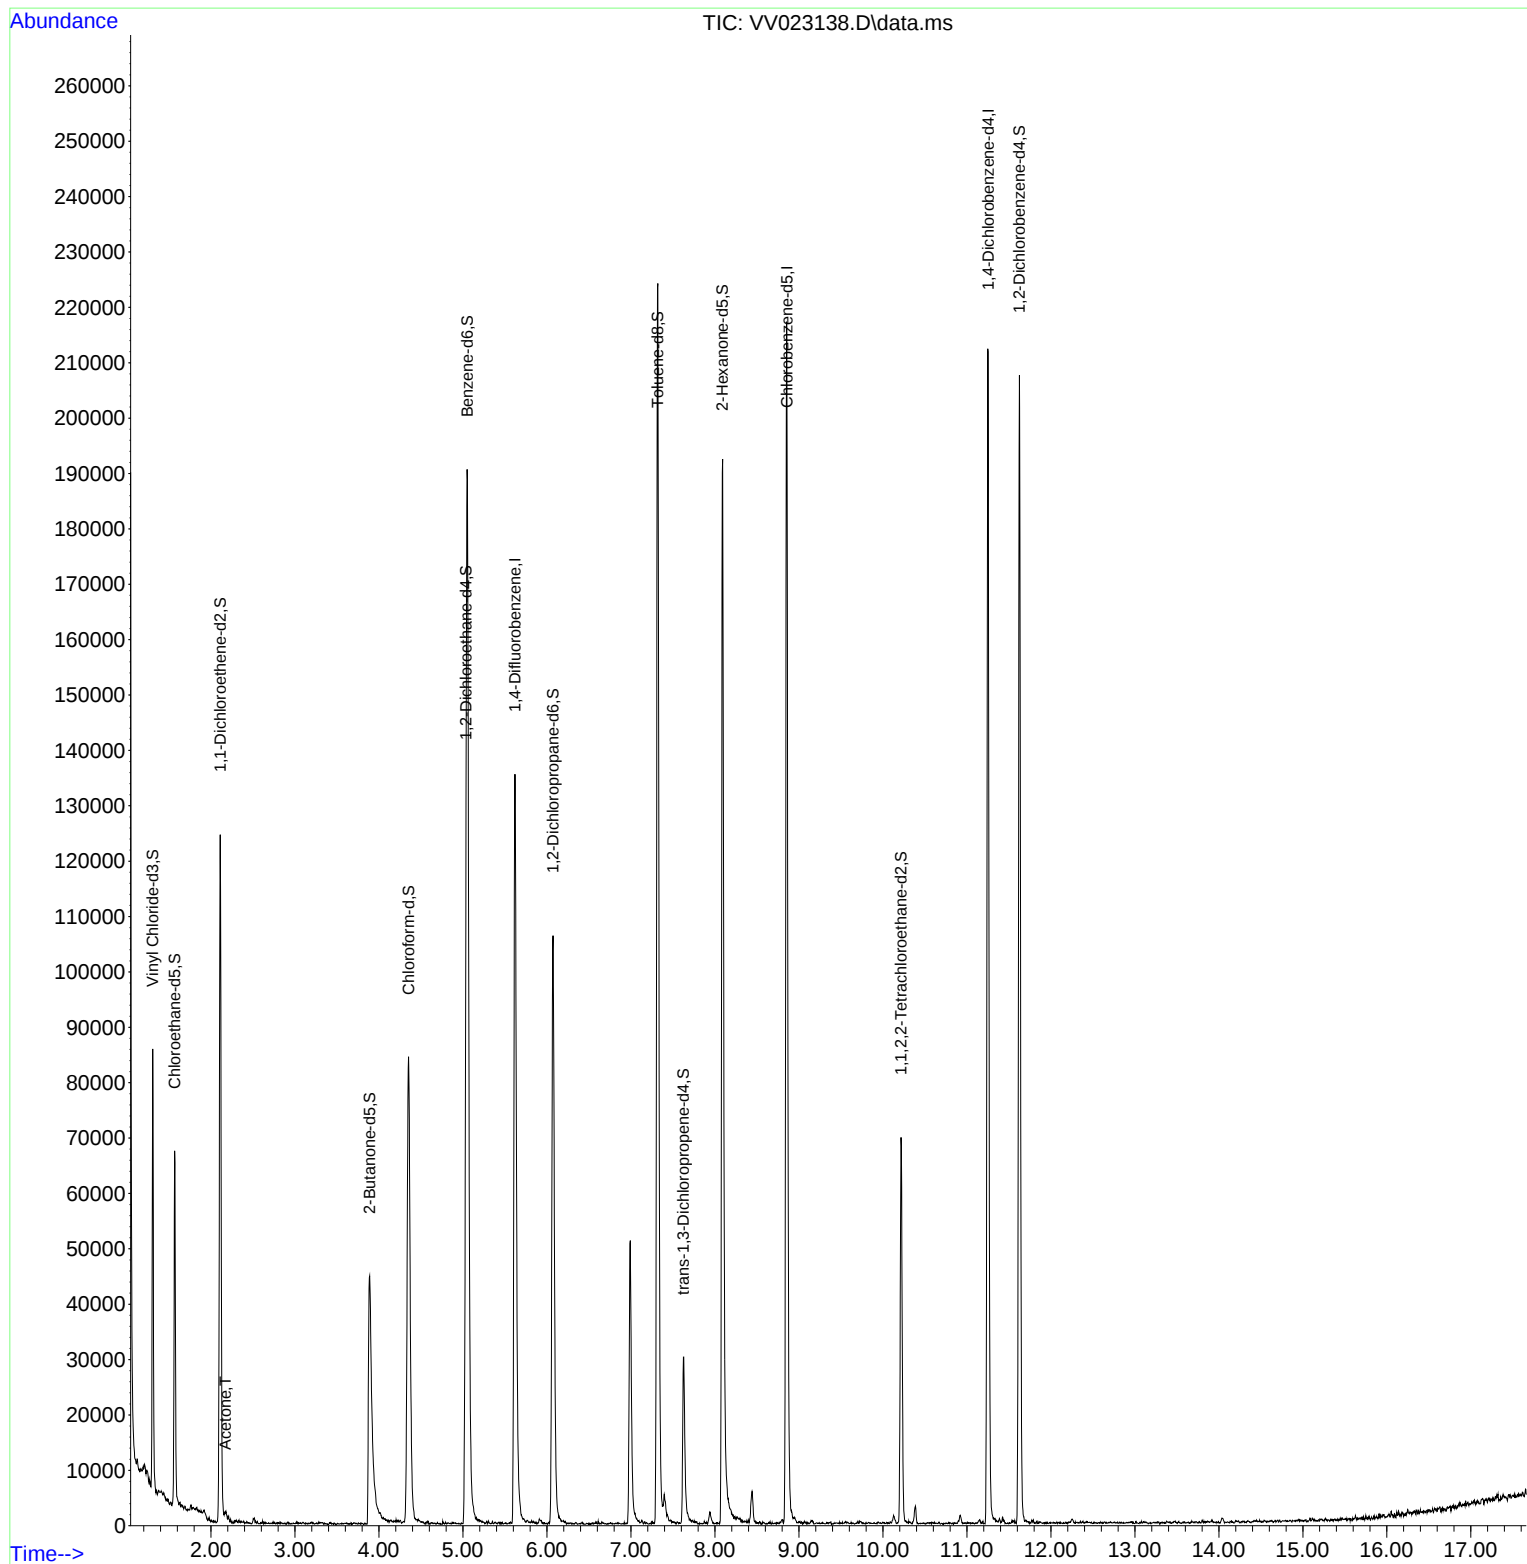

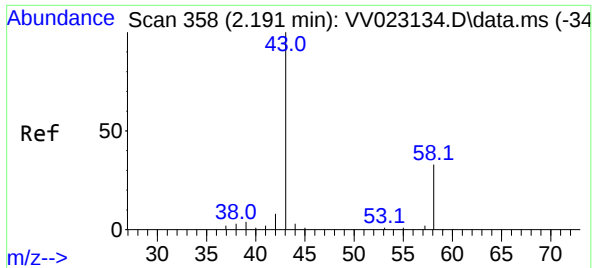

#13
 Acetone
 Concen: 2.241 ug/L
 RT: 2.172 min Scan# 31
 Delta R.T. -0.019 min
 Lab File: VV023138.D
 Acq: 02 Nov 2021 11:16

Instrument :
 MSVOA_V
 ClientSampleId :
 BG365

Tgt Ion: 43 Resp: 1843
 Ion Ratio Lower Upper
 43 100
 58 36.5 0.0 55.4

