

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110221\
 Data File : VW023140.D
 Acq On : 02 Nov 2021 12:02
 Operator : SY/MD
 Sample : M4412-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG367

Quant Time: Nov 02 22:41:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 22:38:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	125104	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	127923	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	61204	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	48026	4.393	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	87.800%	
7) Chloroethane-d5	1.567	69	38570	5.704	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	114.000%	
11) 1,1-Dichloroethene-d2	2.111	63	65244	4.137	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	82.800%	
20) 2-Butanone-d5	3.886	46	83616	47.682	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	95.360%	
24) Chloroform-d	4.352	84	92717	5.217	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.400%	
26) 1,2-Dichloroethane-d4	5.037	65	43654	5.211	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.200%	
32) Benzene-d6	5.053	84	180162	4.824	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.400%	
36) 1,2-Dichloropropane-d6	6.072	67	53375	4.642	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	92.800%	
41) Toluene-d8	7.320	98	155583	4.638	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.800%	
43) trans-1,3-Dichloroprop...	7.628	79	19776	4.909	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	98.200%	
46) 2-Hexanone-d5	8.091	63	67448	45.225	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	90.460%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	35708	4.498	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	90.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	58968	5.400	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	108.000%	
Target Compounds					Qvalue	
13) Acetone	2.175	43	2261	2.628	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
Data File : VV023140.D
Acq On : 02 Nov 2021 12:02
Operator : SY/MD
Sample : M4412-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG367

Quant Time: Nov 02 22:41:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 22:38:58 2021
Response via : Initial Calibration

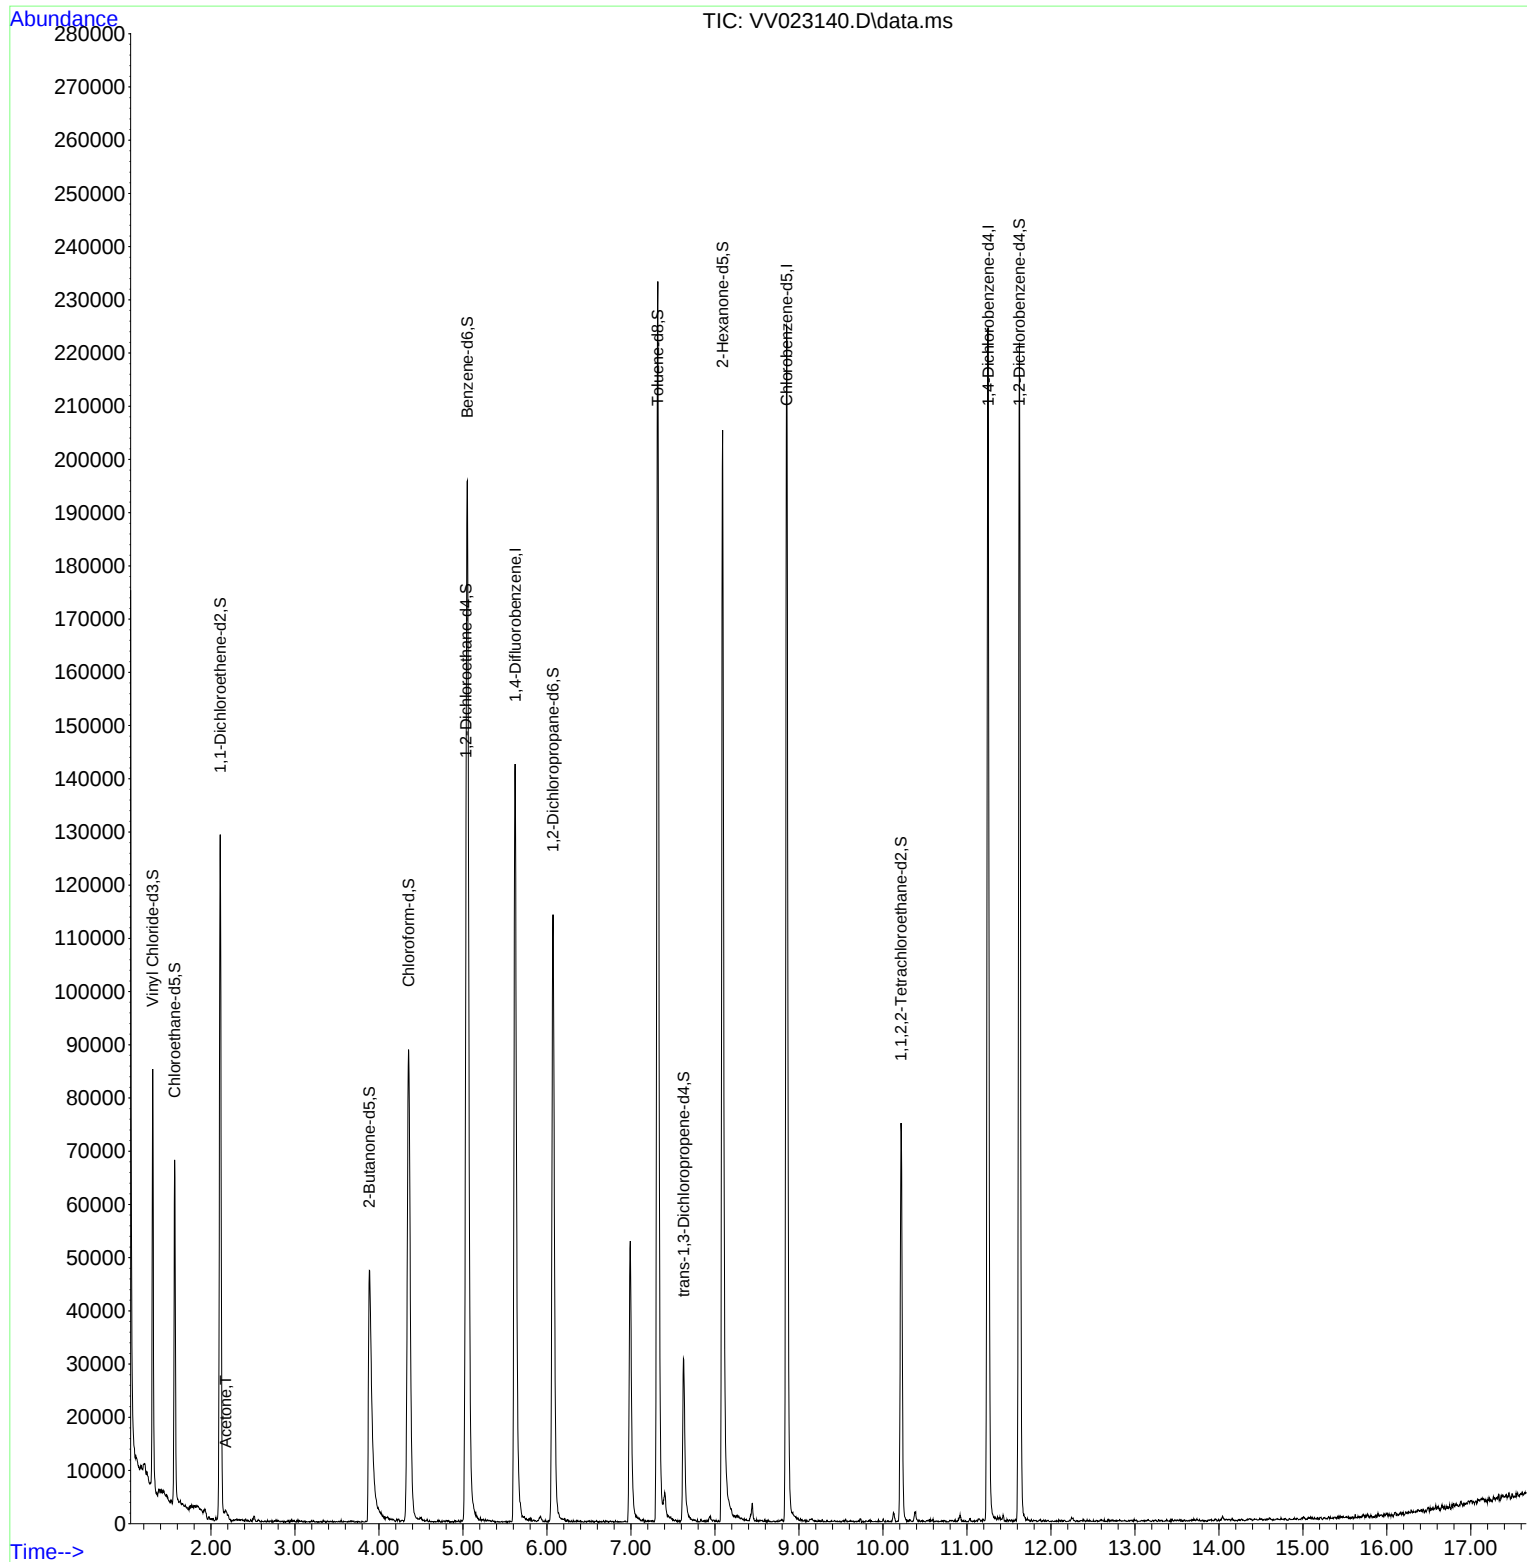

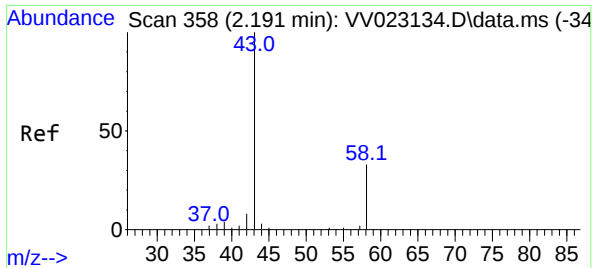

#13
Acetone
Concen: 2.628 ug/L
RT: 2.175 min Scan# 31
Delta R.T. -0.016 min
Lab File: VV023140.D
Acq: 02 Nov 2021 12:02

Instrument :
MSVOA_V
ClientSampleId :
BG367

Tgt Ion: 43 Resp: 2261
Ion Ratio Lower Upper
43 100
58 28.8 0.0 55.4

