

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
 Data File : VV023144.D
 Acq On : 02 Nov 2021 13:35
 Operator : SY/MD
 Sample : M4400-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG349

Quant Time: Nov 02 22:42:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 22:38:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	125580	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	128739	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	59900	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	46997	4.283	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	85.600%	
7) Chloroethane-d5	1.568	69	36884	5.434	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	108.600%	
11) 1,1-Dichloroethene-d2	2.108	63	64932	4.102	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	82.000%	
20) 2-Butanone-d5	3.886	46	81235	46.148	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	92.300%	
24) Chloroform-d	4.352	84	91464	5.127	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.600%	
26) 1,2-Dichloroethane-d4	5.037	65	42289	5.029	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.600%	
32) Benzene-d6	5.053	84	177331	4.718	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.400%	
36) 1,2-Dichloropropane-d6	6.072	67	51866	4.483	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	89.600%	
41) Toluene-d8	7.320	98	152792	4.526	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.600%	
43) trans-1,3-Dichloroprop...	7.625	79	18596	4.587	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	91.800%	
46) 2-Hexanone-d5	8.088	63	66822	44.521	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	89.040%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	35213	4.408	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	88.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	57776	5.406	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	108.200%	
Target Compounds					Qvalue	
13) Acetone	2.172	43	2411	2.792	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
Data File : VV023144.D
Acq On : 02 Nov 2021 13:35
Operator : SY/MD
Sample : M4400-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG349


Quant Time: Nov 02 22:42:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 22:38:58 2021
Response via : Initial Calibration

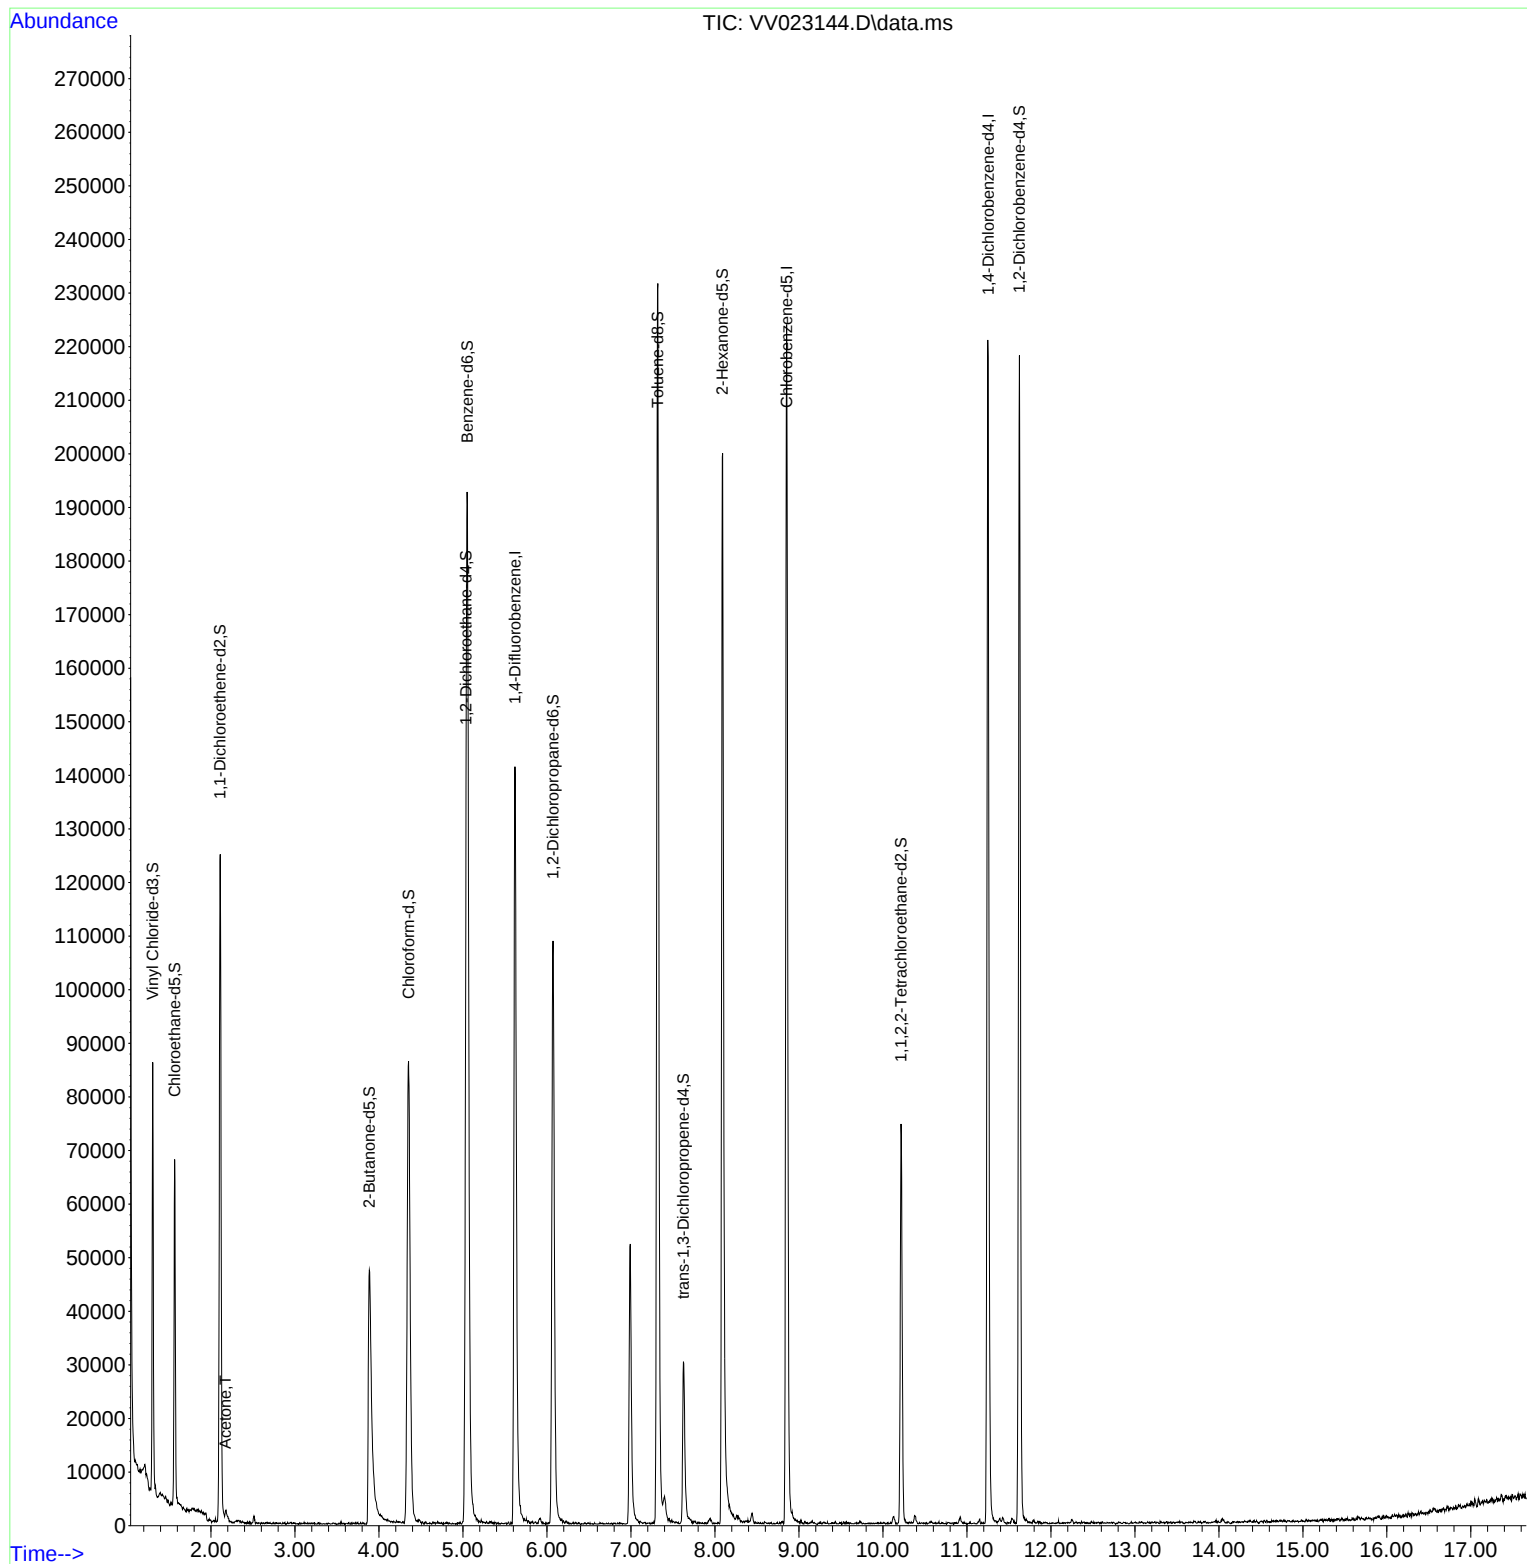

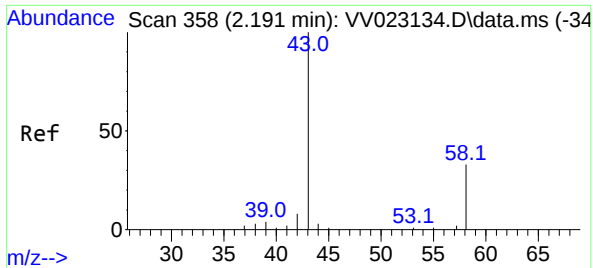

#13
Acetone
Concen: 2.792 ug/L
RT: 2.172 min Scan# 31
Delta R.T. -0.019 min
Lab File: VV023144.D
Acq: 02 Nov 2021 13:35

Instrument :
MSVOA_V
ClientSampleId :
BG349

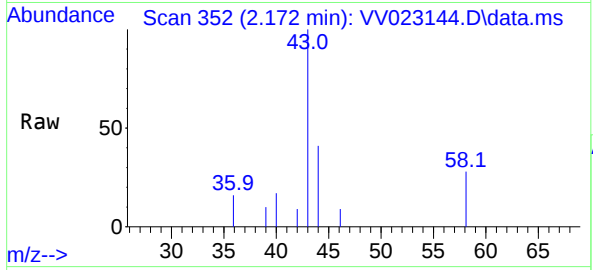

Tgt Ion: 43 Resp: 2411
Ion Ratio Lower Upper
43 100
58 24.9 0.0 55.4

