

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110221\
 Data File : VW023147.D
 Acq On : 02 Nov 2021 14:45
 Operator : SY/MD
 Sample : M4443-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B08

Quant Time: Nov 02 22:42:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 22:38:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	128409	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	130378	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61769	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	43019	3.834	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.600%
7) Chloroethane-d5	1.568	69	34722	5.003	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.000%
11) 1,1-Dichloroethene-d2	2.108	63	59204	3.658	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.200%
20) 2-Butanone-d5	3.892	46	80438	44.689	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.380%
24) Chloroform-d	4.352	84	83514	4.578	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
26) 1,2-Dichloroethane-d4	5.037	65	40124	4.666	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.400%
32) Benzene-d6	5.053	84	164105	4.311	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.200%
36) 1,2-Dichloropropane-d6	6.072	67	49559	4.229	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.600%
41) Toluene-d8	7.317	98	141497	4.138	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.800%
43) trans-1,3-Dichloroprop...	7.628	79	17109	4.167	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.400%
46) 2-Hexanone-d5	8.091	63	64613	42.508	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.020%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	33164	4.099	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	53777	4.879	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.600%
Target Compounds						Qvalue
34) Trichloroethene	5.931	95	487	0.055	ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
Data File : VV023147.D
Acq On : 02 Nov 2021 14:45
Operator : SY/MD
Sample : M4443-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B08


Quant Time: Nov 02 22:42:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 22:38:58 2021
Response via : Initial Calibration

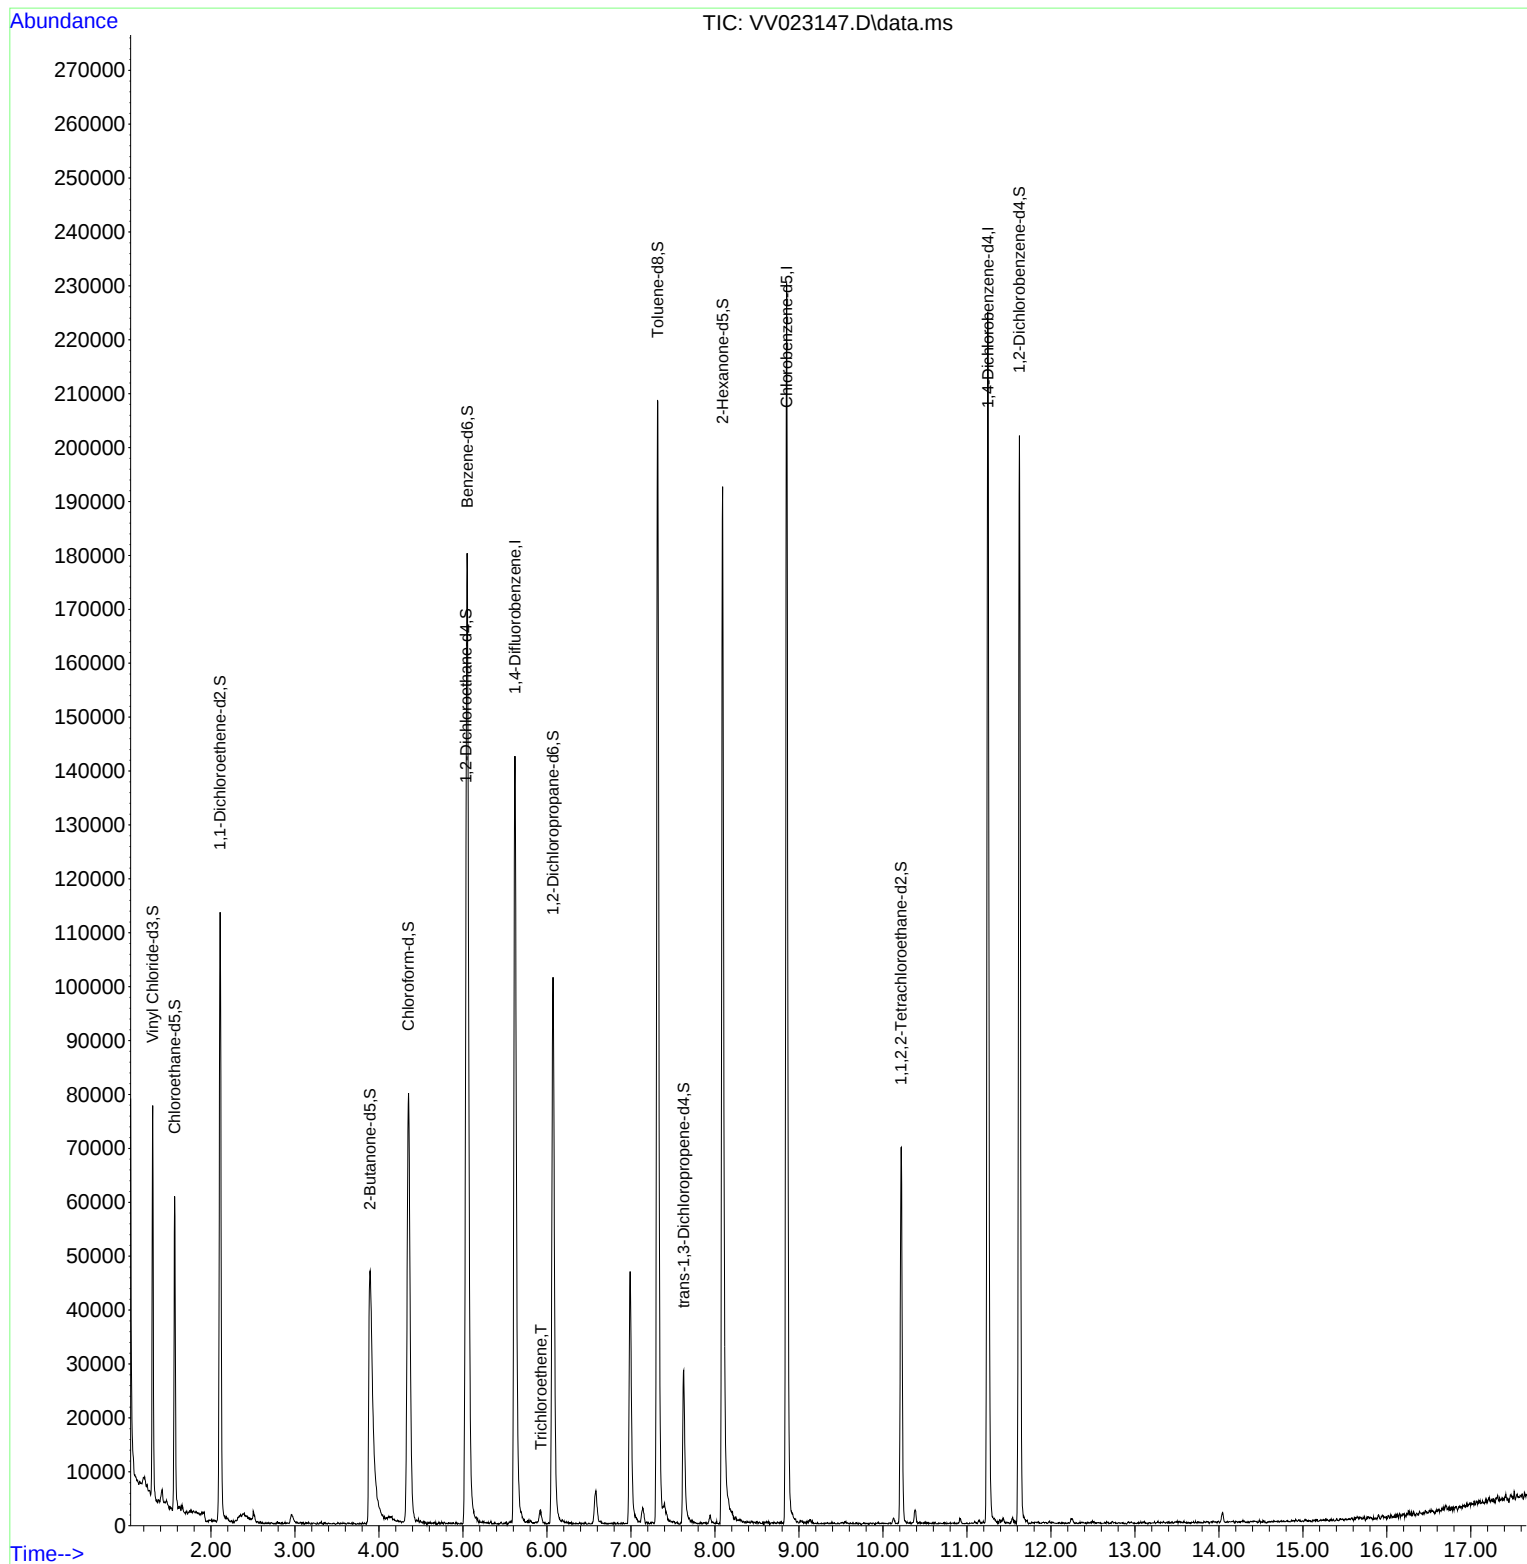

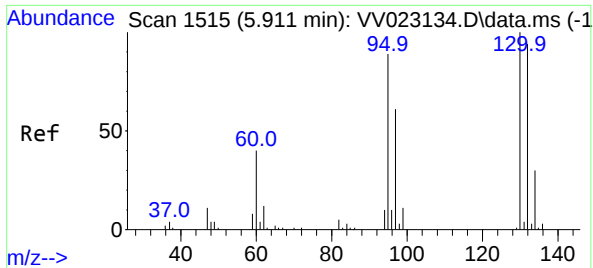

#34
 Trichloroethene
 Concen: 0.055 ug/L
 RT: 5.931 min Scan# 11
 Delta R.T. 0.019 min
 Lab File: VV023147.D
 Acq: 02 Nov 2021 14:45

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B08

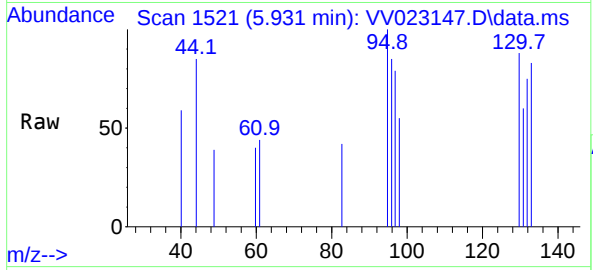

Tgt Ion: 95 Resp: 487

Ion	Ratio	Lower	Upper
95	100		
97	79.2	45.0	83.6
132	75.5	69.7	129.4
130	87.5	73.7	136.9

