

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
 Data File : VV023151.D
 Acq On : 02 Nov 2021 16:46
 Operator : SY/MD
 Sample : VV1102WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK239

Quant Time: Nov 02 23:32:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 23:31:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	121877	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	123378	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	59902	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	41473	3.894	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.800%
7) Chloroethane-d5	1.568	69	34241	5.198	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.000%
11) 1,1-Dichloroethene-d2	2.108	63	58614	3.815	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.400%
20) 2-Butanone-d5	3.902	46	76569	44.819	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.640%
24) Chloroform-d	4.352	84	85673	4.948	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.000%
26) 1,2-Dichloroethane-d4	5.037	65	41495	5.084	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%
32) Benzene-d6	5.053	84	165343	4.590	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.800%
36) 1,2-Dichloropropane-d6	6.072	67	50125	4.520	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.400%
41) Toluene-d8	7.317	98	143658	4.440	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.800%
43) trans-1,3-Dichloroprop...	7.625	79	17969	4.625	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.600%
46) 2-Hexanone-d5	8.092	63	75406	52.424	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.840%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	35807	4.677	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	56028	5.242	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.800%
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	4290	0.626	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
Data File : VV023151.D
Acq On : 02 Nov 2021 16:46
Operator : SY/MD
Sample : VV1102WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK239


Quant Time: Nov 02 23:32:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 23:31:16 2021
Response via : Initial Calibration

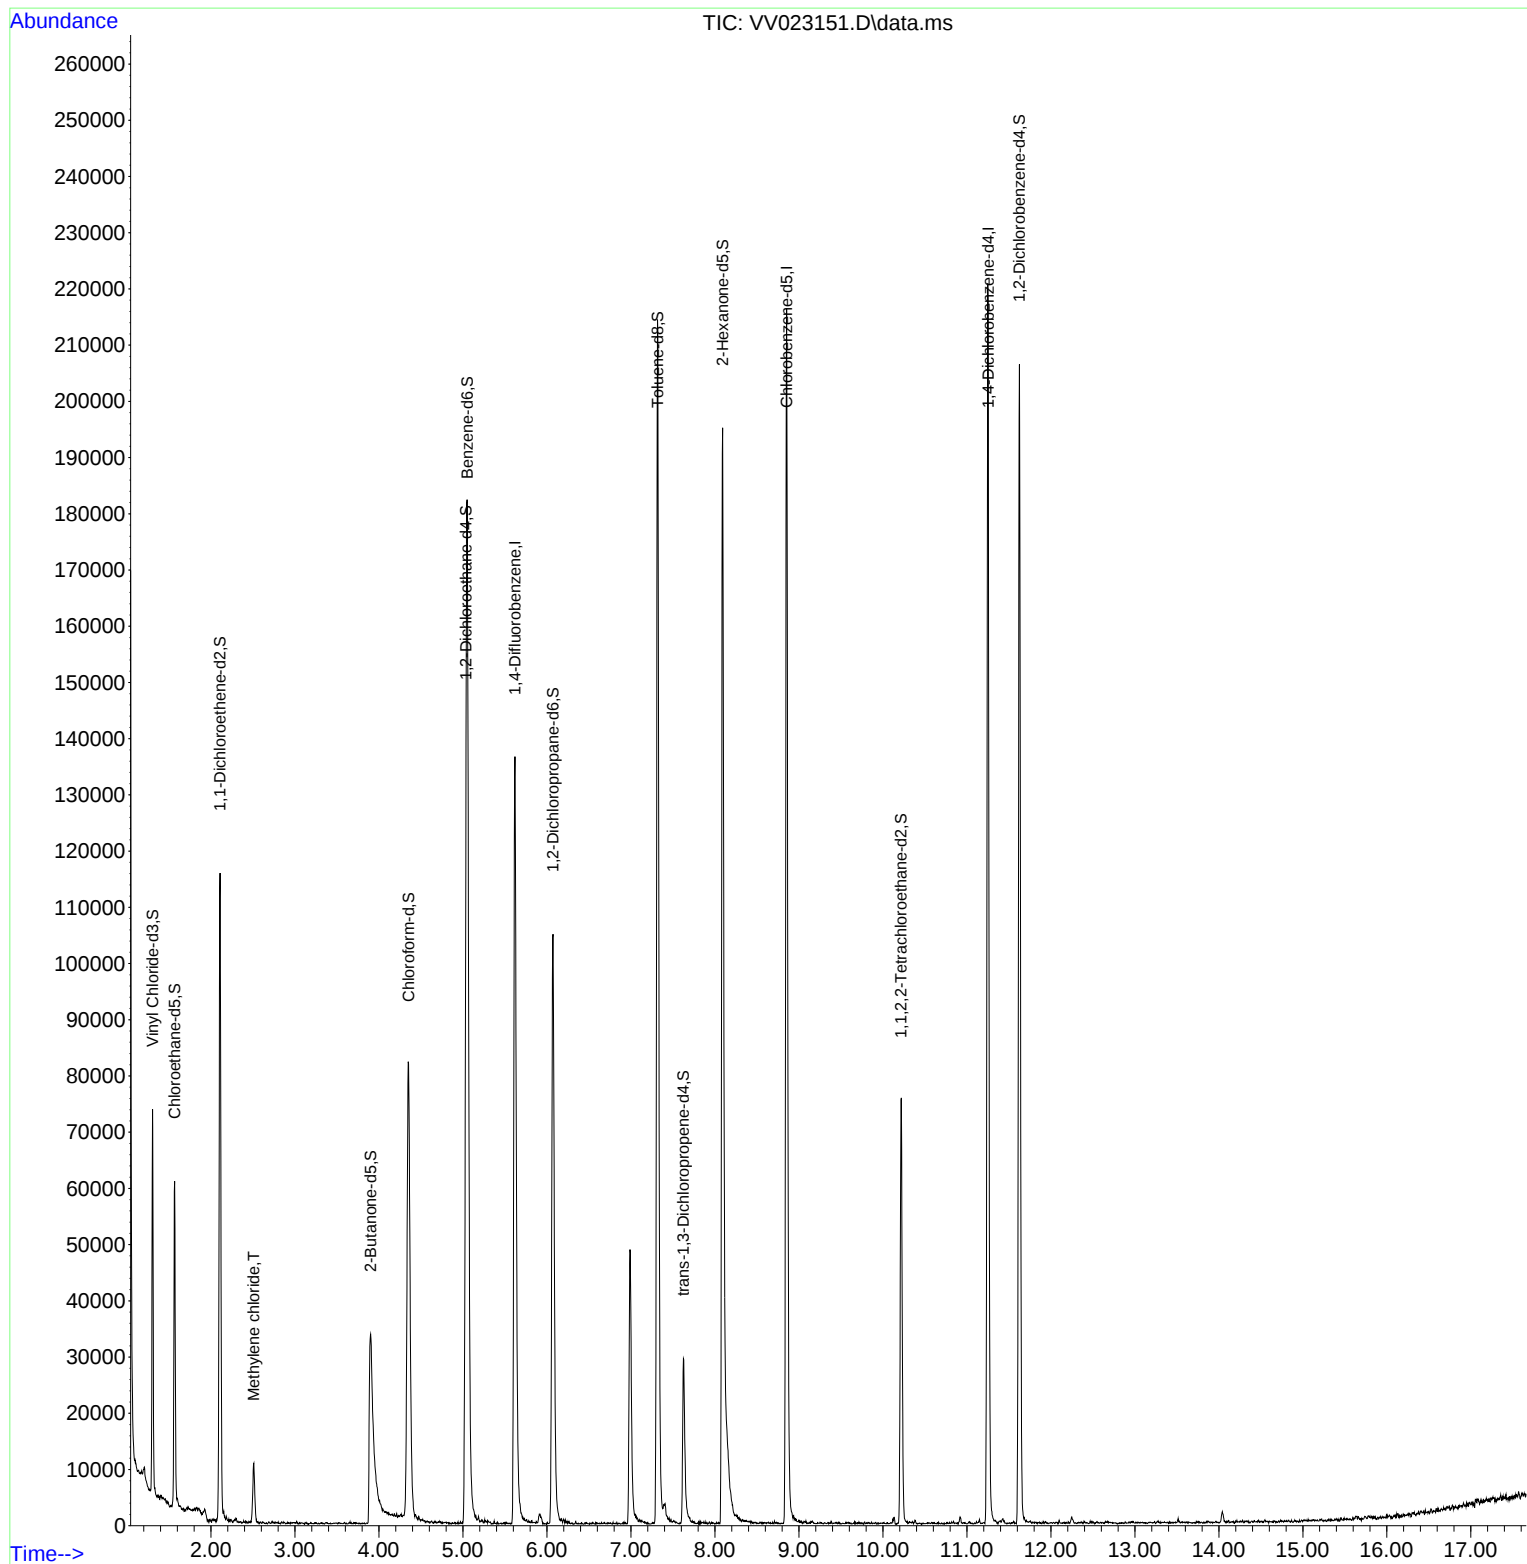

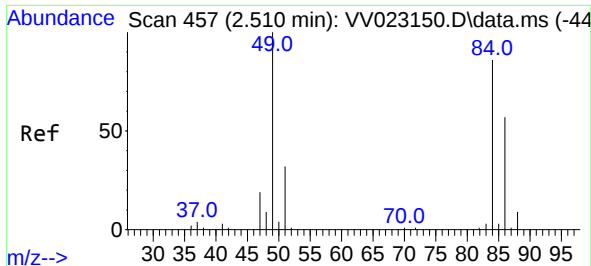

#16
Methylene chloride
Concen: 0.626 ug/L
RT: 2.510 min Scan# 4
Delta R.T. 0.000 min
Lab File: VV023151.D
Acq: 02 Nov 2021 16:46

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

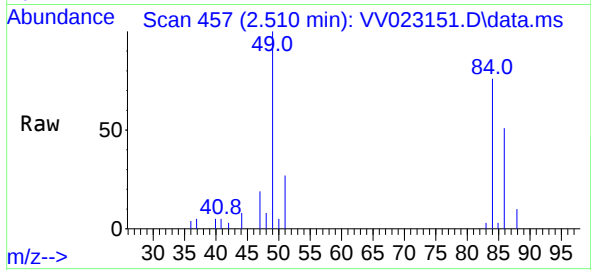

Tgt Ion: 84 Resp: 4290

Ion	Ratio	Lower	Upper
84	100		
86	66.7	42.3	78.5
49	131.1	79.7	148.1

