

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
 Data File : VV023152.D
 Acq On : 02 Nov 2021 17:10
 Operator : SY/MD
 Sample : M4443-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 02 23:32:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 23:31:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	123868	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	125111	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	58901	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	42639	3.939	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.800%
7) Chloroethane-d5	1.567	69	36325	5.426	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.600%
11) 1,1-Dichloroethene-d2	2.108	63	60250	3.859	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.200%
20) 2-Butanone-d5	3.905	46	96518	55.588	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.180%
24) Chloroform-d	4.352	84	90272	5.130	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.600%
26) 1,2-Dichloroethane-d4	5.037	65	43468	5.240	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.800%
32) Benzene-d6	5.053	84	173565	4.752	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.000%
36) 1,2-Dichloropropane-d6	6.072	67	52378	4.658	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.200%
41) Toluene-d8	7.320	98	150819	4.597	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.000%
43) trans-1,3-Dichloroprop...	7.625	79	19461	4.940	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.800%
46) 2-Hexanone-d5	8.091	63	81171	55.650	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.300%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	37342	4.810	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	56668	5.392	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.800%
Target Compounds						
					Qvalue	
16) Methylene chloride	2.510	84	4634	0.665	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
Data File : VV023152.D
Acq On : 02 Nov 2021 17:10
Operator : SY/MD
Sample : M4443-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Nov 02 23:32:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 23:31:16 2021
Response via : Initial Calibration

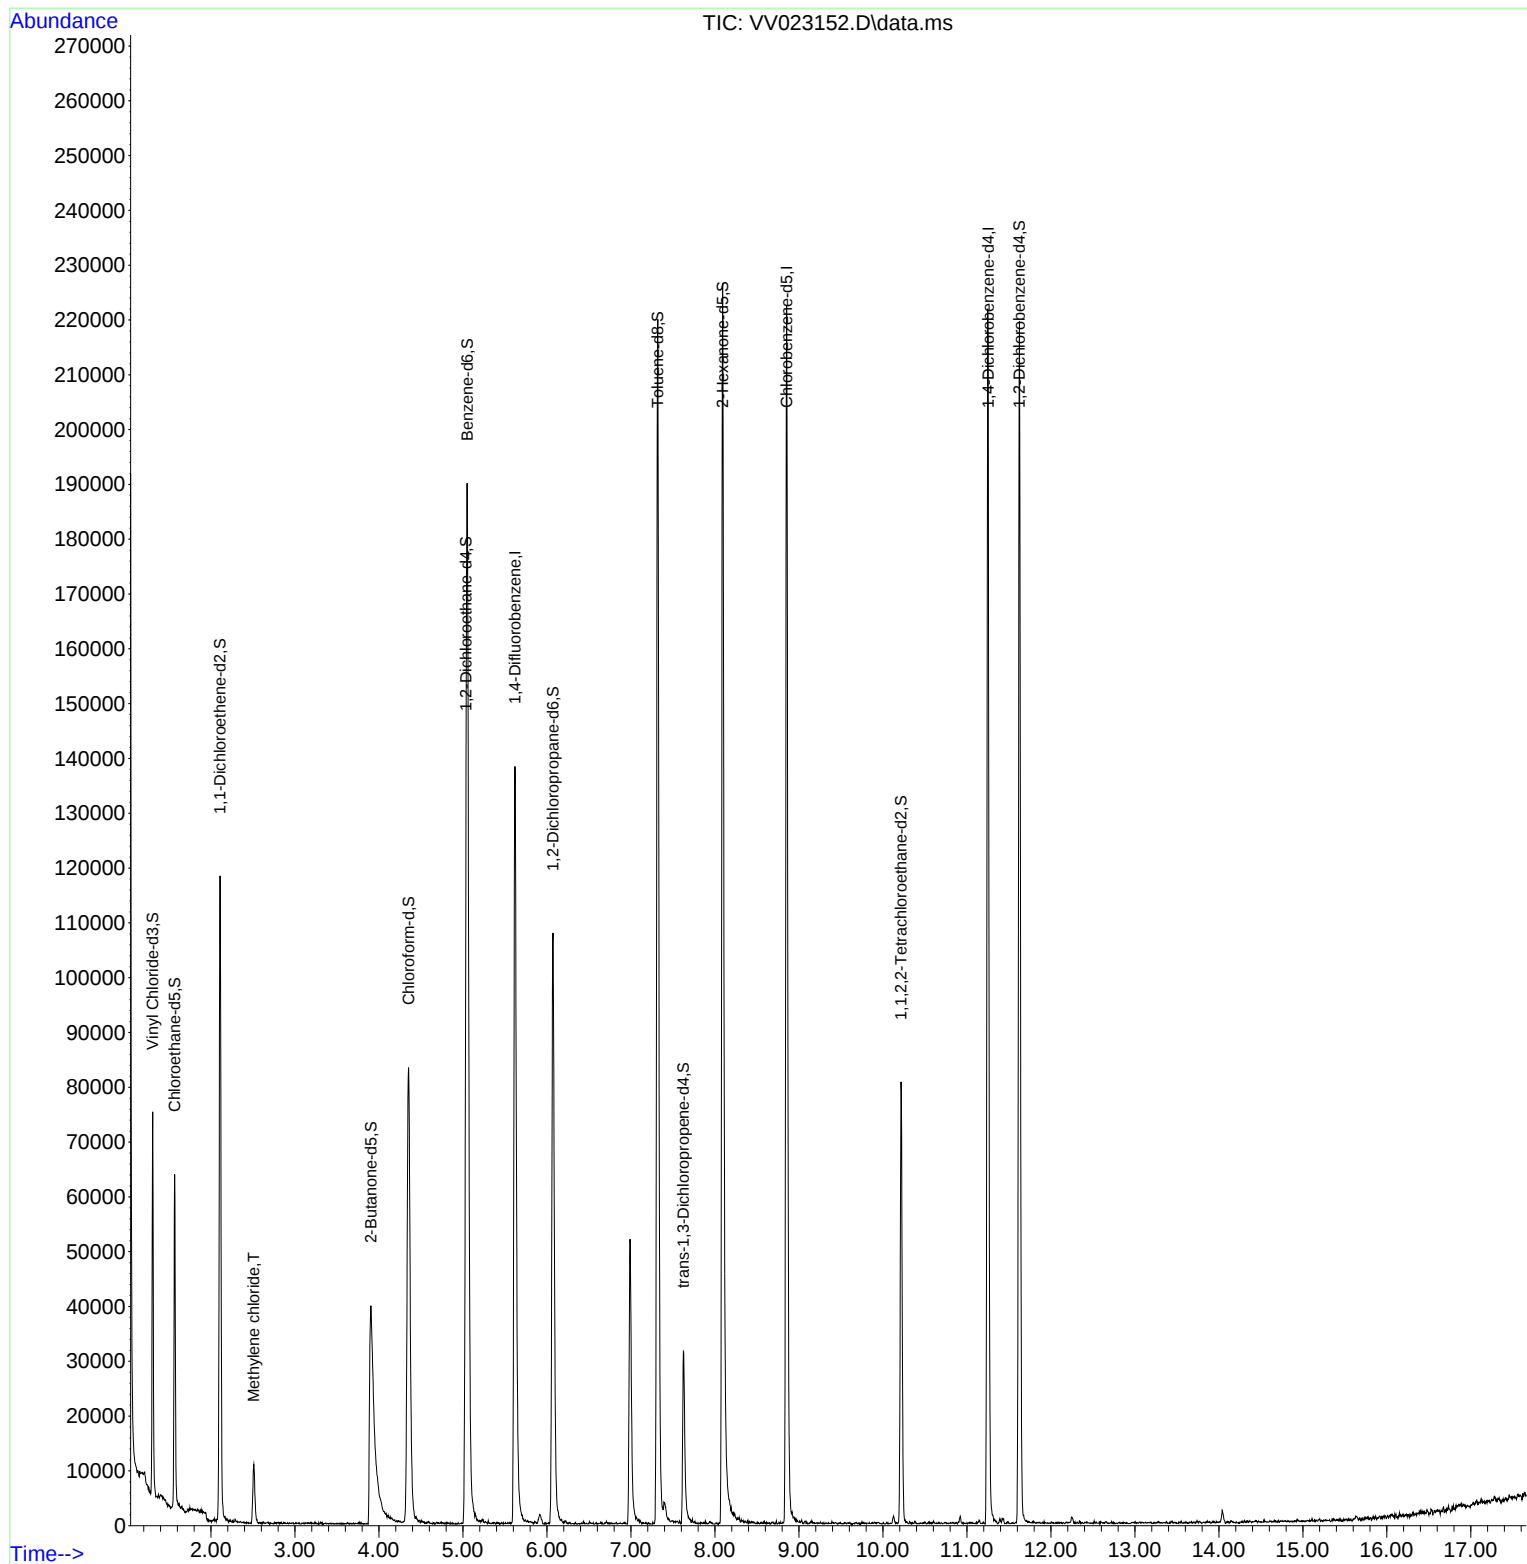

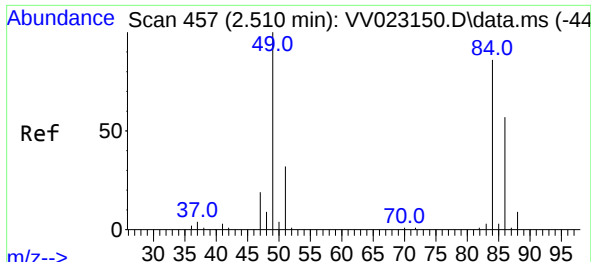

#16
Methylene chloride
Concen: 0.665 ug/L
RT: 2.510 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV023152.D
Acq: 02 Nov 2021 17:10

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

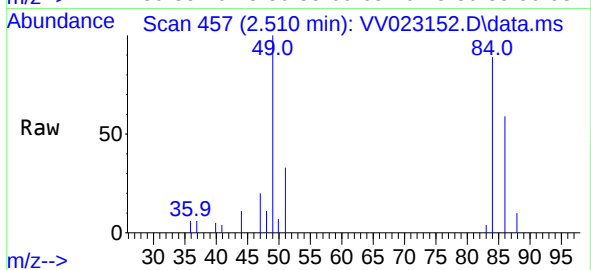

Tgt Ion: 84 Resp: 4634

Ion	Ratio	Lower	Upper
84	100		
86	67.0	42.3	78.5
49	112.6	79.7	148.1

