

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
 Data File : VV023154.D
 Acq On : 02 Nov 2021 17:56
 Operator : SY/MD
 Sample : M4400-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG351

Quant Time: Nov 02 23:33:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 23:31:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	123733	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	124494	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58183	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	46392	4.291	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	85.800%	
7) Chloroethane-d5	1.568	69	35084	5.246	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	105.000%	
11) 1,1-Dichloroethene-d2	2.108	63	62133	3.984	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	79.600%	
20) 2-Butanone-d5	3.889	46	89832	51.794	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	103.580%	
24) Chloroform-d	4.352	84	89770	5.107	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.200%	
26) 1,2-Dichloroethane-d4	5.034	65	43015	5.192	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.800%	
32) Benzene-d6	5.053	84	173092	4.762	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.200%	
36) 1,2-Dichloropropane-d6	6.072	67	52001	4.648	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	93.000%	
41) Toluene-d8	7.317	98	149316	4.573	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.400%	
43) trans-1,3-Dichloroprop...	7.625	79	19083	4.868	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	97.400%	
46) 2-Hexanone-d5	8.088	63	76370	52.618	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	105.240%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	36648	4.744	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	57441	5.533	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	110.600%	
Target Compounds					Qvalue	
13) Acetone	2.175	43	3881	4.561	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
Data File : VV023154.D
Acq On : 02 Nov 2021 17:56
Operator : SY/MD
Sample : M4400-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG351

Quant Time: Nov 02 23:33:00 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 23:31:16 2021
Response via : Initial Calibration

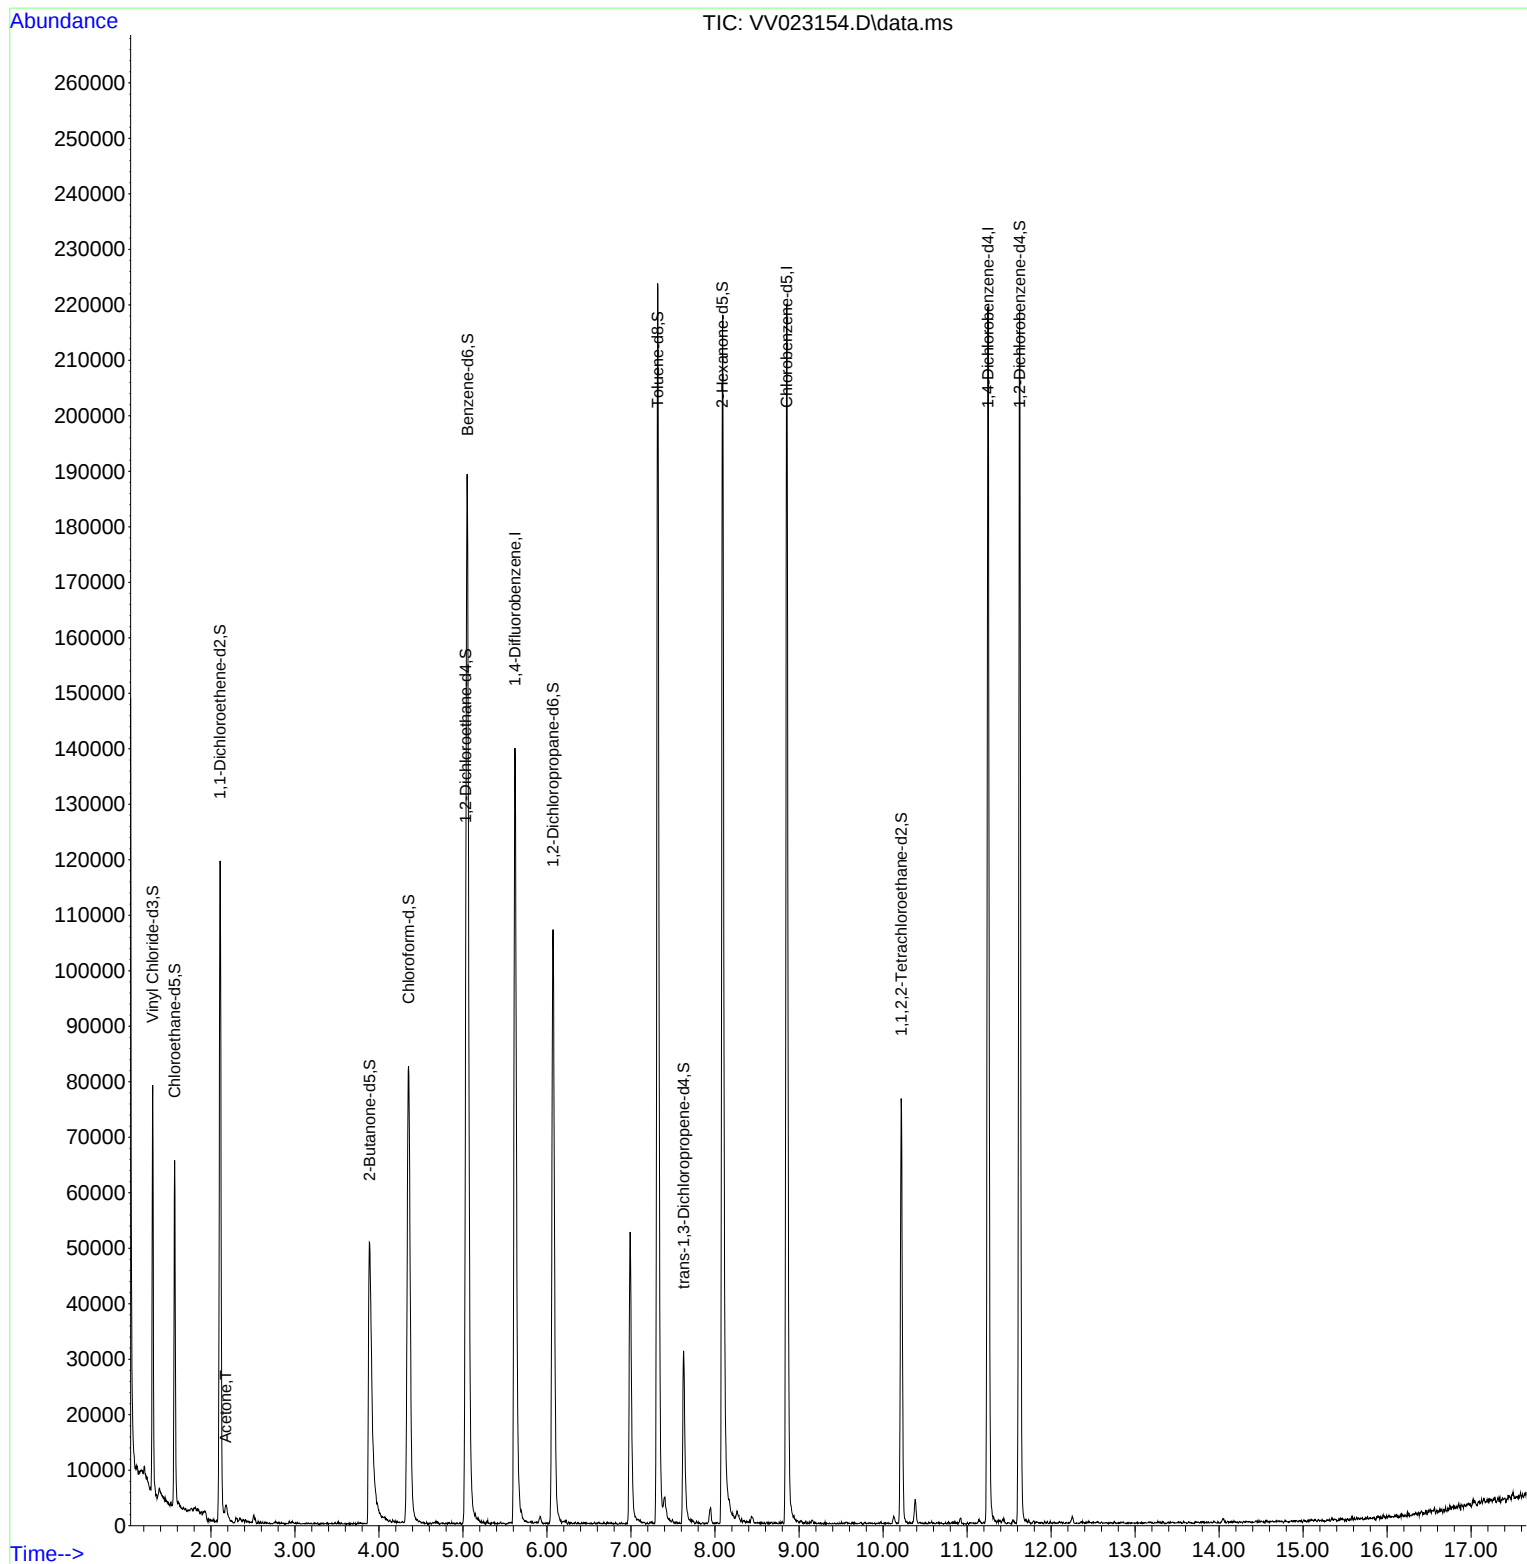

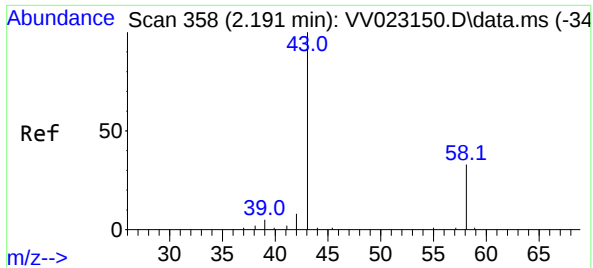

#13
 Acetone
 Concen: 4.561 ug/L
 RT: 2.175 min Scan# 31
 Delta R.T. -0.016 min
 Lab File: VV023154.D
 Acq: 02 Nov 2021 17:56

Instrument :
 MSVOA_V
 ClientSampleId :
 BG351

Tgt Ion: 43 Resp: 3881
 Ion Ratio Lower Upper
 43 100
 58 29.9 0.0 55.4

