

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
 Data File : VV023159.D
 Acq On : 02 Nov 2021 19:54
 Operator : SY/MD
 Sample : M4400-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG356

Quant Time: Nov 02 23:34:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 23:31:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	121554	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	123780	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	57975	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	43152	4.063	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.200%
7) Chloroethane-d5	1.568	69	34305	5.221	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.400%
11) 1,1-Dichloroethene-d2	2.108	63	59643	3.892	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.800%
20) 2-Butanone-d5	3.883	46	75386	44.244	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.480%
24) Chloroform-d	4.349	84	85234	4.936	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.800%
26) 1,2-Dichloroethane-d4	5.034	65	39355	4.835	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.600%
32) Benzene-d6	5.053	84	166005	4.594	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.800%
36) 1,2-Dichloropropane-d6	6.072	67	49944	4.489	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.800%
41) Toluene-d8	7.317	98	144190	4.442	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.800%
43) trans-1,3-Dichloroprop...	7.625	79	16912	4.339	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.800%
46) 2-Hexanone-d5	8.088	63	62317	43.183	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.360%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	33042	4.302	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	54207	5.240	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.800%
Target Compounds						
					Qvalue	
13) Acetone	2.175	43	2614	3.127	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
Data File : VV023159.D
Acq On : 02 Nov 2021 19:54
Operator : SY/MD
Sample : M4400-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG356

Quant Time: Nov 02 23:34:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 23:31:16 2021
Response via : Initial Calibration

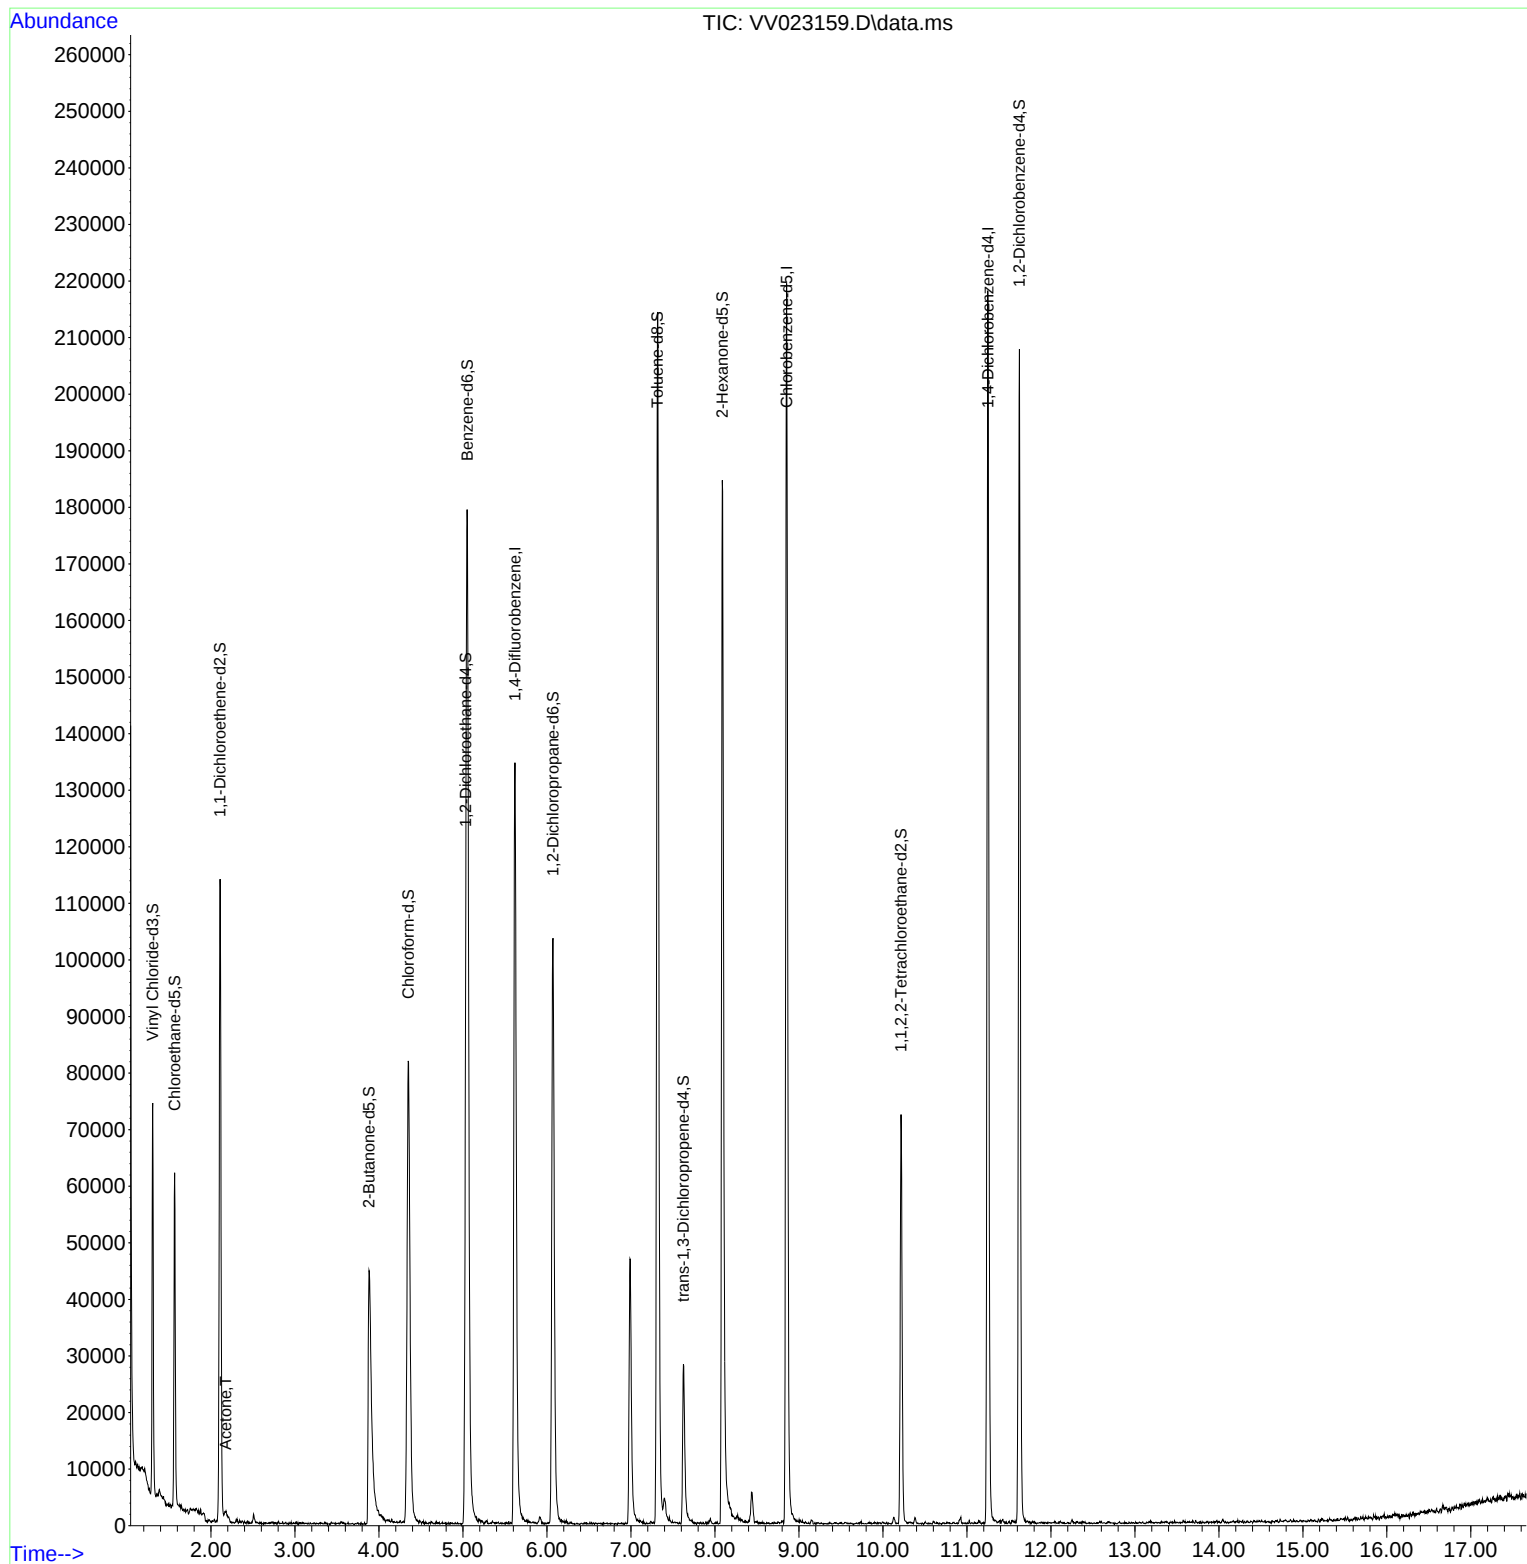

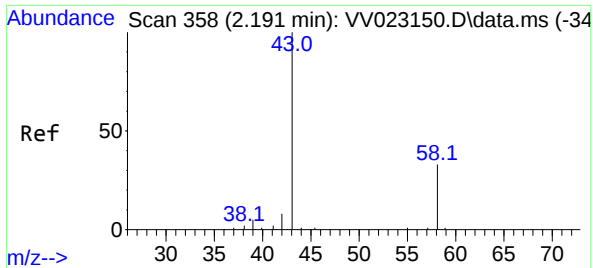

#13
Acetone
Concen: 3.127 ug/L
RT: 2.175 min Scan# 31
Delta R.T. -0.016 min
Lab File: VV023159.D
Acq: 02 Nov 2021 19:54

Instrument :
MSVOA_V
ClientSampleId :
BG356

Tgt Ion: 43 Resp: 2614
Ion Ratio Lower Upper
43 100
58 28.6 0.0 55.4

