

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
 Data File : VV023169.D
 Acq On : 02 Nov 2021 23:48
 Operator : SY/MD
 Sample : M4412-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 03 00:37:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 23:31:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	121232	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	123098	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	59236	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	42808	4.041	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.800%
7) Chloroethane-d5	1.568	69	34932	5.331	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.600%
11) 1,1-Dichloroethene-d2	2.108	63	59980	3.925	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.400%
20) 2-Butanone-d5	3.892	46	81599	48.018	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.040%
24) Chloroform-d	4.352	84	86204	5.006	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.200%
26) 1,2-Dichloroethane-d4	5.037	65	41006	5.051	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.000%
32) Benzene-d6	5.053	84	165009	4.591	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.800%
36) 1,2-Dichloropropane-d6	6.072	67	50316	4.548	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.000%
41) Toluene-d8	7.320	98	141471	4.382	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.600%
43) trans-1,3-Dichloroprop...	7.625	79	16806	4.336	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.800%
46) 2-Hexanone-d5	8.091	63	64934	45.246	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.500%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	33543	4.391	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.800%
66) 1,2-Dichlorobenzene-d4	11.625	152	53521	5.064	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.200%
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	7084	1.039	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
Data File : VV023169.D
Acq On : 02 Nov 2021 23:48
Operator : SY/MD
Sample : M4412-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 65 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Nov 03 00:37:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 23:31:16 2021
Response via : Initial Calibration

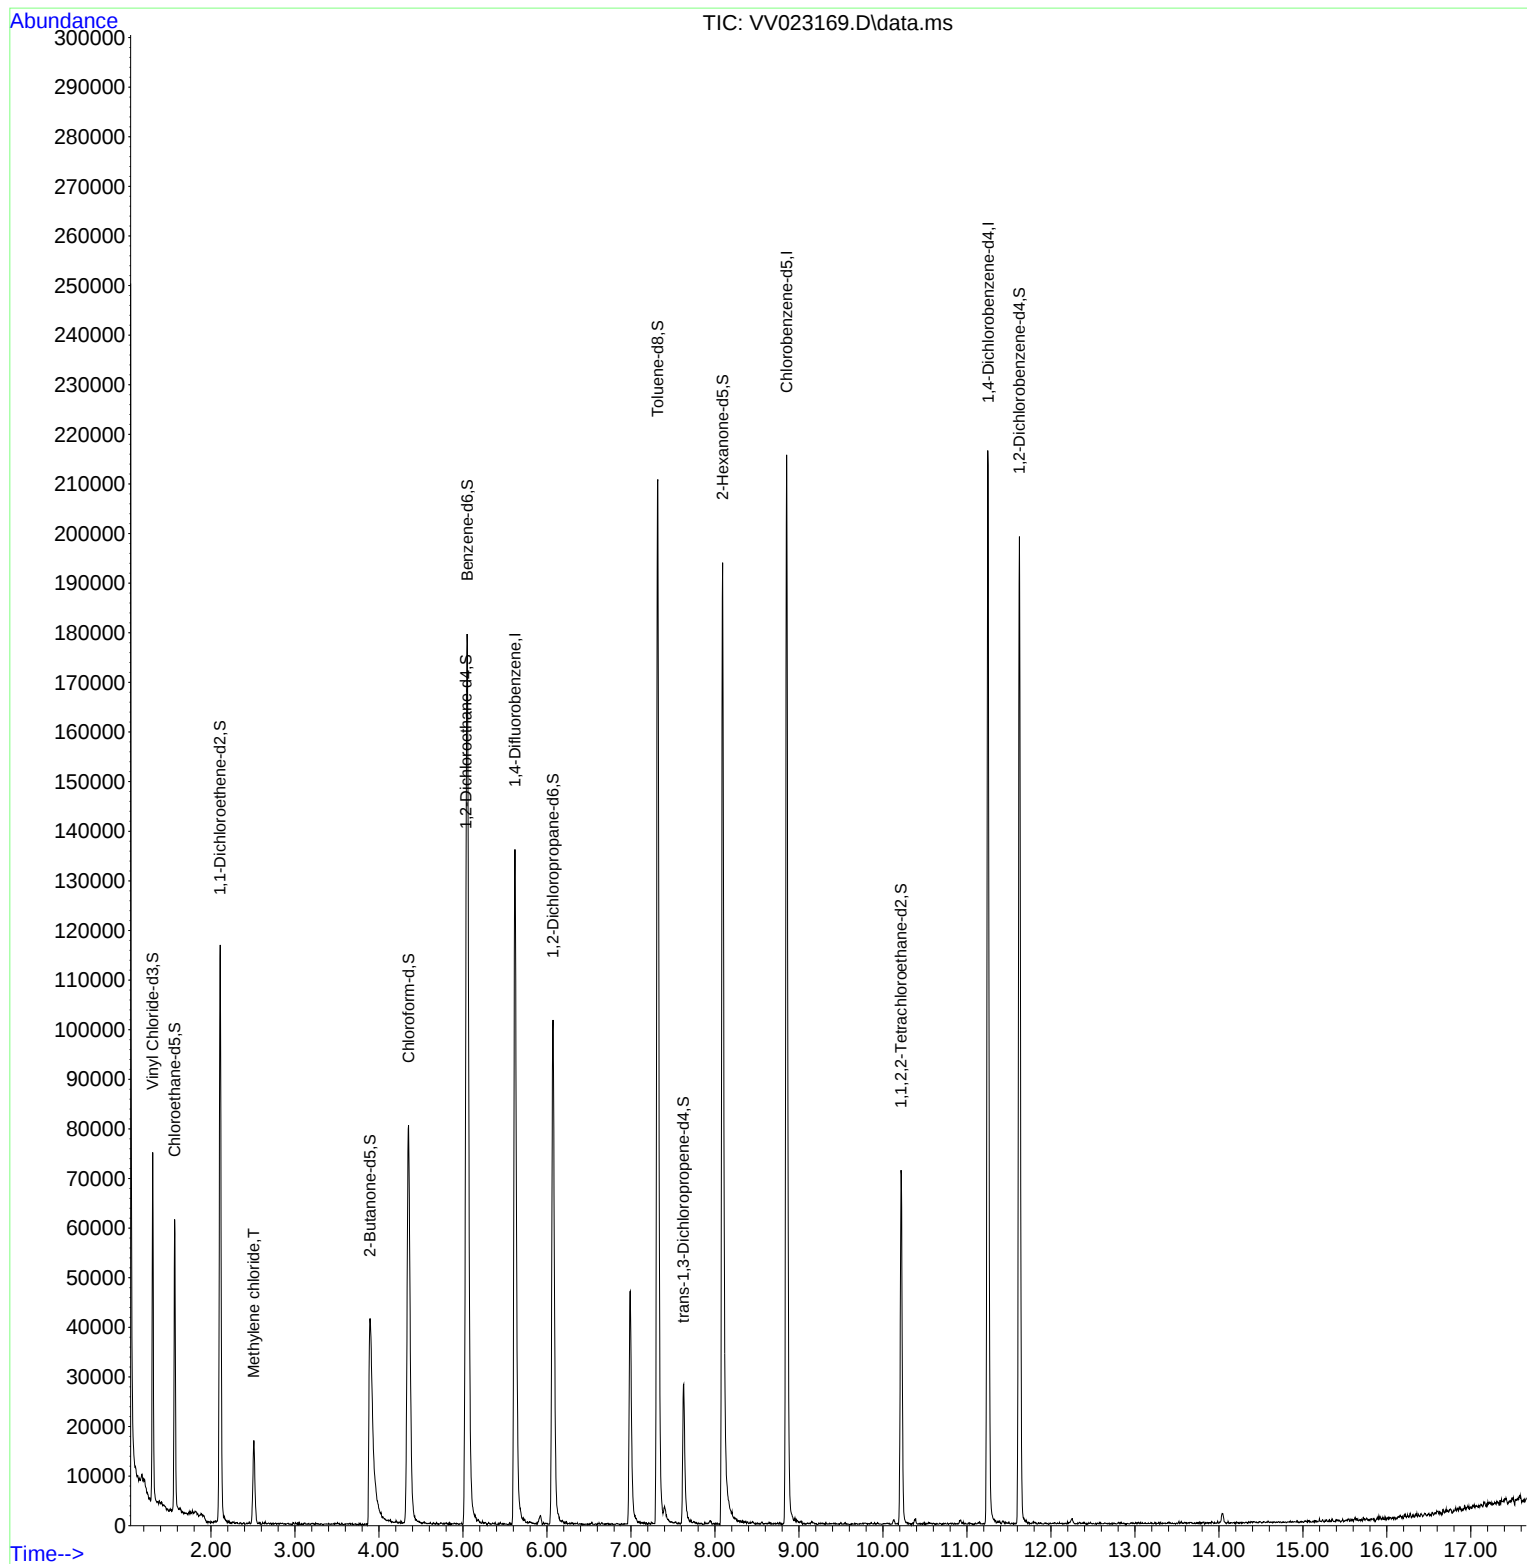

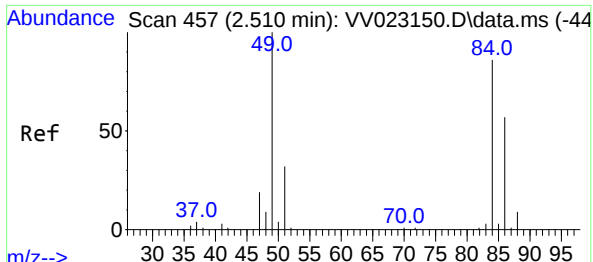

#16
Methylene chloride
Concen: 1.039 ug/L
RT: 2.510 min Scan# 4
Delta R.T. -0.000 min
Lab File: VV023169.D
Acq: 02 Nov 2021 23:48

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

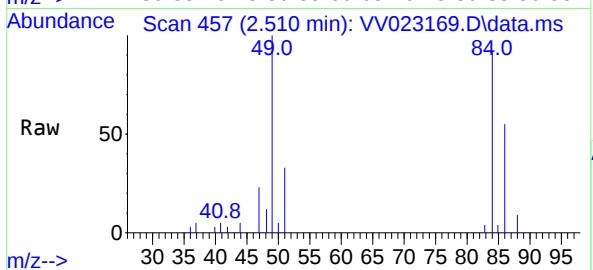

Tgt Ion: 84 Resp: 7084

Ion	Ratio	Lower	Upper
84	100		
86	60.0	42.3	78.5
49	108.7	79.7	148.1

