

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110221\
 Data File : VW023172.D
 Acq On : 03 Nov 2021 00:58
 Operator : SY/MD
 Sample : M4445-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG380

Quant Time: Nov 03 01:53:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Nov 02 23:31:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	120628	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	122820	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58191	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	42686	4.050	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	81.000%	
7) Chloroethane-d5	1.568	69	35723	5.479	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	109.600%	
11) 1,1-Dichloroethene-d2	2.111	63	58348	3.837	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	76.800%	
20) 2-Butanone-d5	3.889	46	81842	48.402	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	96.800%	
24) Chloroform-d	4.352	84	86685	5.059	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.200%	
26) 1,2-Dichloroethane-d4	5.034	65	40841	5.056	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.200%	
32) Benzene-d6	5.053	84	166899	4.655	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.000%	
36) 1,2-Dichloropropane-d6	6.072	67	50206	4.548	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	91.000%	
41) Toluene-d8	7.317	98	145156	4.507	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.200%	
43) trans-1,3-Dichloroprop...	7.625	79	17582	4.546	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	91.000%	
46) 2-Hexanone-d5	8.088	63	63721	44.501	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	89.000%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	33396	4.382	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	87.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	55337	5.330	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	106.600%	
Target Compounds						Qvalue
13) Acetone	2.175	43	2502	3.016	ug/L	94
42) Toluene	7.400	91	5232	0.156	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
Data File : VV023172.D
Acq On : 03 Nov 2021 00:58
Operator : SY/MD
Sample : M4445-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG380

Quant Time: Nov 03 01:53:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Nov 02 23:31:16 2021
Response via : Initial Calibration

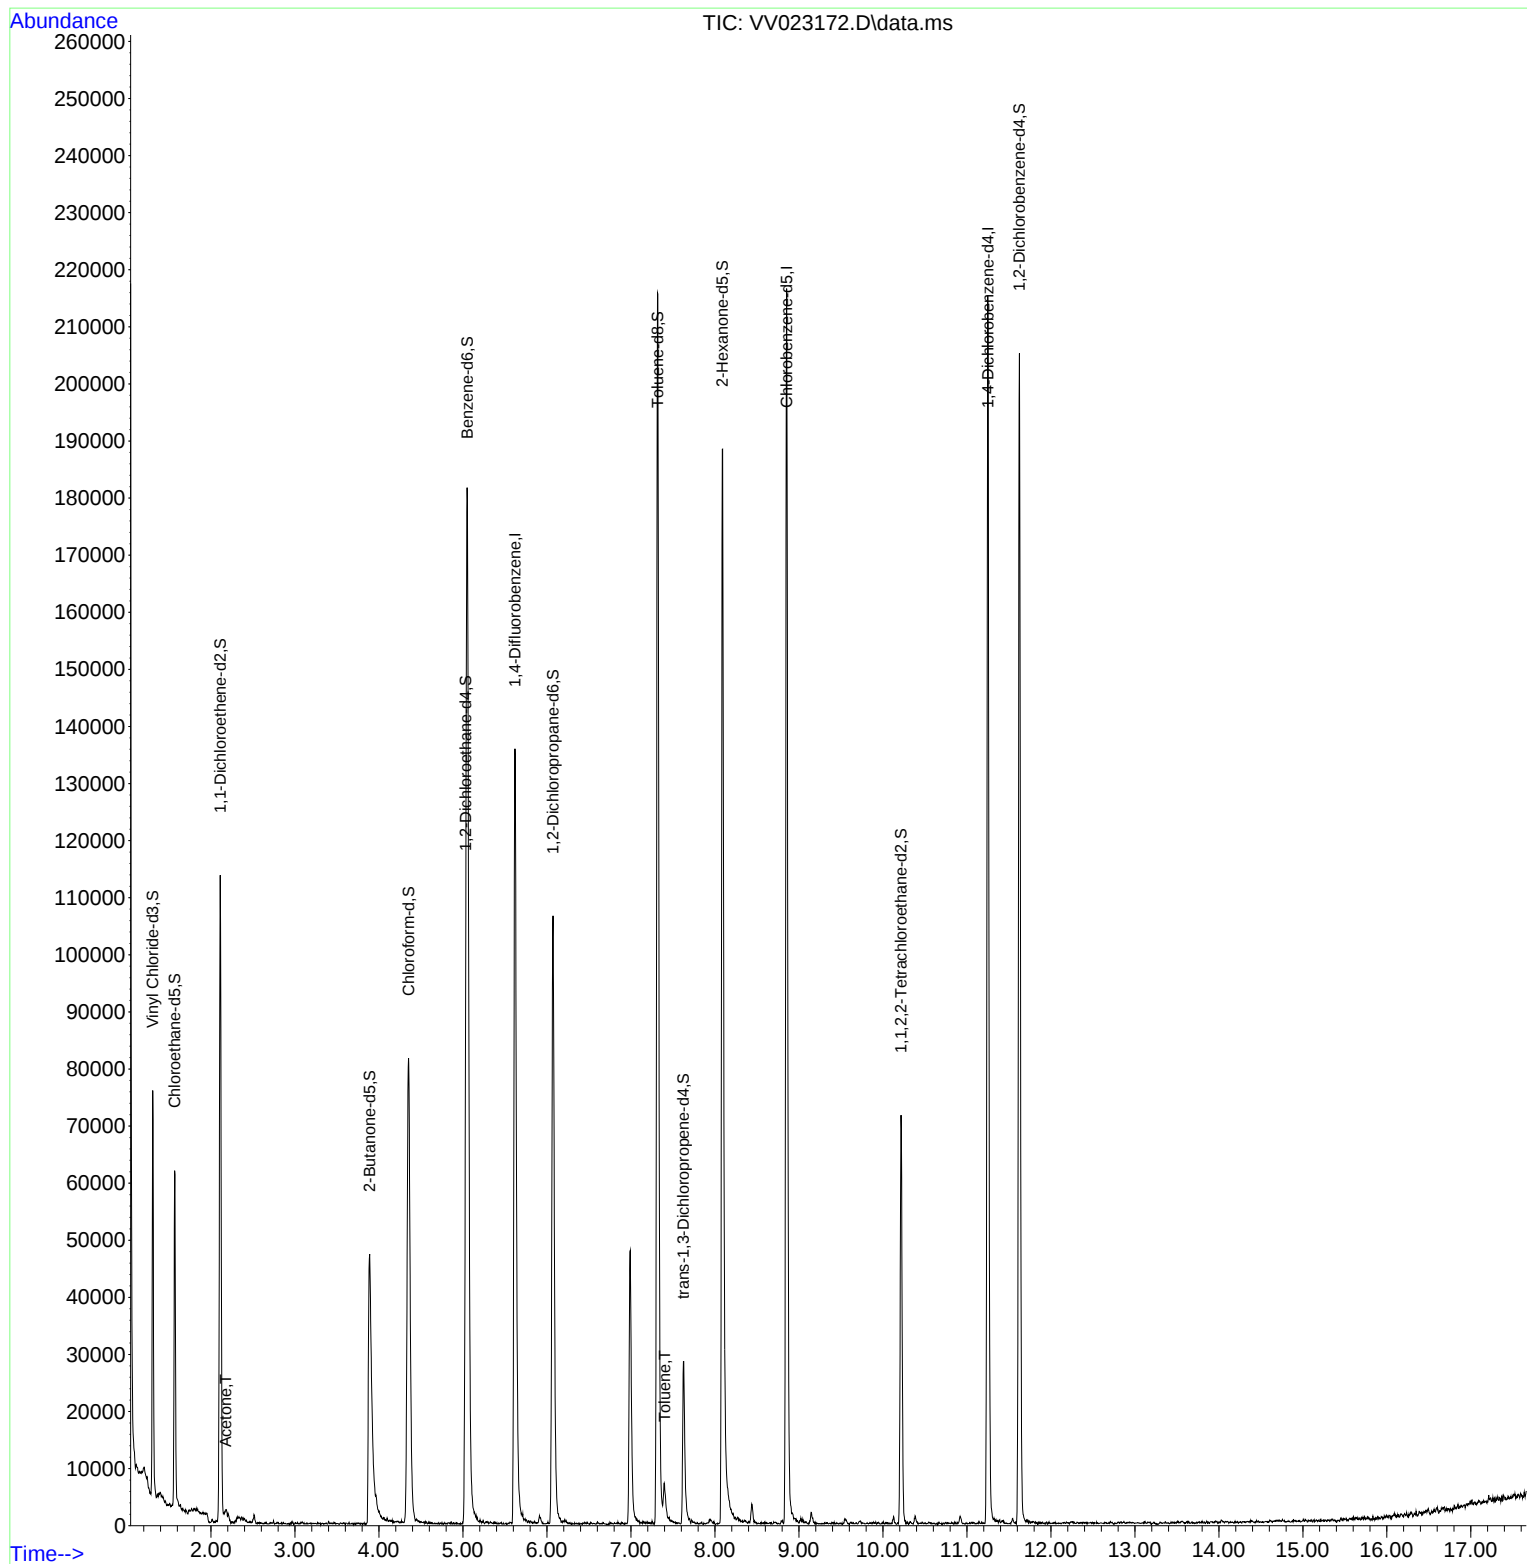

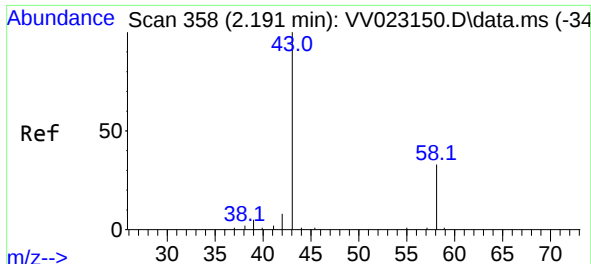

#13

Acetone

Concen: 3.016 ug/L

RT: 2.175 min Scan# 31

Delta R.T. -0.016 min

Lab File: VV023172.D

Acq: 03 Nov 2021 00:58

Instrument :

MSVOA_V

ClientSampleId :





BG380

Tgt Ion: 43 Resp: 2502

Ion Ratio Lower Upper

43 100

58 31.1 0.0 55.4

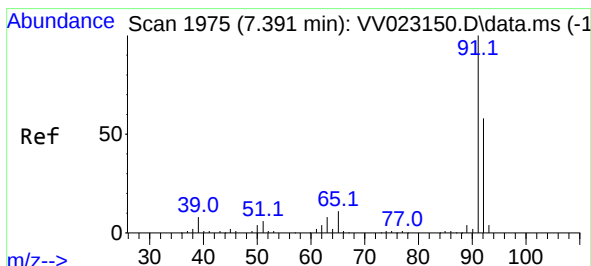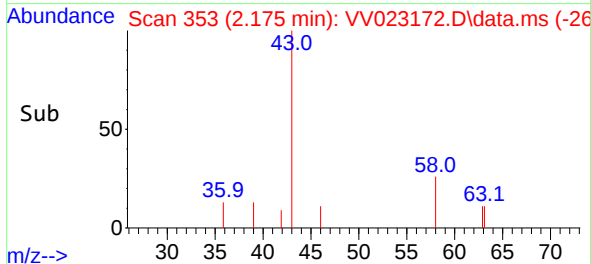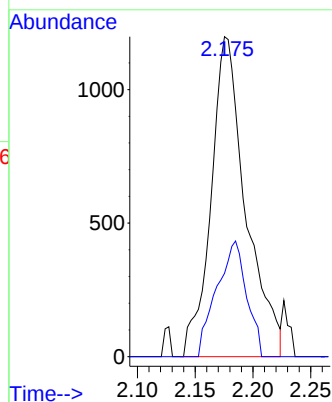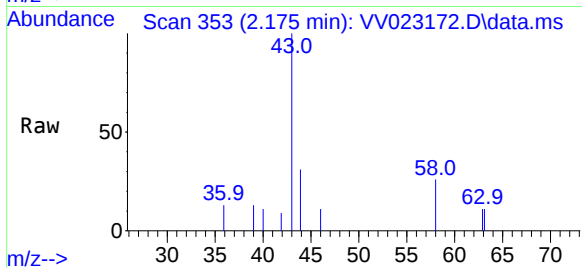

#42

Toluene

Concen: 0.156 ug/L

RT: 7.400 min Scan# 1978

Delta R.T. 0.010 min

Lab File: VV023172.D

Acq: 03 Nov 2021 00:58

Tgt Ion: 91 Resp: 5232

Ion Ratio Lower Upper

91 100

92 64.1 39.3 72.9

