

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
 Data File : VV023143.D
 Acq On : 02 Nov 2021 13:12
 Operator : SY/MD
 Sample : M4400-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG348

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	79551	79803	16.45%	2.051%
2	1.568	157	164	177	rBV	64368	70217	14.47%	1.805%
3	2.111	322	333	345	rBV	125446	184470	38.02%	4.741%
4	2.179	346	354	362	rVB3	2823	5205	1.07%	0.134%
5	2.333	383	402	424	rBV2	12108	57181	11.78%	1.470%
6	3.889	870	886	920	rBV2	56805	173721	35.80%	4.465%
7	4.352	1014	1030	1057	rBV	86723	217848	44.90%	5.599%
8	5.050	1228	1247	1279	rBV2	195244	485206	100.00%	12.470%
9	5.619	1412	1424	1448	rBV	139804	289746	59.72%	7.447%
10	6.072	1551	1565	1587	rBV	110260	228598	47.11%	5.875%
11	6.992	1840	1851	1873	rBV	51395	97817	20.16%	2.514%
12	7.320	1940	1953	1971	rBV	228725	406057	83.69%	10.436%
13	7.400	1972	1978	1990	rVB3	6005	11077	2.28%	0.285%
14	7.628	2036	2049	2066	rBV2	30847	56654	11.68%	1.456%
15	8.091	2182	2193	2225	rBV	201888	357742	73.73%	9.194%
16	8.854	2419	2430	2452	rBV	223649	367009	75.64%	9.432%
17	10.217	2844	2854	2872	rBV	70879	115894	23.89%	2.979%
18	11.249	3164	3175	3194	rBV	220051	341195	70.32%	8.769%
19	11.535	3257	3264	3275	rBV6	3223	5022	1.04%	0.129%
20	11.625	3280	3292	3313	rBV	219411	340485	70.17%	8.751%




Sum of corrected areas: 3890947

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
Data File : VV023143.D
Acq On : 02 Nov 2021 13:12
Operator : SY/MD
Sample : M4400-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG348

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

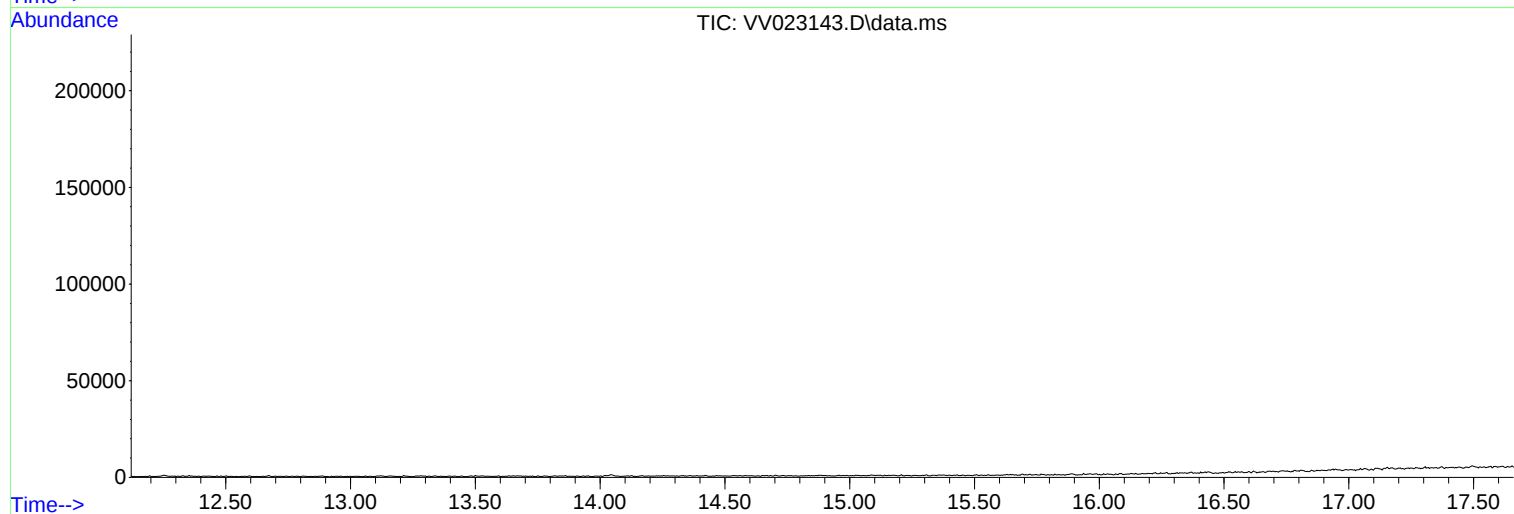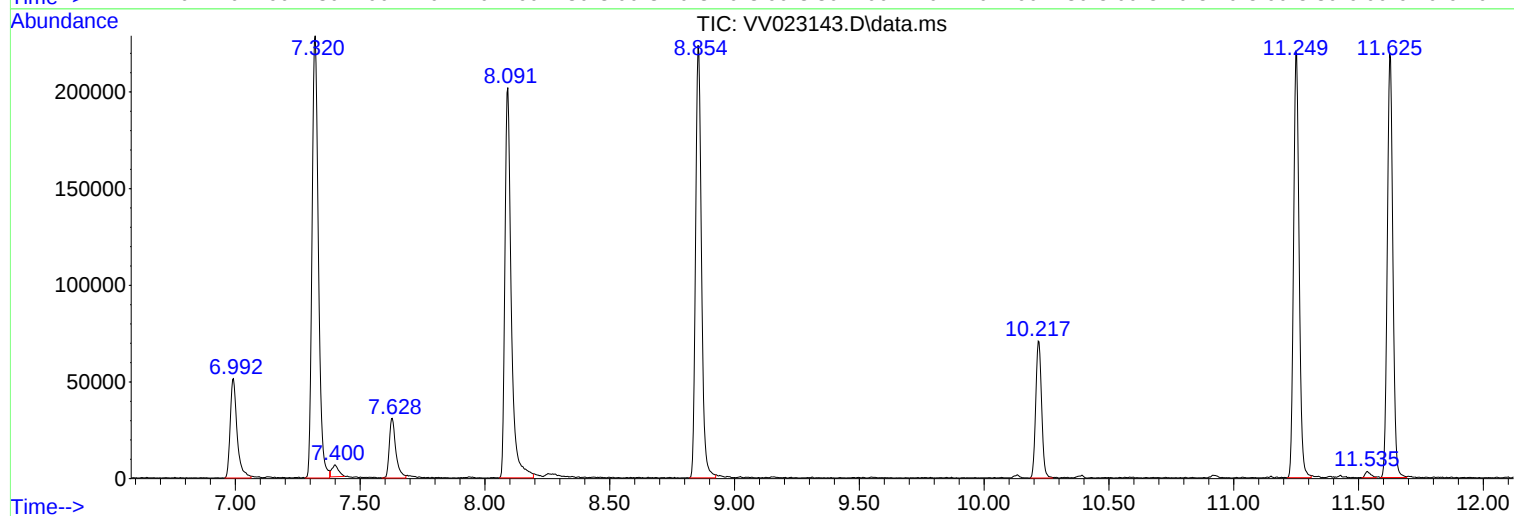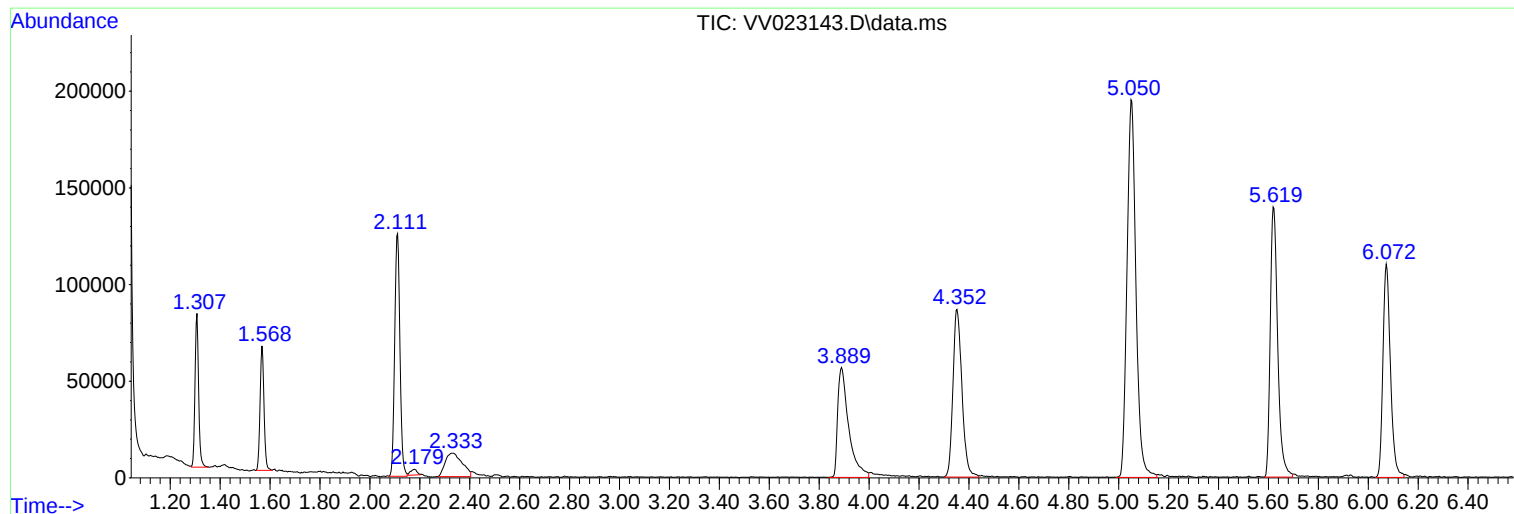

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
Data File : VV023143.D
Acq On : 02 Nov 2021 13:12
Operator : SY/MD
Sample : M4400-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG348










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.333	0.99 ug/L	57181	1,4-Difluorobenzene	5.622

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
3			4-Penten-2-ol	86	C5H10O	000625-31-0	9
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
5			Methane, nitroso-	45	CH3NO	000865-40-7	4

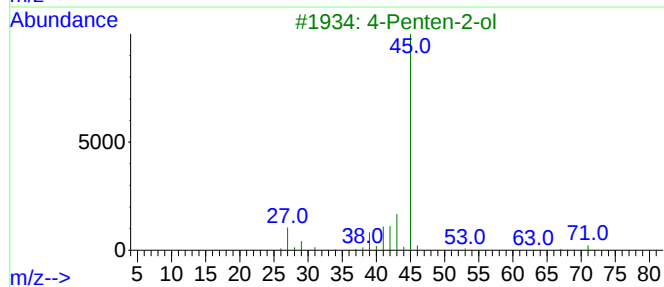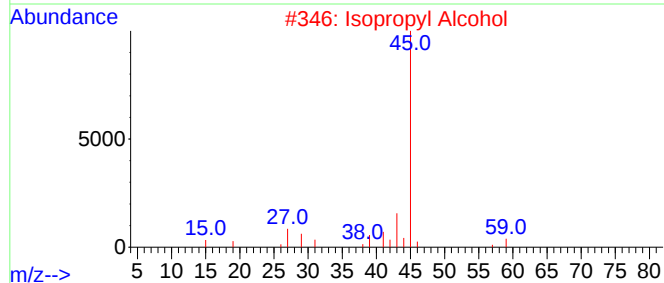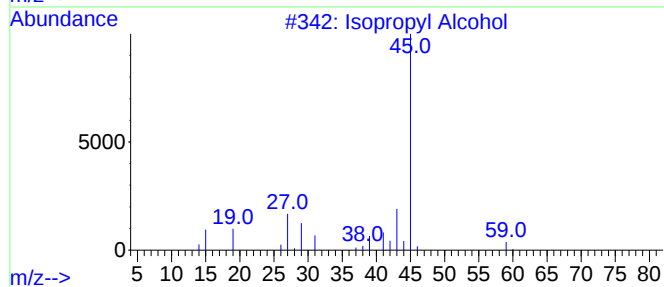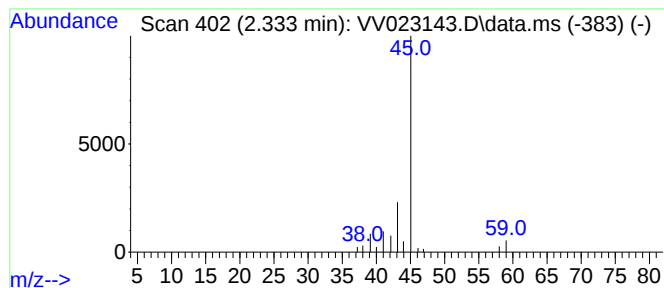

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
Data File : VV023143.D
Acq On : 02 Nov 2021 13:12
Operator : SY/MD
Sample : M4400-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG348

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.333	1.0	ug/L	57181	1	5.622	289746	5.0