
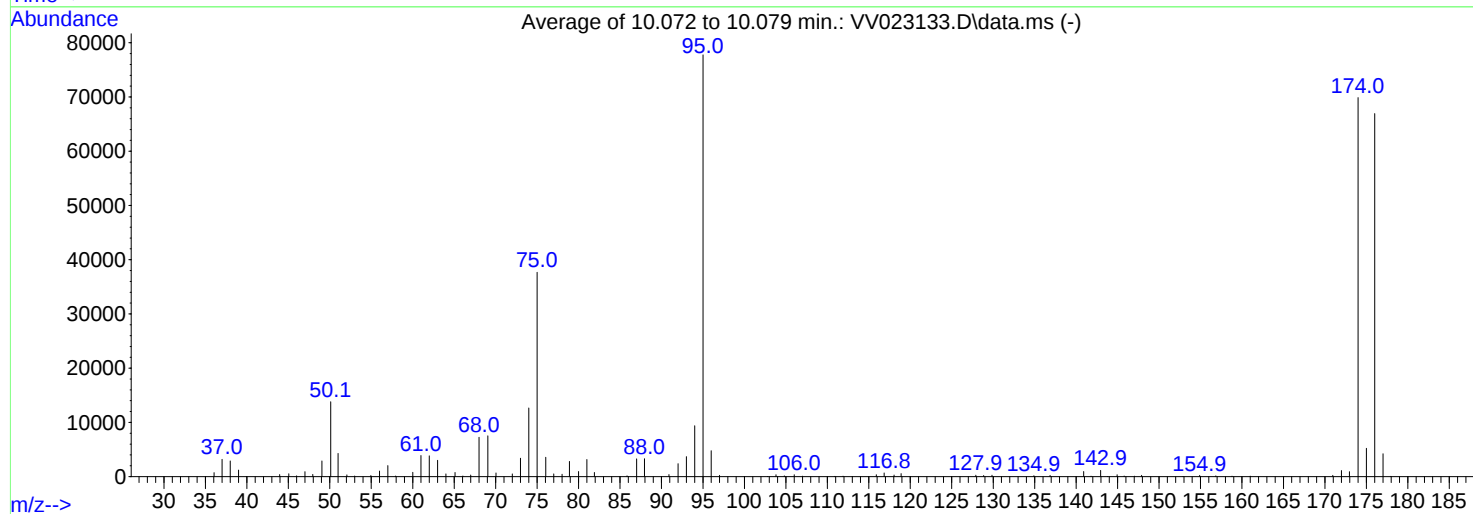


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
 Data File : VV023133.D
 Acq On : 02 Nov 2021 08:50
 Operator : SY/MD
 Sample : BFB225
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB225

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Nov 02 23:31:16 2021

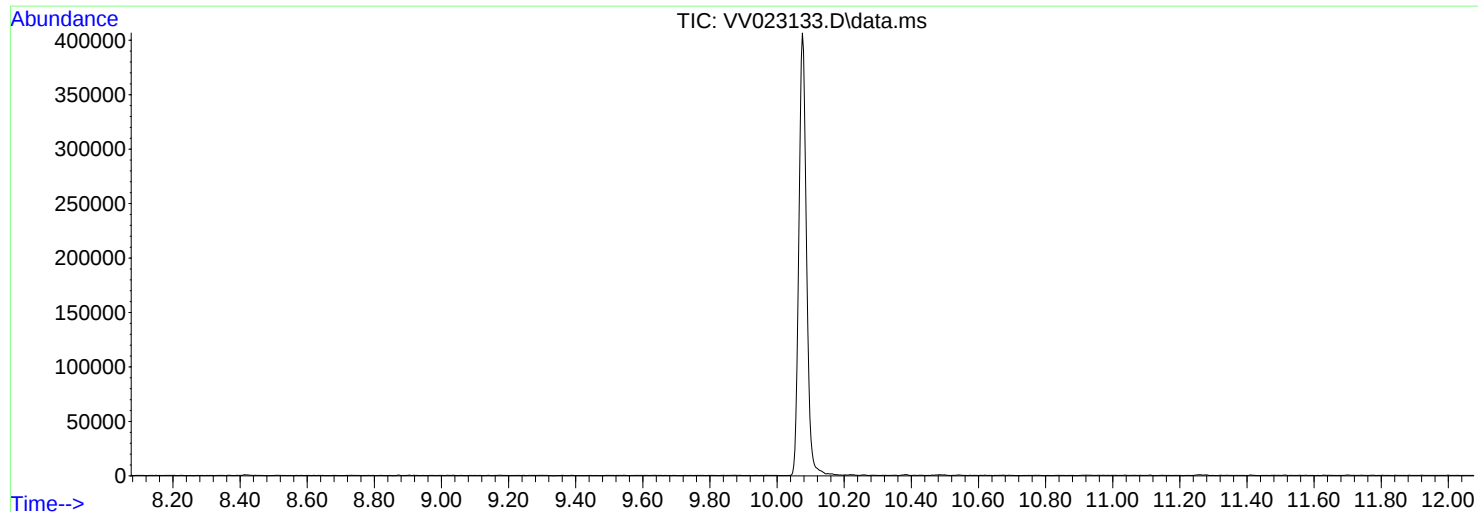

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	13806	PASS
75	95	30	80	48.5	37683	PASS
95	95	100	100	100.0	77773	PASS
96	95	5	9	6.1	4780	PASS
173	174	0.00	2	1.3	911	PASS
174	95	50	120	89.9	69880	PASS
175	174	5	9	7.5	5225	PASS
176	174	95	105	95.8	66947	PASS
177	176	5	10	6.3	4210	PASS

m/z	Abundance
40.00	168.0
44.00	250.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
36.00	785.0
37.00	3078.0
38.00	3045.0
39.00	1267.0
39.90	220.0
43.90	605.0
45.00	520.0
46.00	131.0
47.00	962.0
47.90	402.0
49.10	2942.0
50.10	13667.0
51.00	4475.0
52.10	292.0
53.00	118.0
54.90	193.0
56.00	1056.0
57.00	1977.0
58.00	121.0
60.00	807.0
61.00	3883.0
62.00	3762.0
63.00	3012.0
64.00	455.0
65.10	694.0
66.10	111.0
67.00	300.0
68.00	7118.0
69.10	7385.0
70.10	718.0
72.00	527.0
73.00	3394.0
74.00	12376.0
75.00	37224.0
76.00	3626.0
77.00	475.0
78.00	458.0
78.90	2759.0
80.00	1037.0
81.00	3188.0
81.90	704.0
85.90	138.0
87.00	3307.0
87.90	3062.0
90.90	437.0
92.00	2451.0
93.00	3496.0
94.00	9333.0
95.00	75368.0
96.00	4697.0
97.00	214.0
103.80	295.0
104.80	135.0
106.00	374.0
110.90	115.0
115.90	335.0
116.80	621.0
118.00	304.0
118.90	538.0
127.90	290.0
128.90	171.0
129.80	260.0
134.90	152.0
136.80	195.0
140.90	902.0
141.80	146.0
142.90	1158.0
144.90	348.0
145.80	135.0
147.90	262.0
154.90	220.0
156.80	164.0
171.00	243.0
172.00	1008.0
172.90	876.0
174.00	66848.0
175.00	5001.0
176.00	63960.0
177.00	4084.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
36.10	686.0
37.00	3232.0
38.00	2710.0
39.00	1117.0
40.00	176.0
44.00	649.0
45.10	524.0
46.00	147.0
47.00	869.0
48.00	429.0
49.00	2781.0
50.10	13401.0
51.00	3987.0
52.00	335.0
53.00	120.0
55.00	233.0
56.00	1015.0
57.00	2001.0
57.90	130.0
60.00	781.0
61.00	3745.0
62.00	3784.0
63.00	2922.0
64.00	542.0
65.10	822.0
66.00	139.0
67.00	286.0
68.00	7148.0
69.00	7446.0
70.00	638.0
72.00	473.0
73.00	3330.0
74.00	12527.0
75.00	36880.0
76.10	3329.0
77.00	491.0
78.00	418.0
78.90	2773.0
80.00	853.0
81.00	3028.0
81.90	814.0
85.90	157.0
87.00	3095.0
88.00	3405.0
90.90	327.0
92.00	2268.0
93.00	3741.0
94.00	9061.0
95.00	77296.0
96.00	4671.0
97.00	256.0
102.80	109.0
103.80	401.0
104.80	152.0
106.00	339.0
107.00	112.0
111.90	120.0
113.00	108.0
115.90	372.0
116.90	707.0
118.10	274.0
118.90	594.0
127.90	261.0
128.80	238.0
129.90	301.0
134.90	165.0
136.90	284.0
140.90	949.0
143.00	1149.0
143.80	117.0
144.90	335.0
145.80	140.0
147.10	161.0
147.90	224.0
152.90	111.0
154.90	235.0
156.90	157.0
158.80	131.0
161.00	132.0
170.90	206.0
172.00	1192.0
173.00	923.0
174.00	70440.0
175.00	5263.0
176.00	67664.0
177.00	4138.0
178.00	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225

m/z	Abundance
36.10	787.0
37.00	3253.0
38.00	2903.0
39.00	1276.0
39.90	189.0
44.00	647.0
45.10	568.0
46.00	156.0
47.00	943.0
48.00	459.0
49.10	2975.0
50.10	14350.0
51.00	4396.0
52.00	353.0
53.00	121.0
55.00	224.0
56.00	1055.0
57.00	2156.0
58.00	120.0
60.00	813.0
61.00	4027.0
62.00	3964.0
63.00	3104.0
64.00	528.0
65.10	763.0
66.10	125.0
67.00	303.0
68.00	7473.0
69.00	7781.0
70.10	721.0
72.00	536.0
73.00	3481.0
74.00	13066.0
75.00	38944.0
76.00	3728.0
77.00	509.0
78.00	443.0
78.90	2894.0
80.00	947.0
81.00	3289.0
81.90	796.0
85.80	151.0
87.00	3404.0
87.90	3449.0
90.90	416.0
92.00	2485.0
93.00	3814.0
94.00	9757.0
95.00	80656.0
96.00	4971.0
97.00	266.0
103.80	351.0
104.80	150.0
106.00	389.0
107.00	120.0
110.90	109.0
111.90	123.0
115.90	376.0
116.90	675.0
118.10	307.0
118.90	593.0
127.90	287.0
128.80	213.0
129.90	277.0
134.90	187.0
136.90	253.0
140.90	985.0
141.80	123.0
142.90	1184.0
145.00	352.0
145.80	122.0
147.00	116.0
147.90	268.0
154.90	255.0
156.90	168.0
158.80	106.0
161.00	114.0
171.00	242.0
172.00	1211.0
172.90	935.0
174.00	72352.0
175.00	5412.0
176.00	69216.0
177.00	4409.0
177.90	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB225