


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110221\
 Data File : VV023174.D
 Acq On : 03 Nov 2021 09:36
 Operator : SY/MD
 Sample : BFB226
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB226

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Nov 02 23:31:16 2021

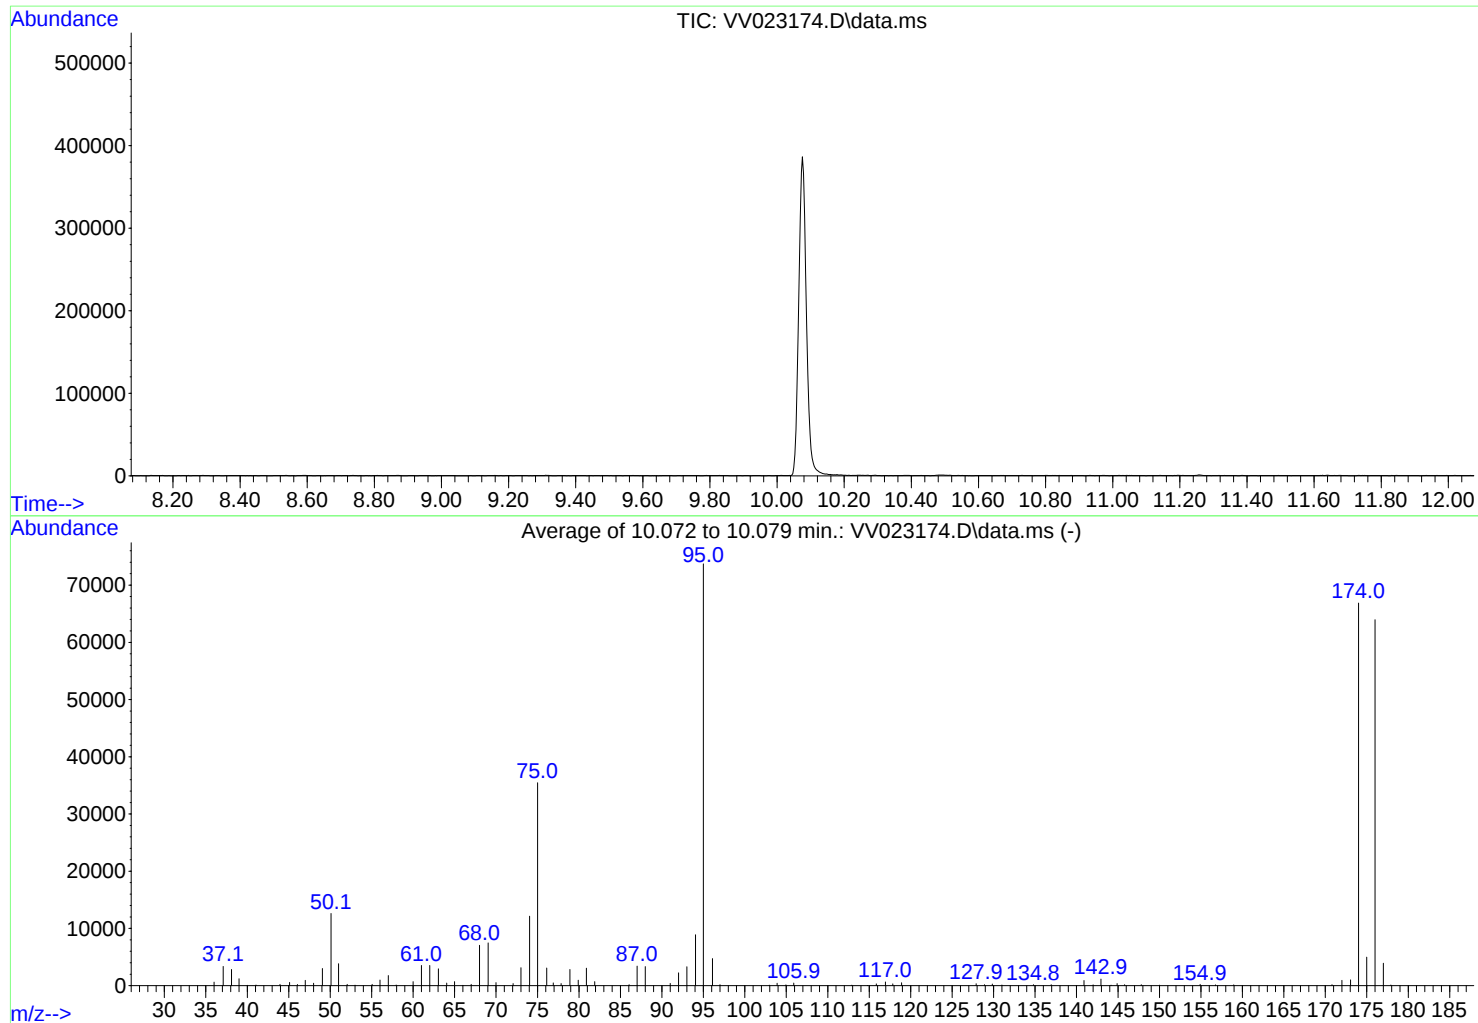

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	12626	PASS
75	95	30	80	48.1	35453	PASS
95	95	100	100	100.0	73725	PASS
96	95	5	9	6.4	4743	PASS
173	174	0.00	2	1.5	1003	PASS
174	95	50	120	90.7	66859	PASS
175	174	5	9	7.5	4984	PASS
176	174	95	105	95.7	63963	PASS
177	176	5	10	6.1	3926	PASS

m/z	Abundance
36.00	628.0
37.10	3482.0
38.10	2904.0
39.00	1269.0
40.00	254.0
41.10	146.0
44.00	565.0
45.10	594.0
46.00	200.0
47.00	953.0
48.00	423.0
49.00	3129.0
50.10	12988.0
51.00	3929.0
52.10	221.0
53.00	107.0
55.10	218.0
56.00	996.0
57.00	1823.0
58.00	122.0
60.00	727.0
61.00	3678.0
62.00	3631.0
63.10	3053.0
64.00	445.0
65.00	704.0
67.00	223.0
68.00	7248.0
69.10	7790.0
70.00	524.0
72.10	364.0
73.00	3240.0
74.00	12616.0
75.00	36680.0
76.10	3169.0
76.90	522.0
77.80	374.0
78.90	2919.0
79.90	988.0
80.90	3155.0
81.90	731.0
86.00	179.0
87.00	3592.0
88.00	3493.0
91.00	395.0
92.00	2345.0
93.00	3370.0
94.10	9184.0
95.00	75784.0
96.10	4921.0
97.00	183.0
102.90	102.0
103.90	433.0
105.00	136.0
105.90	445.0
112.90	121.0
115.90	330.0
117.00	685.0
117.80	296.0
118.90	531.0
127.90	367.0
128.90	168.0
129.80	298.0
131.00	128.0
134.80	179.0
137.00	172.0
140.90	917.0
142.00	156.0
142.90	1172.0
144.10	102.0
144.90	382.0
145.80	183.0
147.80	166.0
150.00	112.0
154.90	231.0
156.70	169.0
158.90	153.0
170.80	188.0
172.00	951.0
173.00	1026.0
174.00	69328.0
175.00	5148.0
176.00	66344.0
177.00	4044.0
177.90	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
40.00	170.0
43.80	176.0
44.20	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
36.00	692.0
37.10	3404.0
38.10	2849.0
39.00	1072.0
40.00	230.0
41.00	114.0
44.00	606.0
45.10	589.0
46.10	161.0
47.00	974.0
48.00	440.0
49.00	3027.0
50.10	12748.0
51.00	3740.0
52.00	206.0
53.00	112.0
55.00	228.0
56.00	1021.0
57.00	1727.0
57.90	116.0
60.00	737.0
61.00	3755.0
62.00	3451.0
63.00	3024.0
64.10	406.0
65.00	705.0
66.00	134.0
67.00	222.0
68.00	7042.0
69.10	7602.0
70.00	521.0
72.00	367.0
73.00	3104.0
74.10	11791.0
75.00	34944.0
76.10	3155.0
76.90	483.0
77.80	385.0
78.90	2797.0
79.90	905.0
80.90	2949.0
81.90	717.0
86.10	190.0
87.00	3421.0
88.00	3116.0
91.00	383.0
92.00	2191.0
93.00	3266.0
94.10	8795.0
95.00	73936.0
96.10	4927.0
97.00	178.0
103.00	113.0
103.90	356.0
104.90	149.0
105.90	449.0
115.80	320.0
116.90	654.0
117.90	293.0
118.90	549.0
127.90	298.0
128.90	158.0
129.90	269.0
131.00	152.0
134.80	178.0
137.00	212.0
140.90	811.0
142.00	108.0
143.00	1203.0
144.20	123.0
144.90	361.0
145.80	177.0
147.80	161.0
150.00	115.0
154.90	238.0
156.80	161.0
159.00	112.0
161.00	103.0
170.80	160.0
172.00	854.0
173.10	952.0
174.00	64480.0
175.00	5120.0
176.00	61208.0
177.00	3796.0
177.90	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
36.00	522.0
37.10	3221.0
38.10	2710.0
39.00	1291.0
40.00	216.0
41.10	115.0
44.00	517.0
45.10	504.0
46.00	195.0
47.00	843.0
48.00	398.0
49.10	2825.0
50.10	12142.0
51.00	3837.0
52.10	215.0
55.10	222.0
56.00	914.0
57.00	1758.0
58.00	132.0
60.00	607.0
61.00	3138.0
62.00	3489.0
63.10	2702.0
64.00	467.0
65.00	687.0
67.00	212.0
68.00	6898.0
69.00	7028.0
70.00	552.0
72.00	354.0
73.00	3091.0
74.00	12024.0
75.00	34736.0
76.10	2921.0
76.90	469.0
77.90	359.0
78.90	2760.0
79.90	976.0
80.90	3015.0
81.90	688.0
86.00	124.0
87.00	3258.0
88.00	3341.0
91.00	365.0
92.00	2178.0
93.00	3229.0
94.00	8671.0
95.00	71456.0
96.10	4380.0
97.00	137.0
103.90	447.0
105.00	108.0
105.90	425.0
112.90	142.0
114.80	106.0
115.90	284.0
117.00	633.0
117.80	324.0
118.90	470.0
127.90	353.0
128.90	184.0
129.80	296.0
131.00	102.0
134.80	161.0
136.80	151.0
140.90	939.0
142.00	172.0
142.90	1039.0
144.90	369.0
145.80	161.0
147.80	156.0
154.90	197.0
156.70	136.0
158.90	144.0
170.80	165.0
172.00	940.0
173.00	1032.0
174.00	66768.0
175.00	4684.0
176.00	64336.0
177.00	3938.0
177.90	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226