

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110222\
 Data File : VW028843.D
 Acq On : 02 Nov 2022 15:57
 Operator : SY/MD
 Sample : N5421-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 03 03:31:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 02 05:10:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	377317	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	349332	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	148811	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	132529	37.052	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	74.100%		
7) Chloroethane-d5	1.561	69	132388	43.297	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.600%		
11) 1,1-Dichloroethene-d2	2.243	63	305	0.045	ug/L	0.14
Spiked Amount 50.000	Range 60 - 125		Recovery =	0.080%#		
21) 2-Butanone-d5	3.873	46	269467	103.492	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	103.490%		
24) Chloroform-d	4.342	84	233391	43.263	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.520%		
26) 1,2-Dichloroethane-d4	5.027	65	168499	47.227	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.460%		
32) Benzene-d6	5.047	84	474523	43.513	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.020%		
36) 1,2-Dichloropropane-d6	6.063	67	171553	45.821	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.640%		
41) Toluene-d8	7.310	98	394160	41.114	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.220%		
43) trans-1,3-Dichloroprop...	7.619	79	58143	40.435	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.860%		
47) 2-Hexanone-d5	8.085	63	161477	95.439	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	95.440%		
56) 1,1,2,2-Tetrachloroeth...	10.207	84	228109	46.204	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.400%		
66) 1,2-Dichlorobenzene-d4	11.615	152	134516	45.794	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.580%		
Target Compounds					Qvalue	
27) 1,2-Dichloroethane	5.043	62	3292	0.732	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028843.D
Acq On : 02 Nov 2022 15:57
Operator : SY/MD
Sample : N5421-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Nov 03 03:31:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 02 05:10:28 2022
Response via : Initial Calibration

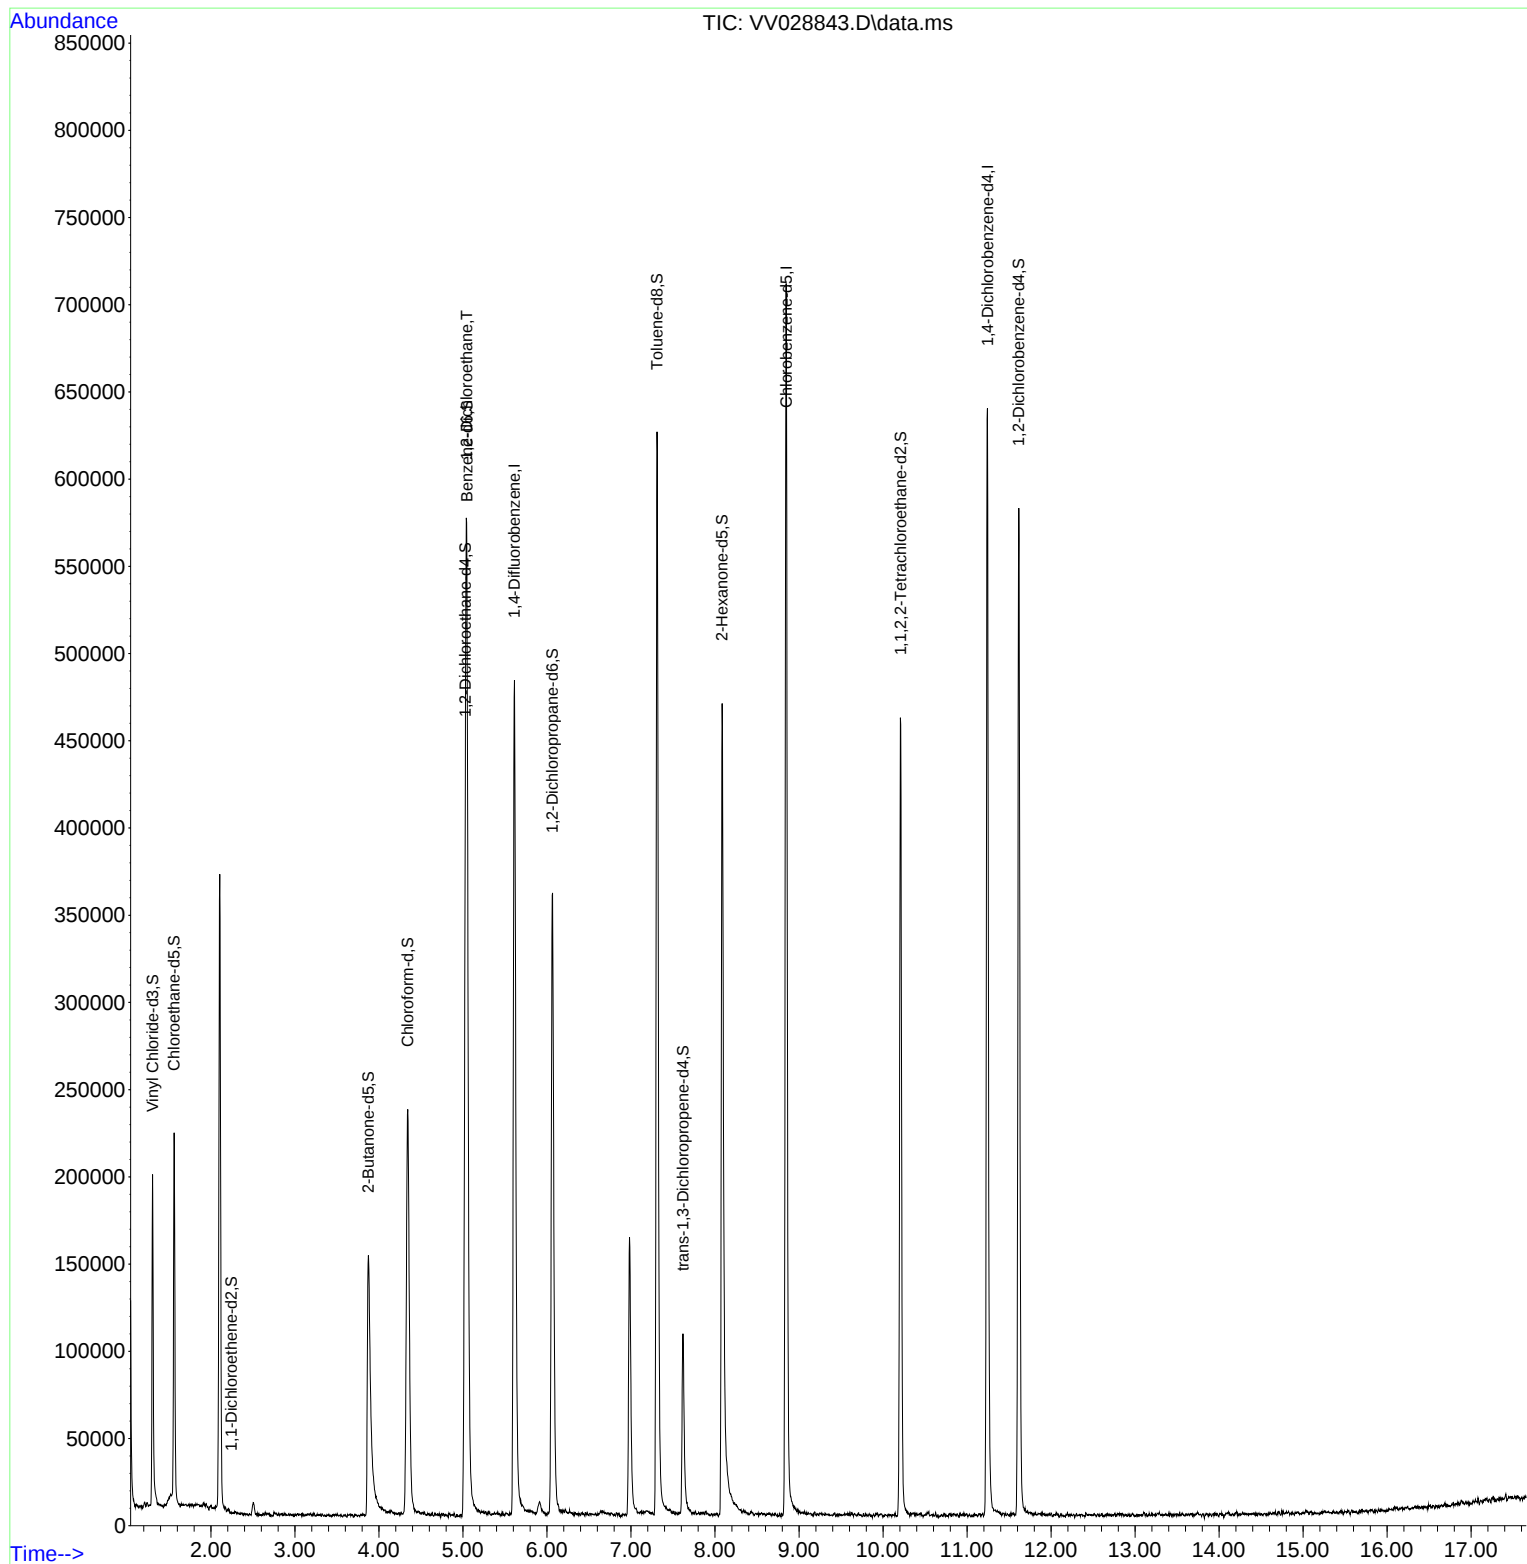

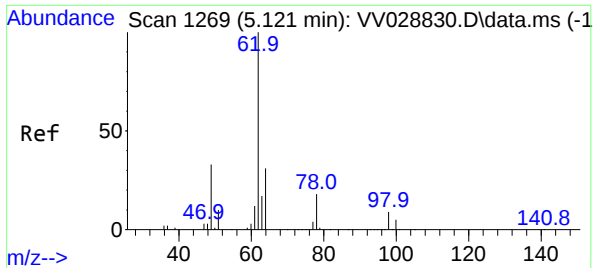

#27
1,2-Dichloroethane
Concen: 0.732 ug/L
RT: 5.043 min Scan# 11
Delta R.T. -0.077 min
Lab File: VV028843.D
Acq: 02 Nov 2022 15:57

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 62 Resp: 3292
Ion Ratio Lower Upper
62 100
98 7.8 6.9 10.3

