

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110222\
 Data File : VW028841.D
 Acq On : 02 Nov 2022 15:08
 Operator : SY/MD
 Sample : N5421-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1118

Quant Time: Nov 03 03:30:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 02 05:10:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	386295	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	349142	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	147153	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	144640	39.498	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.000%
7) Chloroethane-d5	1.561	69	133826	42.750	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.500%
11) 1,1-Dichloroethene-d2	2.105	63	213433	30.640	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	61.280%
21) 2-Butanone-d5	3.873	46	244972	91.898	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.900%
24) Chloroform-d	4.342	84	239968	43.448	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.900%
26) 1,2-Dichloroethane-d4	5.027	65	170240	46.606	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.220%
32) Benzene-d6	5.043	84	489478	44.909	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.820%
36) 1,2-Dichloropropane-d6	6.066	67	176320	47.120	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.240%
41) Toluene-d8	7.310	98	403397	42.100	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.200%
43) trans-1,3-Dichloroprop...	7.619	79	58012	40.365	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.740%
47) 2-Hexanone-d5	8.085	63	148008	87.526	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	87.530%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	226687	45.941	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.880%
66) 1,2-Dichlorobenzene-d4	11.615	152	135568	46.672	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.340%
Target Compounds						
13) Acetone	2.166	43	11611	4.499	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028841.D
Acq On : 02 Nov 2022 15:08
Operator : SY/MD
Sample : N5421-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1118

Quant Time: Nov 03 03:30:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 02 05:10:28 2022
Response via : Initial Calibration

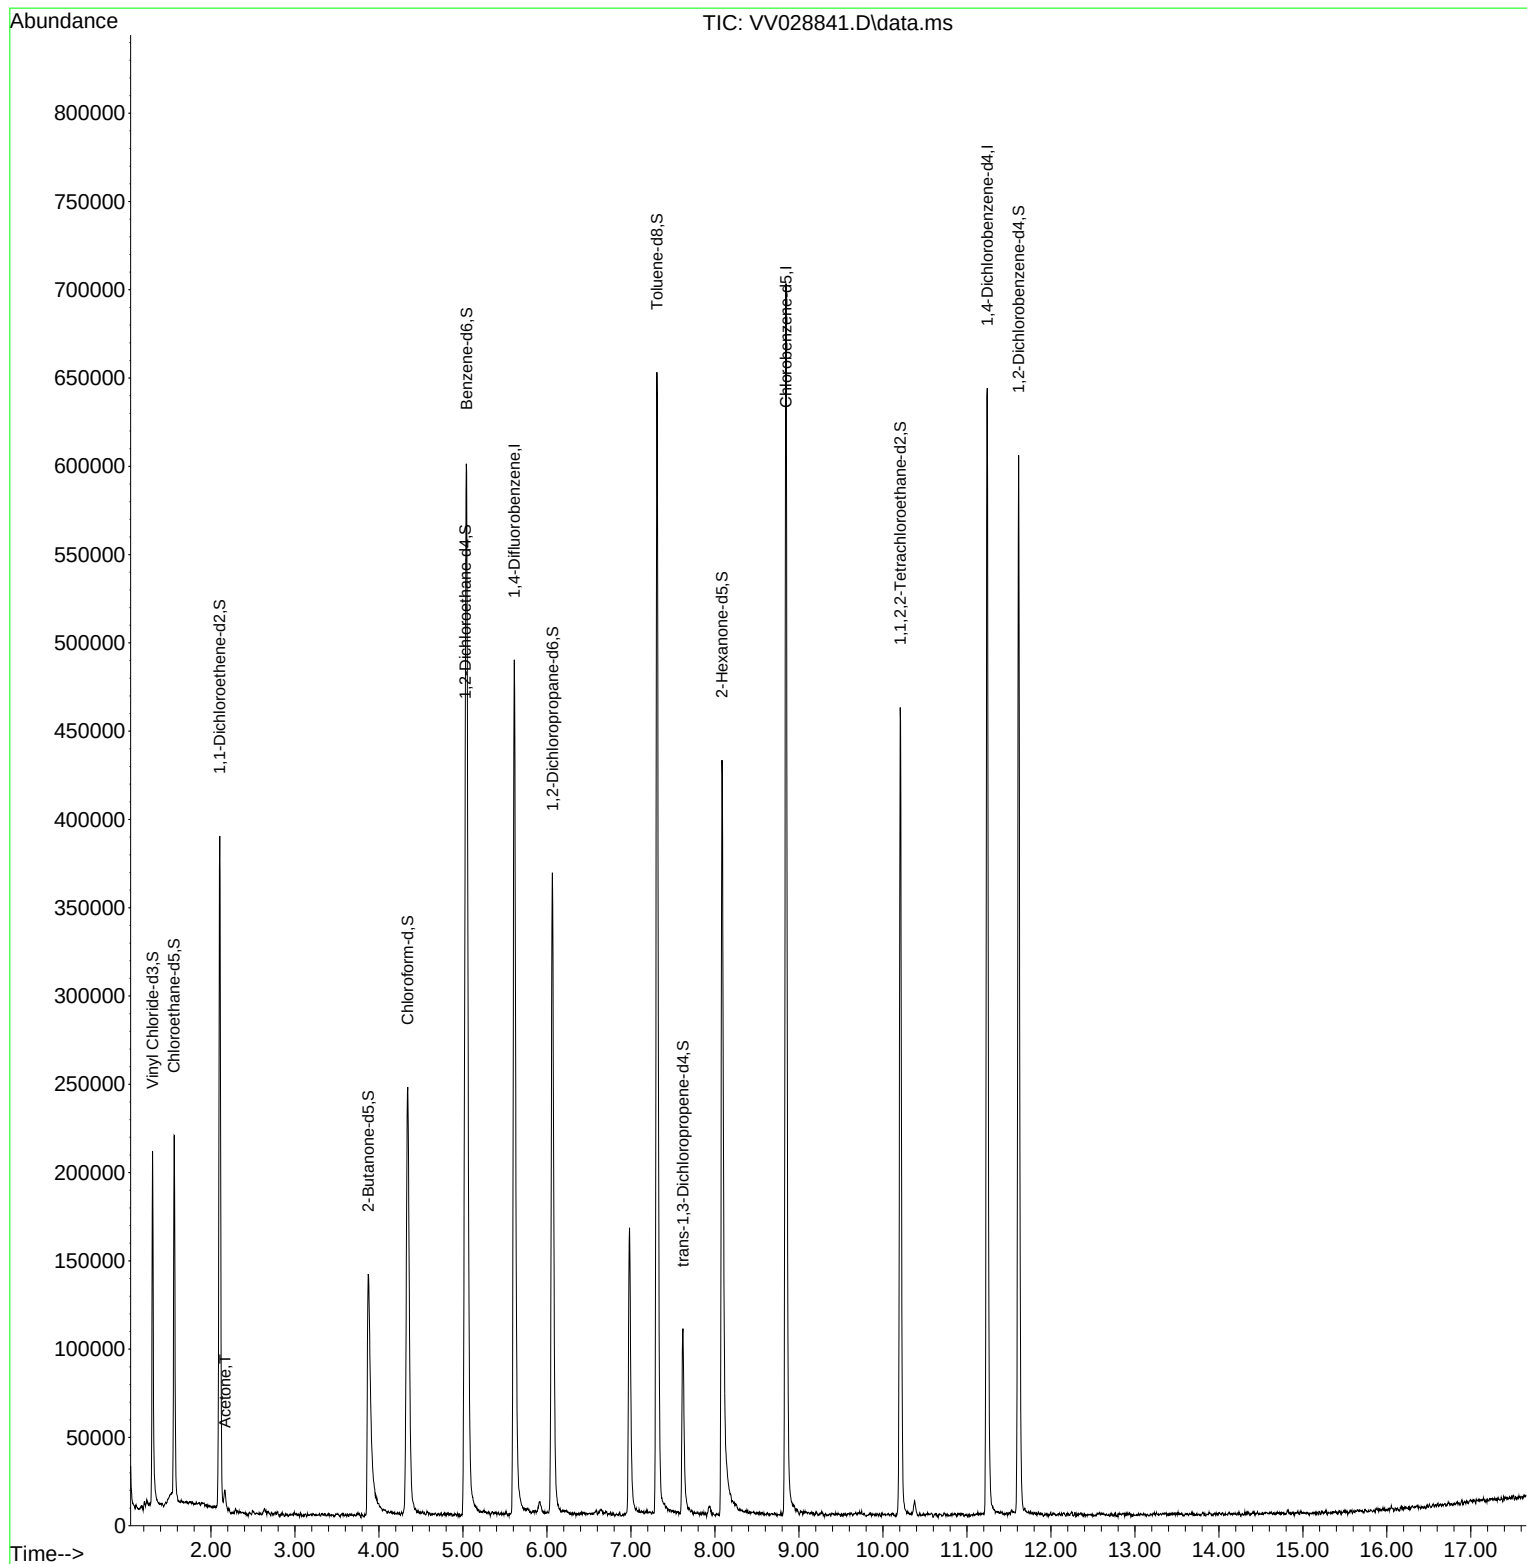

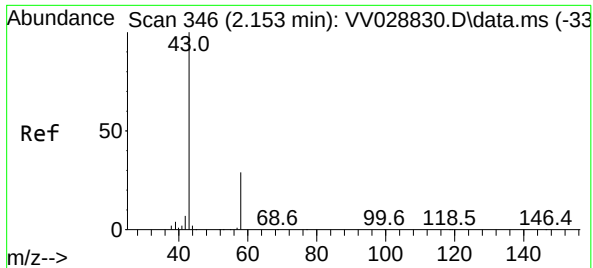

#13
 Acetone
 Concen: 4.499 ug/L
 RT: 2.166 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VV028841.D
 Acq: 02 Nov 2022 15:08

Instrument :
 MSVOA_V
 ClientSampleId :
 C1118

Tgt Ion: 43 Resp: 11611
 Ion Ratio Lower Upper
 43 100
 58 33.3 0.0 59.0

