

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028834.D
 Acq On : 02 Nov 2022 12:19
 Operator : SY/MD
 Sample : N5353-11 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVV1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028834.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rBV	222651	251660	10.18%	1.513%
2	1.564	157	163	179	rVB	240717	276261	11.17%	1.661%
3	2.105	322	331	347	rVB	430155	616087	24.92%	3.704%
4	2.355	407	409	413	rBV3	1917	1358	0.05%	0.008%
5	2.452	436	439	443	rBV5	1886	1731	0.07%	0.010%
6	2.642	496	498	503	rVB5	1339	753	0.03%	0.005%
7	2.687	510	512	516	rBV5	1719	1111	0.04%	0.007%
8	2.757	526	534	551	rVB	54543	96675	3.91%	0.581%
9	3.140	645	653	656	rBV10	2242	2584	0.10%	0.016%
10	3.410	734	737	740	rBV5	2305	1361	0.06%	0.008%
11	3.455	749	751	755	rBV4	1032	862	0.03%	0.005%
12	3.484	758	760	764	rVB5	1505	865	0.03%	0.005%
13	3.516	767	770	771	rBV3	1395	652	0.03%	0.004%
14	3.532	772	775	778	rVB4	1256	777	0.03%	0.005%
15	3.751	841	843	849	rVB6	1957	1300	0.05%	0.008%
16	3.780	849	852	854	rBV4	1056	617	0.02%	0.004%
17	3.902	873	890	921	rBV2	921493	2472431	100.00%	14.863%
18	4.342	1013	1027	1056	rVB	259053	639759	25.88%	3.846%
19	4.748	1150	1153	1156	rVB5	1858	1178	0.05%	0.007%
20	4.767	1156	1159	1163	rBV5	1757	1457	0.06%	0.009%
21	4.918	1202	1206	1208	rBV4	1749	1635	0.07%	0.010%
22	4.960	1218	1219	1223	rBV4	1112	730	0.03%	0.004%
23	5.040	1228	1244	1276	rBV2	651812	1713541	69.31%	10.301%
24	5.461	1371	1375	1378	rVB6	1852	1408	0.06%	0.008%
25	5.551	1399	1403	1408	rBV7	1809	1799	0.07%	0.011%
26	5.612	1408	1422	1452	rBV	535034	1091812	44.16%	6.563%
27	5.908	1502	1514	1537	rBV	793047	1546377	62.54%	9.296%
28	6.066	1551	1563	1583	rBV	394577	794720	32.14%	4.777%
29	6.612	1731	1733	1734	rBV2	1386	596	0.02%	0.004%
30	6.802	1789	1792	1795	rBV4	1481	1010	0.04%	0.006%
31	6.854	1805	1808	1810	rBV4	1195	659	0.03%	0.004%
32	6.911	1821	1826	1831	rBV9	2390	3163	0.13%	0.019%
33	6.982	1837	1848	1864	rBV	181559	337744	13.66%	2.030%
34	7.310	1939	1950	1978	rBV	712384	1254753	50.75%	7.543%
35	7.619	2036	2046	2066	rBV	119760	216042	8.74%	1.299%
36	7.911	2134	2137	2139	rBV4	1713	1077	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028834.D
 Acq On : 02 Nov 2022 12:19
 Operator : SY/MD
 Sample : N5353-11 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVV1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	8.085	2181	2191	2228	rBV	478681	994378	40.22%	5.978%
38	8.632	2355	2361	2363	rBV5	1650	1483	0.06%	0.009%
39	8.741	2393	2395	2397	rBV3	1474	840	0.03%	0.005%
40	8.789	2409	2410	2414	rBV4	893	611	0.02%	0.004%
41	8.847	2414	2428	2450	rBV	761203	1284795	51.96%	7.724%
42	9.320	2572	2575	2578	rBV4	1956	1318	0.05%	0.008%
43	9.390	2593	2597	2601	rBV6	1206	1229	0.05%	0.007%
44	9.718	2697	2699	2704	rBV6	2332	2439	0.10%	0.015%
45	9.757	2709	2711	2714	rVB4	1717	881	0.04%	0.005%
46	9.779	2714	2718	2723	rBV7	1793	1761	0.07%	0.011%
47	9.805	2723	2726	2730	rBV6	1390	1136	0.05%	0.007%
48	9.870	2743	2746	2749	rBV5	1202	702	0.03%	0.004%
49	9.892	2749	2753	2754	rBV4	992	648	0.03%	0.004%
50	10.008	2785	2789	2791	rBV4	1460	919	0.04%	0.006%
51	10.030	2794	2796	2799	rBV4	2057	1208	0.05%	0.007%
52	10.043	2799	2800	2802	rBV2	1511	789	0.03%	0.005%
53	10.075	2808	2810	2814	rBV5	1391	1034	0.04%	0.006%
54	10.207	2840	2851	2870	rBV	499632	799571	32.34%	4.807%
55	10.374	2899	2903	2906	rBV6	2811	2679	0.11%	0.016%
56	10.419	2913	2917	2920	rBV6	1091	802	0.03%	0.005%
57	10.435	2920	2922	2924	rBV3	1369	883	0.04%	0.005%
58	10.480	2933	2936	2939	rBV5	1412	998	0.04%	0.006%
59	10.574	2961	2965	2966	rBV4	1516	1025	0.04%	0.006%
60	10.651	2987	2989	2991	rBV3	1341	594	0.02%	0.004%
61	10.664	2991	2993	2997	rVV6	1561	639	0.03%	0.004%
62	10.837	3044	3047	3049	rBV4	1628	1131	0.05%	0.007%
63	10.956	3082	3084	3087	rBV4	1128	917	0.04%	0.006%
64	10.972	3087	3089	3092	rVV4	1332	584	0.02%	0.004%
65	11.066	3116	3118	3121	rVB4	2246	1101	0.04%	0.007%
66	11.239	3162	3172	3192	rBV	686392	1115277	45.11%	6.705%
67	11.432	3230	3232	3239	rBV8	1762	1779	0.07%	0.011%
68	11.615	3278	3289	3308	rBV	644555	1038886	42.02%	6.245%
69	11.953	3390	3394	3397	rBV6	2244	1592	0.06%	0.010%
70	12.021	3412	3415	3417	rBV4	1308	962	0.04%	0.006%
71	12.053	3422	3425	3426	rBV3	1117	736	0.03%	0.004%
72	12.159	3456	3458	3460	rBV3	1688	790	0.03%	0.005%
73	12.339	3513	3514	3518	rVB4	1193	782	0.03%	0.005%
74	12.371	3521	3524	3526	rBV4	1403	1101	0.04%	0.007%
75	12.500	3561	3564	3566	rBV4	1459	806	0.03%	0.005%
76	12.622	3600	3602	3604	rBV3	1298	655	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
 Data File : VV028834.D
 Acq On : 02 Nov 2022 12:19
 Operator : SY/MD
 Sample : N5353-11 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVV1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.641	3604	3608	3615	rVV9	2137	2696	0.11%	0.016%
78	12.686	3620	3622	3625	rBV4	1274	1064	0.04%	0.006%
79	12.747	3639	3641	3644	rVB4	1325	617	0.02%	0.004%
80	12.850	3670	3673	3676	rBV4	1606	979	0.04%	0.006%
81	12.918	3689	3694	3703	rBV9	2017	2653	0.11%	0.016%
82	12.953	3703	3705	3708	rBV3	911	609	0.02%	0.004%
83	13.075	3741	3743	3747	rVB5	1683	812	0.03%	0.005%
84	13.207	3782	3784	3786	rBV4	1708	824	0.03%	0.005%
85	13.387	3837	3840	3842	rBV4	1408	790	0.03%	0.005%
86	13.426	3848	3852	3853	rBV3	1460	992	0.04%	0.006%
87	13.487	3869	3871	3873	rBV3	1098	644	0.03%	0.004%
88	13.593	3900	3904	3906	rBV5	1469	1251	0.05%	0.008%
89	13.651	3920	3922	3924	rBV3	1750	1117	0.05%	0.007%
90	13.709	3938	3940	3943	rVB5	2577	1286	0.05%	0.008%
91	13.728	3943	3946	3949	rBV4	2208	1999	0.08%	0.012%
92	13.850	3981	3984	3986	rBV3	1873	1149	0.05%	0.007%
93	13.940	4010	4012	4014	rBV3	1486	811	0.03%	0.005%
94	13.998	4027	4030	4031	rBV3	1621	786	0.03%	0.005%
95	14.120	4066	4068	4069	rBV2	1485	586	0.02%	0.004%
96	14.239	4102	4105	4108	rVB4	887	648	0.03%	0.004%
97	14.265	4111	4113	4114	rBV2	1565	693	0.03%	0.004%
98	14.365	4141	4144	4147	rBV3	1761	1307	0.05%	0.008%
99	14.705	4248	4250	4255	rBV5	2589	1817	0.07%	0.011%
100	15.255	4419	4421	4428	rVB8	2623	1583	0.06%	0.010%




Sum of corrected areas: 16634719

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028834.D
Acq On : 02 Nov 2022 12:19
Operator : SY/MD
Sample : N5353-11 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWV1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

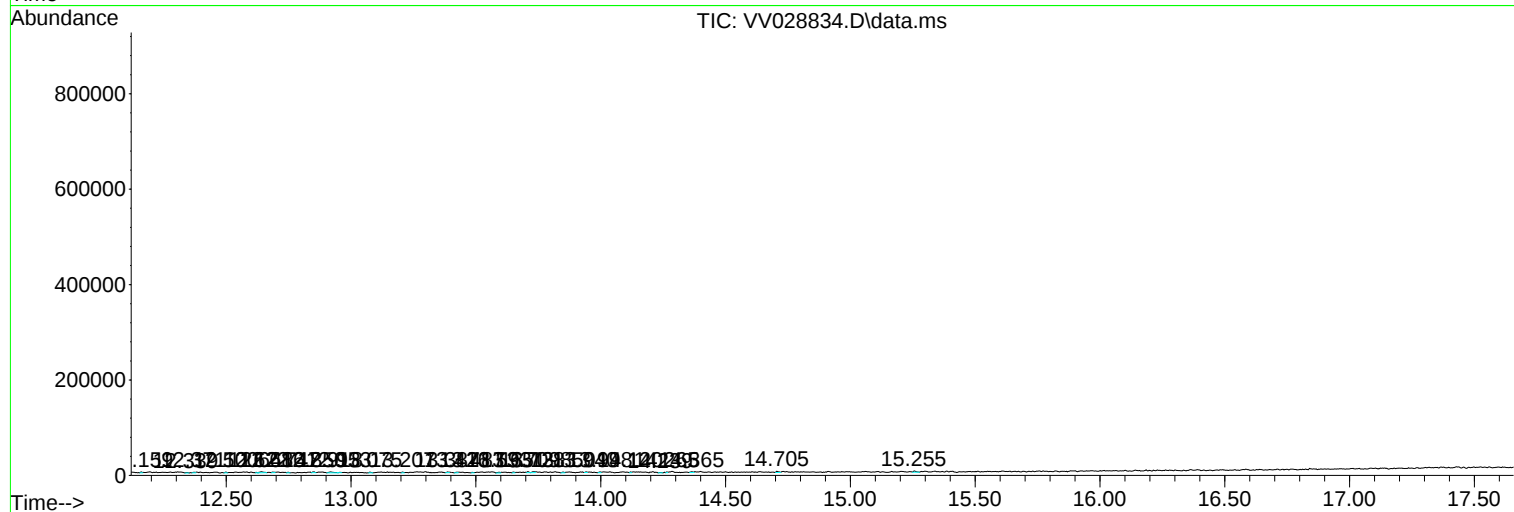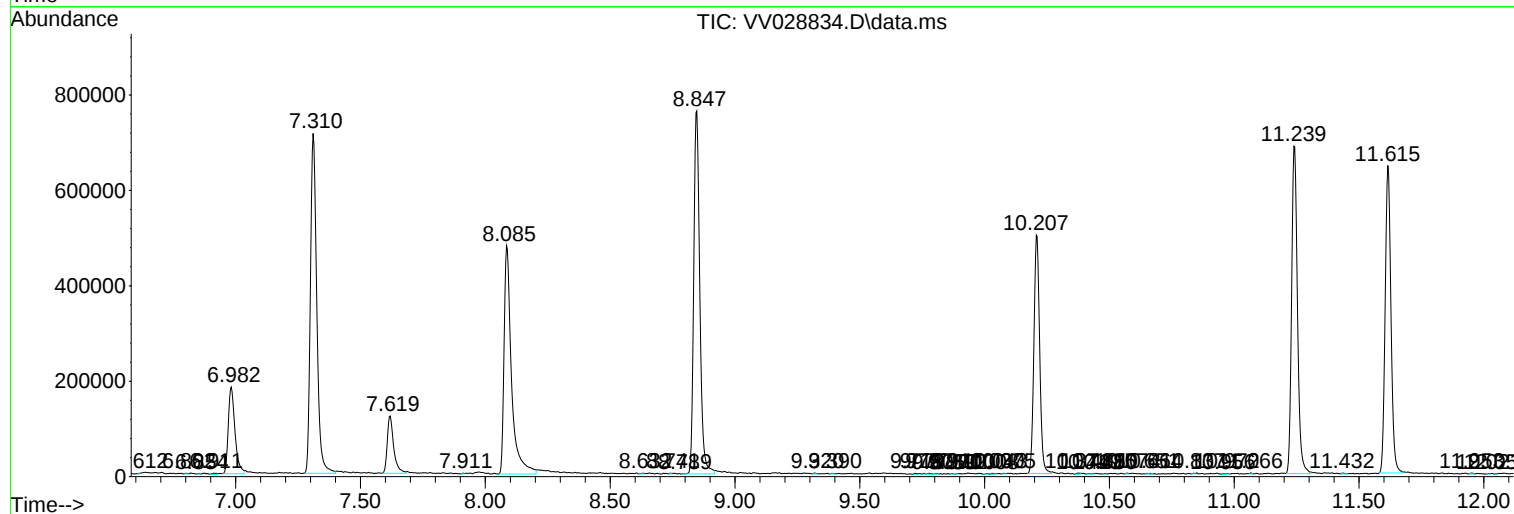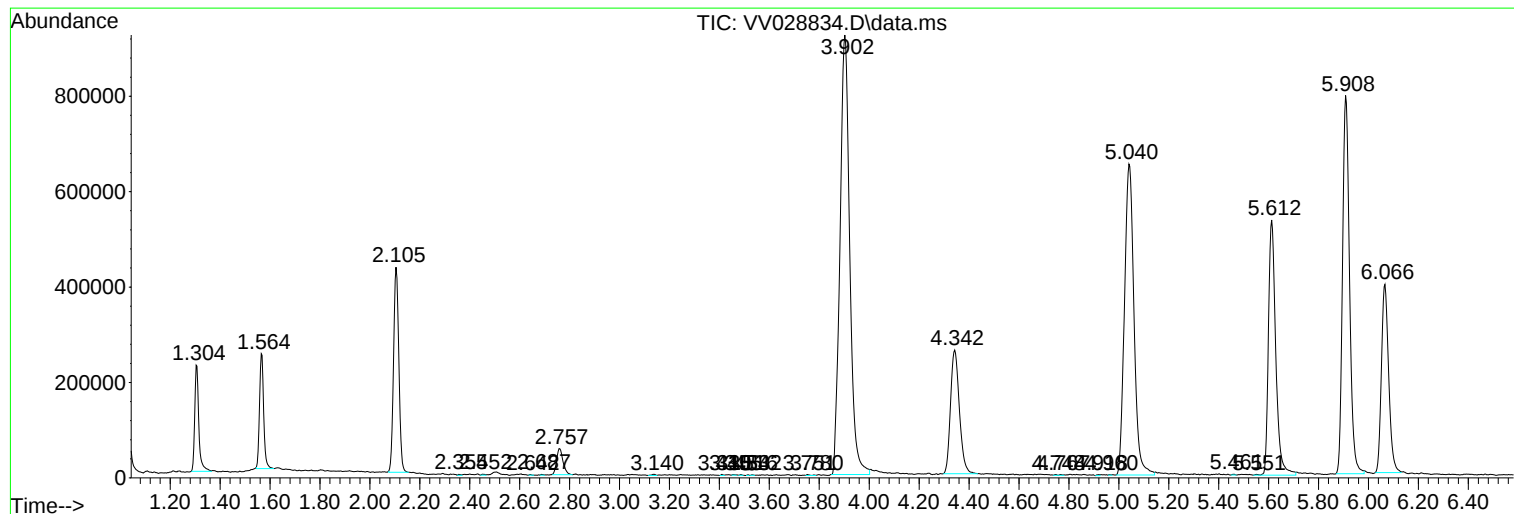

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028834.D
Acq On : 02 Nov 2022 12:19
Operator : SY/MD
Sample : N5353-11 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVV1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110222\
Data File : VV028834.D
Acq On : 02 Nov 2022 12:19
Operator : SY/MD
Sample : N5353-11 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBWV1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------